
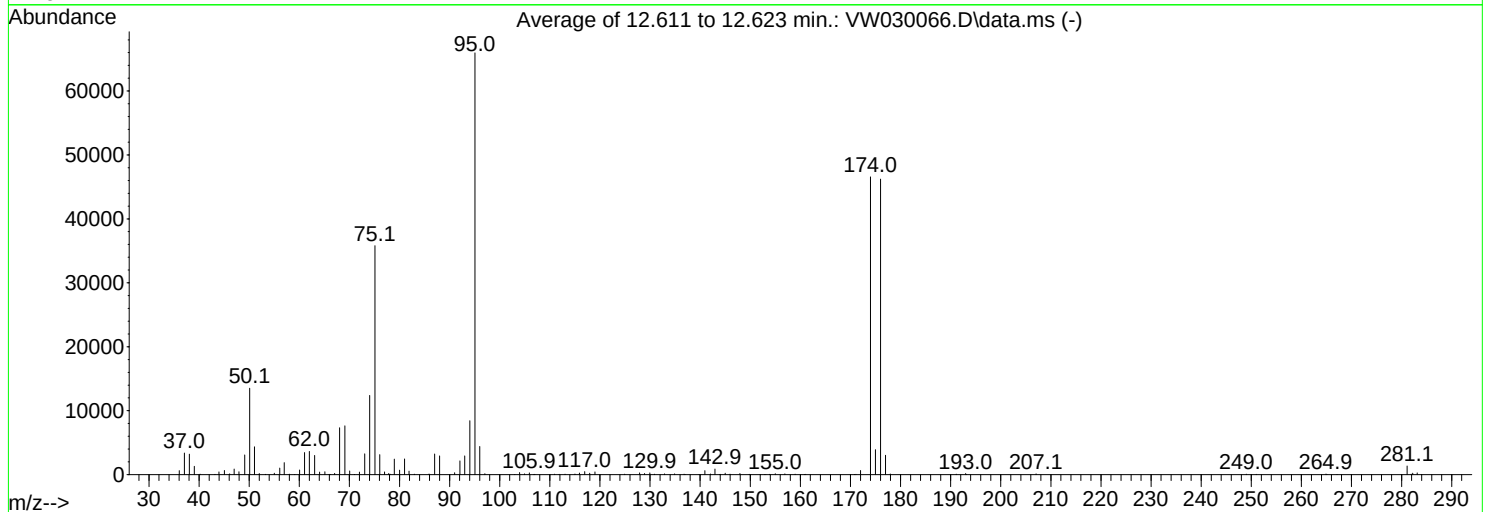


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082824\
Data File : VW030066.D
Acq On : 28 Aug 2024 08:49
Operator : SY/MD
Sample : BFB553
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB553

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
Title : SFAM01.0
Last Update : Fri Aug 30 23:54:36 2024

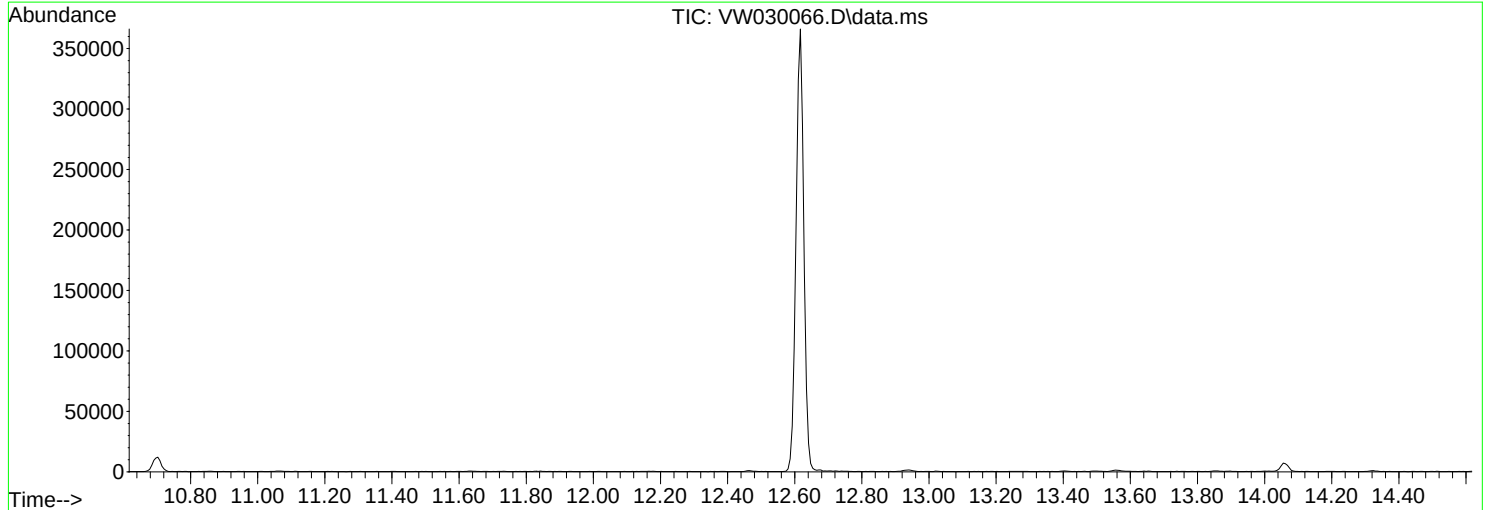

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1752

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	13516	PASS
75	95	30	80	54.3	35808	PASS
95	95	100	100	100.0	65968	PASS
96	95	5	9	6.7	4398	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	70.6	46571	PASS
175	174	5	9	8.4	3896	PASS
176	174	95	101	99.2	46208	PASS
177	176	5	9	6.6	3043	PASS

m/z	Abundance
40.00	150.0
43.80	132.0
57.00	54.0
72.80	59.0

Instrument :
MSVOA_W
ClientSampleId :
BFB553

m/z	Abundance
36.00	648.0
37.10	3711.0
38.10	3437.0
39.10	1370.0
40.00	268.0
44.00	535.0
45.10	676.0
46.20	153.0
47.00	957.0
48.00	425.0
49.10	3083.0
50.10	14188.0
51.10	4829.0
52.00	209.0
53.20	54.0
55.00	206.0
56.10	1108.0
57.10	2089.0
57.90	79.0
59.10	62.0
60.00	771.0
61.00	3638.0
62.00	3809.0
63.10	3169.0
64.00	466.0
65.10	479.0
66.00	72.0
67.00	171.0
68.00	7654.0
69.10	7804.0
70.00	654.0
71.00	64.0
72.00	452.0
73.00	3408.0
74.00	12476.0
75.10	37728.0
76.10	3223.0
77.00	423.0
77.90	280.0
79.00	2459.0
80.00	649.0
81.00	2404.0
81.90	575.0
83.00	53.0
85.90	116.0
87.00	3255.0
88.00	2786.0
91.00	301.0
92.10	1983.0
93.00	2834.0
94.00	8667.0
95.10	66144.0
96.00	4878.0
97.10	160.0
103.00	105.0
103.90	355.0
104.90	149.0
105.90	255.0
106.80	69.0
110.90	52.0
113.00	78.0
115.00	98.0
115.90	263.0
116.90	532.0
117.90	255.0
119.00	447.0
125.00	86.0
128.00	240.0
129.00	252.0
129.90	201.0
130.90	75.0
132.90	219.0
134.90	172.0
136.90	91.0
141.00	546.0
142.10	90.0
143.00	806.0
143.90	57.0
145.00	337.0
146.00	93.0
147.90	131.0
152.00	62.0
153.90	76.0
155.00	178.0
156.90	89.0
159.00	56.0
161.00	68.0
170.00	56.0
170.80	80.0
172.00	743.0
174.00	42976.0
175.00	3644.0

Instrument :
MSVOA_W
ClientSampleId :
BFB553

176.00	40632.0
177.00	2849.0
178.00	82.0
191.10	140.0
193.00	248.0
207.10	213.0
249.00	195.0
250.00	64.0
251.00	128.0
264.90	196.0
267.10	52.0
281.10	2137.0
282.20	540.0
283.10	368.0
284.00	54.0

Instrument :
MSVOA_W
ClientSampleId :
BFB553

m/z	Abundance
36.00	724.0
37.00	3485.0
38.10	3633.0
39.00	1529.0
40.20	197.0
43.10	91.0
44.00	663.0
45.00	744.0
46.00	165.0
47.00	1001.0
47.90	499.0
49.10	3378.0
50.10	15311.0
51.10	4620.0
52.10	202.0
53.30	80.0
54.90	246.0
56.10	1117.0
57.00	2105.0
58.00	92.0
60.10	837.0
61.00	3776.0
62.00	4176.0
63.00	3299.0
64.10	461.0
65.10	445.0
65.90	57.0
66.20	53.0
67.00	213.0
68.00	8466.0
69.10	8921.0
70.10	609.0
71.00	51.0
72.00	413.0
73.00	3684.0
74.10	13895.0
75.10	39392.0
76.10	3682.0
77.00	497.0
77.80	241.0
78.90	2857.0
80.00	922.0
81.00	2674.0
81.90	588.0
83.00	102.0
85.90	118.0
87.00	3535.0
88.00	3131.0
91.00	279.0
92.00	2799.0
93.00	3201.0
94.10	9404.0
95.00	72048.0
96.00	4700.0
97.10	168.0
104.00	351.0
105.00	100.0
105.80	349.0
107.00	82.0
110.00	51.0
111.00	88.0
111.90	68.0
113.10	91.0
115.00	120.0
115.90	301.0
117.00	532.0
117.90	251.0
119.00	480.0
124.90	115.0
127.80	317.0
128.80	106.0
130.00	378.0
130.90	141.0
132.90	184.0
135.00	114.0
136.70	121.0
139.80	59.0
141.00	700.0
142.00	157.0
143.00	999.0
144.10	68.0
145.00	262.0
145.90	111.0
147.90	195.0
149.80	69.0
152.90	69.0
153.80	58.0
155.10	137.0
156.80	125.0
158.90	109.0
161.10	87.0
171.10	163.0

Instrument :
MSVOA_W
ClientSampleId :
BFB553

172.00	762.0
174.00	56392.0
175.00	4163.0
176.00	51392.0
177.00	3527.0
177.90	114.0
191.10	88.0
193.00	245.0
207.00	75.0
249.00	71.0
264.90	127.0
281.10	1354.0
281.90	229.0
283.10	330.0

Instrument :
MSVOA_W
ClientSampleId :
BFB553

m/z	Abundance
36.10	510.0
37.10	2977.0
38.00	2569.0
39.10	1018.0
40.00	140.0
43.20	74.0
44.00	460.0
45.10	527.0
46.10	54.0
47.00	686.0
47.90	425.0
49.10	2769.0
50.10	11050.0
51.00	3642.0
51.90	138.0
55.10	231.0
56.10	846.0
57.00	1579.0
58.10	94.0
60.00	584.0
61.10	2918.0
62.00	2914.0
63.00	2529.0
64.10	318.0
65.10	439.0
67.10	214.0
68.10	5867.0
69.10	6166.0
70.00	461.0
72.00	377.0
73.10	2674.0
74.10	10776.0
75.10	30304.0
76.00	2463.0
77.00	380.0
78.10	236.0
79.00	1985.0
80.00	519.0
81.00	2304.0
81.90	491.0
82.90	98.0
85.90	74.0
87.00	2872.0
88.00	2895.0
91.00	316.0
92.00	1689.0
93.00	2784.0
94.10	7228.0
95.00	59712.0
96.00	3616.0
97.00	136.0
104.00	274.0
105.00	143.0
106.00	258.0
107.00	61.0
111.00	60.0
111.80	97.0
113.10	77.0
115.00	58.0
116.00	158.0
117.00	372.0
118.00	189.0
119.00	320.0
127.90	246.0
128.80	143.0
129.90	286.0
131.00	57.0
134.80	127.0
137.00	109.0
139.80	57.0
140.90	637.0
142.10	59.0
142.90	842.0
144.00	56.0
144.90	111.0
146.00	60.0
148.00	166.0
149.80	56.0
153.10	59.0
154.90	121.0
157.00	141.0
158.90	76.0
160.80	63.0
172.00	463.0
174.00	40344.0
175.00	3881.0
176.00	46600.0
177.00	2753.0
177.90	84.0
193.20	65.0
207.00	62.0
265.10	68.0

Instrument :
MSVOA_W
ClientSampleId :
BFB553

281.10	586.0
282.20	120.0
283.00	114.0

Instrument :
MSVOA_W
ClientSampleId :
BFB553