
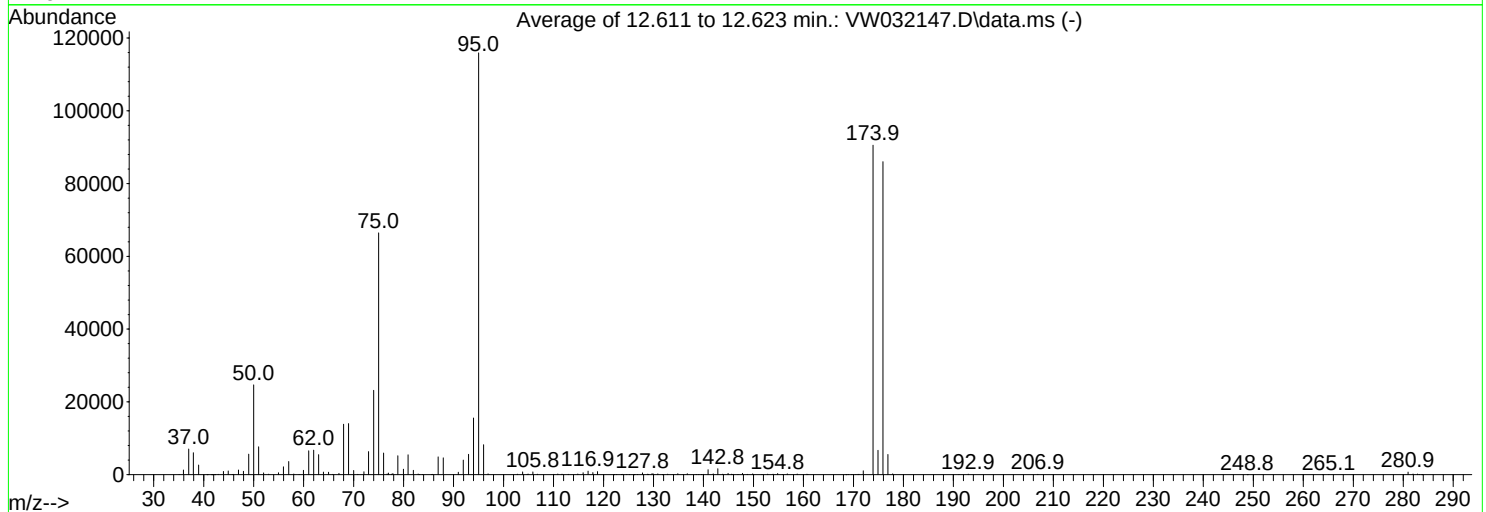


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082825\
Data File : VW032147.D
Acq On : 28 Aug 2025 08:57
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5mL/MSVOA_W/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W082625S.M
Title : SW846 8260
Last Update : Wed Aug 27 04:13:40 2025

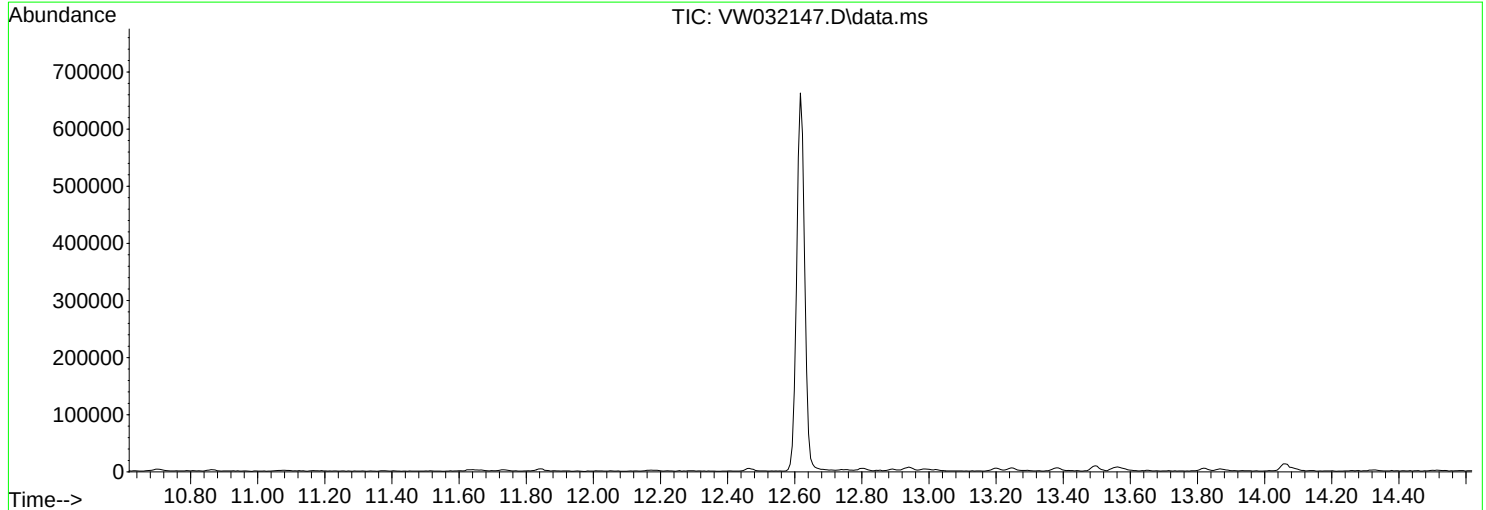

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	24656	PASS
75	95	30	60	57.3	66469	PASS
95	95	100	100	100.0	115933	PASS
96	95	5	9	7.1	8232	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	78.1	90536	PASS
175	174	5	9	7.4	6706	PASS
176	174	95	101	95.0	86024	PASS
177	176	5	9	6.4	5540	PASS