
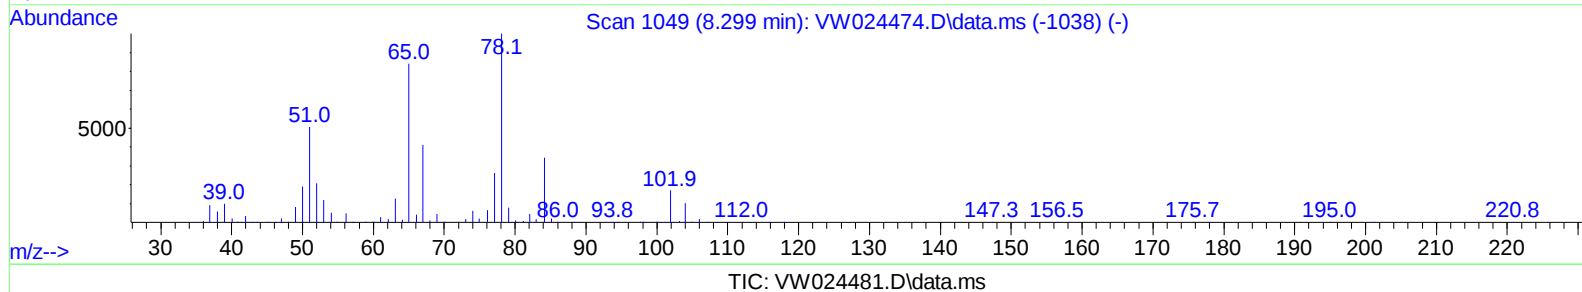
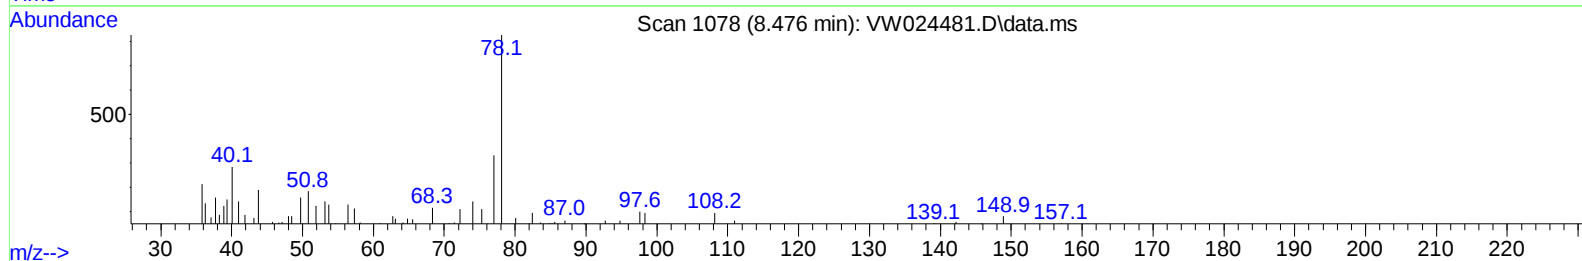


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
Data File : VW024481.D
Acq On : 30 Aug 2022 08:50
Operator : SY/VA
Sample : N4319-11RE
Misc : 4.67g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 31 01:18:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Aug 30 07:05:43 2022
Response via : Initial Calibration

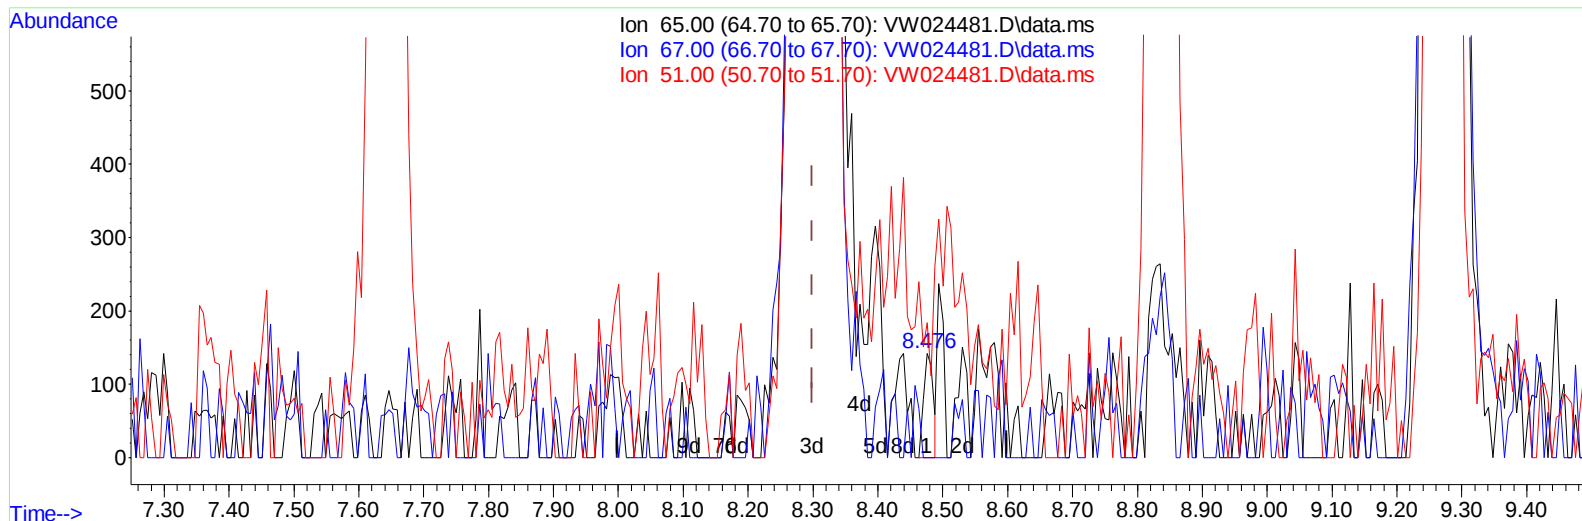

(26) 1,2-Dichloroethane-d4 (S)

8.476min (+ 0.177) 0.02 ug/L

response 148

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.10	40.54
51.00	96.50	91.89
0.00	0.00	0.00