
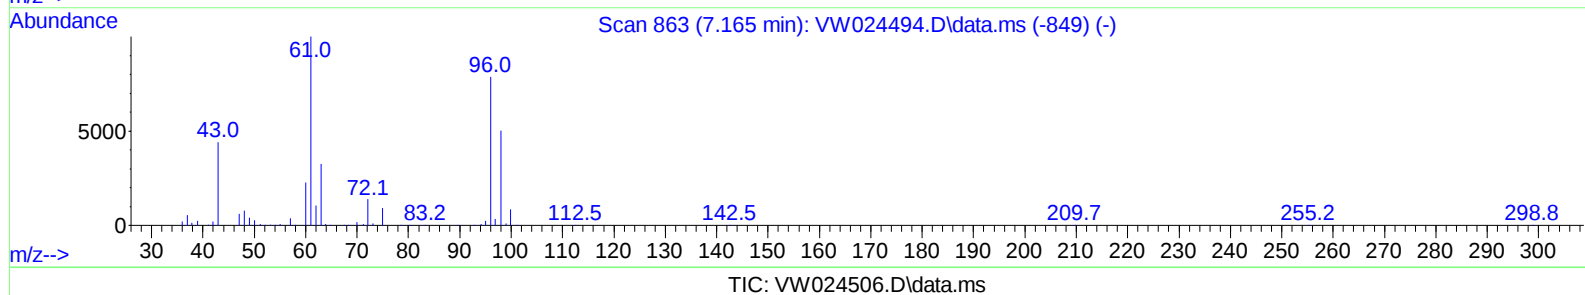
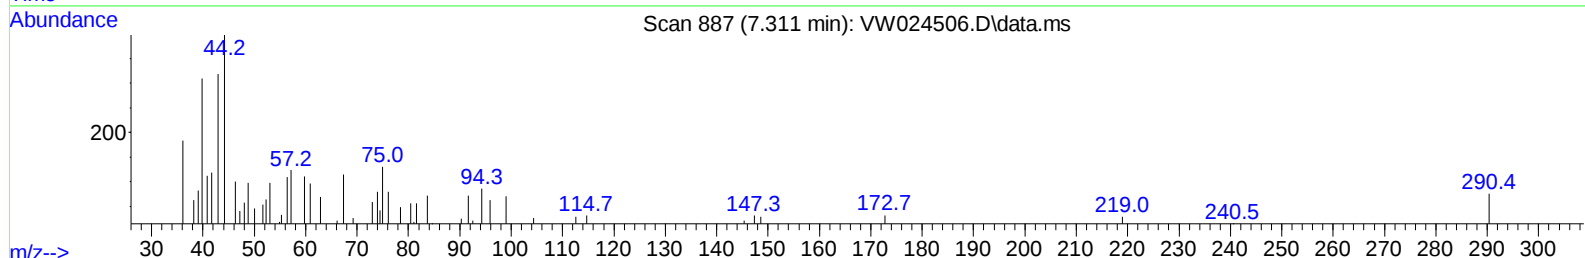


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024506.D
 Acq On : 30 Aug 2022 21:43
 Operator : SY/VA
 Sample : VSTDCCC025EC
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 31 02:57:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 31 02:55:40 2022
 Response via : Initial Calibration

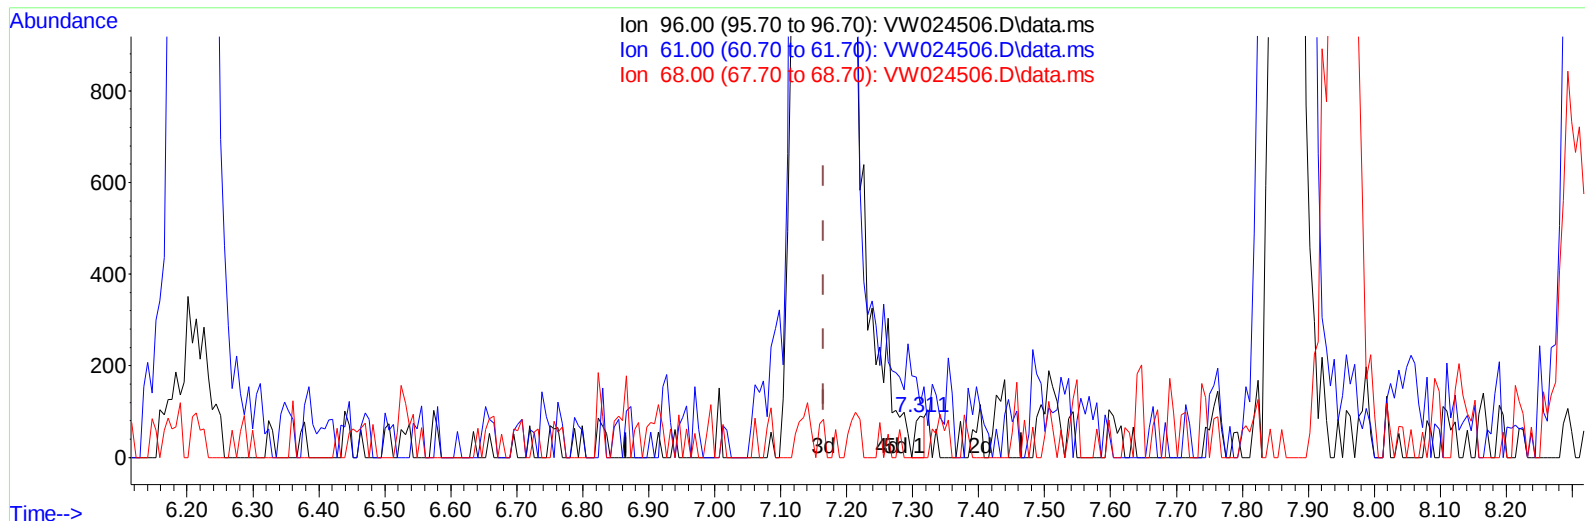

(20) cis-1,2-Dichloroethene (T)

7.311min (+ 0.146) 0.02 ug/L

response	94	
Ion	Exp%	Act%
96.00	100.00	100.00
61.00	128.90	130.00
68.00	0.00	0.00
0.00	0.00	0.00