

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024454.D
 Acq On : 29 Aug 2022 18:52
 Operator : SY/VA
 Sample : VW0829SBL02
 Misc : 5.53g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Aug 30 00:25:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 30 00:24:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	330192	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	316282	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	146497	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.337	65	177012	19.448	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	77.800%	
7) Chloroethane-d5	2.873	69	125992	18.475	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	73.880%	
11) 1,1-Dichloroethene-d2	4.001	63	116226	14.723	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110	Recovery	=	58.880%	
21) 2-Butanone-d5	7.074	46	78707	46.947	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	93.900%	
24) Chloroform-d	7.641	84	230668	21.730	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	86.920%	
26) 1,2-Dichloroethane-d4	8.098	65	140	0.022	ug/L	-0.21
Spiked Amount 25.000	Range 70	- 130	Recovery	=	0.080%#	
32) Benzene-d6	8.269	84	409212	22.582	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	90.320%	
36) 1,2-Dichloropropane-d6	9.275	67	132050	23.431	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	93.720%	
41) Toluene-d8	10.323	98	348155	20.207	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	80.840%	
43) trans-1,3-Dichloroprop...	10.579	79	54991	20.851	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	83.400%	
47) 2-Hexanone-d5	10.921	63	62058	49.207	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	98.420%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	136046	21.322	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	85.280%	
66) 1,2-Dichlorobenzene-d4	13.853	152	134998	24.471	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	97.880%	
Target Compounds						
39) cis-1,3-Dichloropropene	10.031	75	5003	0.704	ug/L	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
Data File : VW024454.D
Acq On : 29 Aug 2022 18:52
Operator : SY/VA
Sample : VW0829SBL02
Misc : 5.53g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Aug 30 00:25:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Aug 30 00:24:06 2022
Response via : Initial Calibration

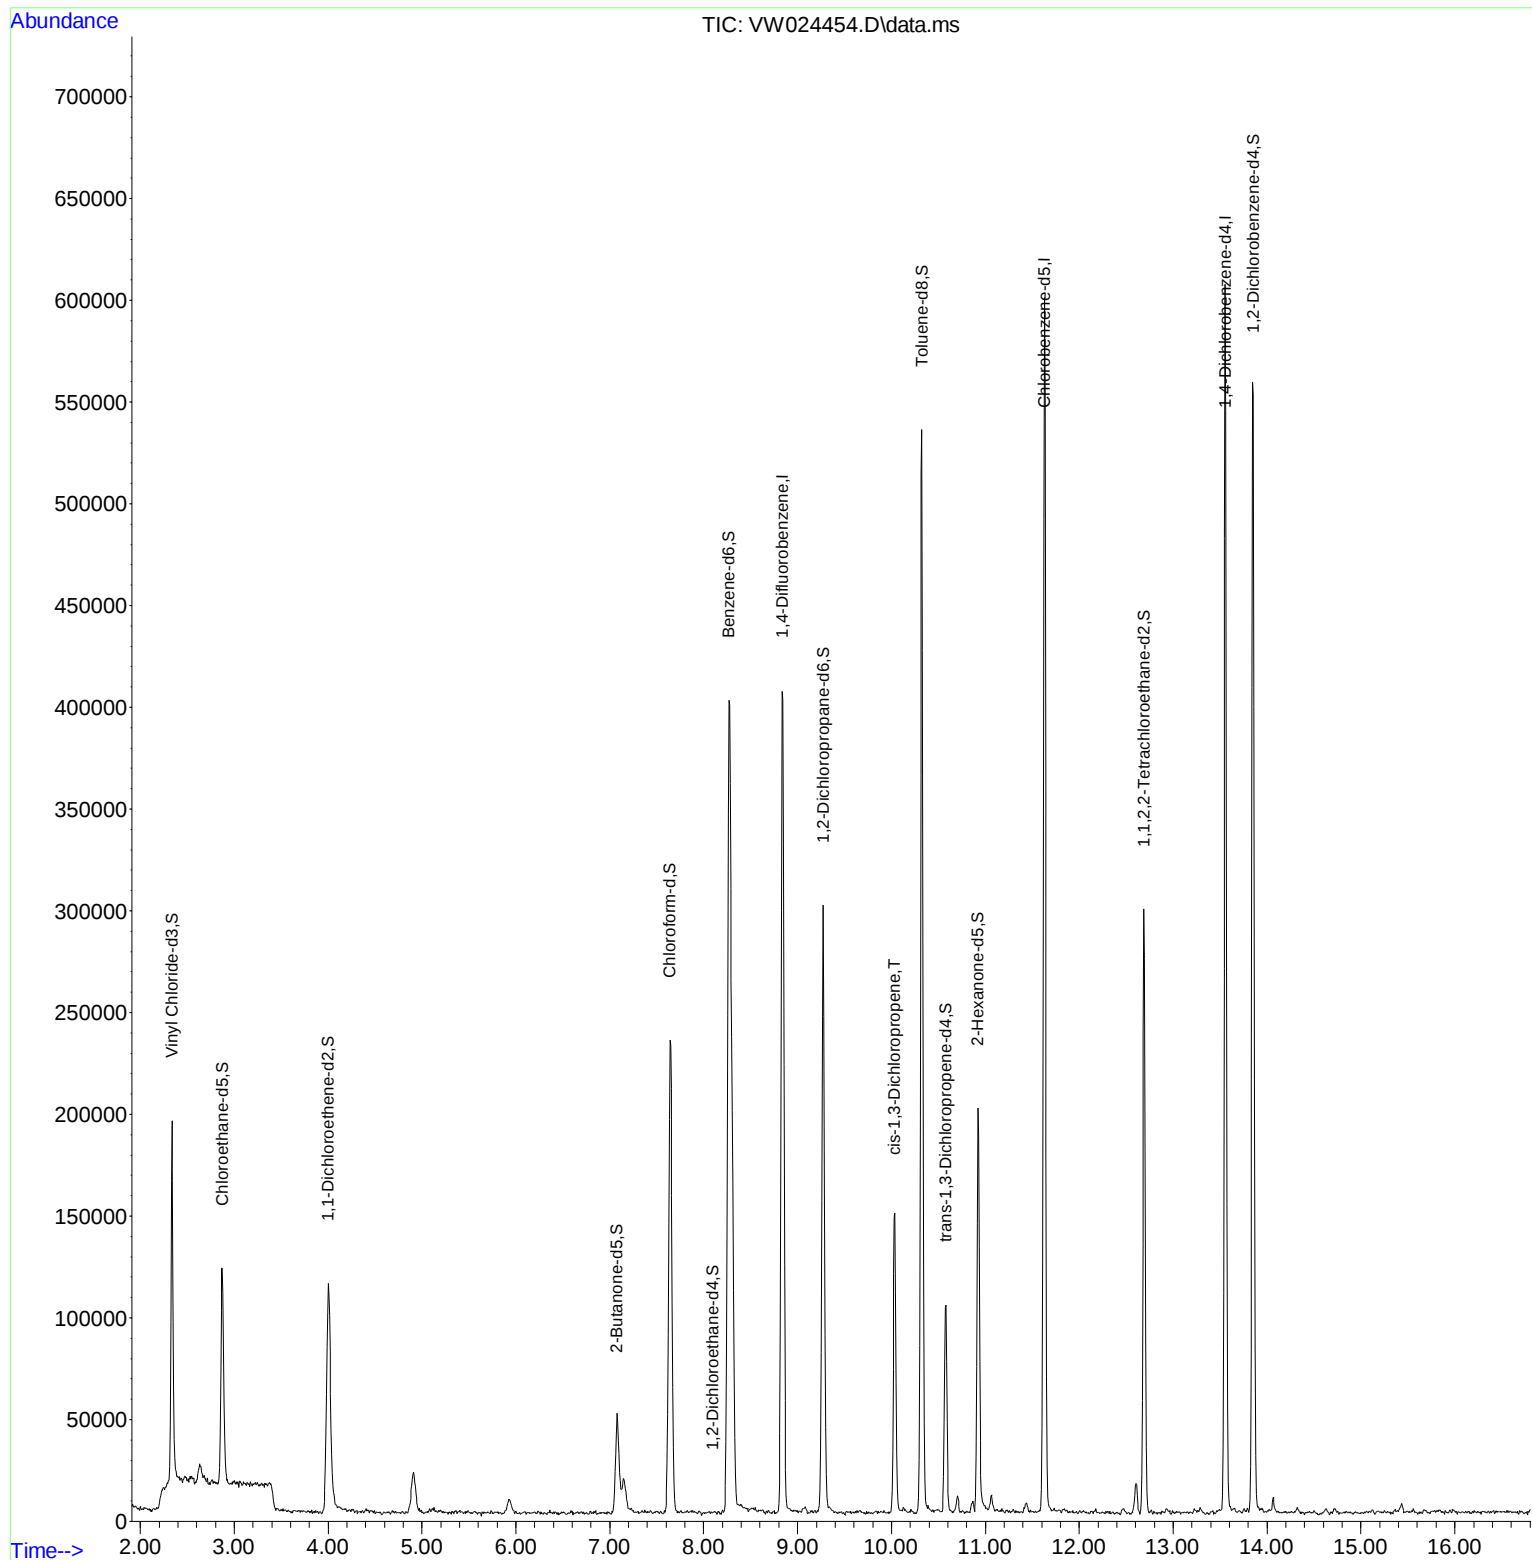

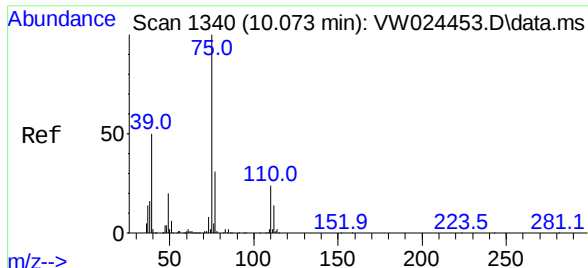

cis-1,3-Dichloropropene
 Concen: 0.704 ug/L
 RT: 10.031 min Scan# 1333
 Delta R.T. -0.043 min
 Lab File: VW024454.D
 Acq: 29 Aug 2022 18:52

Instrument : MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 5003
 Ion Ratio Lower Upper
 75 100
 77 35.0 21.8 40.6

