

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024457.D
 Acq On : 29 Aug 2022 20:06
 Operator : SY/VA
 Sample : N4362-06
 Misc : 5.98g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Aug 30 00:25:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 30 00:24:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	402563	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	390282	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	179553	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.337	65	209795	18.906	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	75.640%	
7) Chloroethane-d5	2.873	69	131108	15.769	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	63.080%	
11) 1,1-Dichloroethene-d2	4.001	63	153145	15.913	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110	Recovery	=	63.640%	
21) 2-Butanone-d5	7.074	46	60848	29.770	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	59.540%	
24) Chloroform-d	7.641	84	234151	18.092	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	72.360%	
26) 1,2-Dichloroethane-d4	8.299	65	131986	16.817	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	67.280%#	
32) Benzene-d6	8.268	84	452499	20.236	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	80.960%	
36) 1,2-Dichloropropane-d6	9.274	67	131465	18.904	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	75.600%	
41) Toluene-d8	10.323	98	420018	19.756	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	79.040%	
43) trans-1,3-Dichloroprop...	10.579	79	53313	16.382	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	65.520%	
47) 2-Hexanone-d5	10.920	63	47275	30.378	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	60.760%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	116859	14.842	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	59.360%	
66) 1,2-Dichlorobenzene-d4	13.853	152	131421	19.437	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	77.760%	
Target Compounds						
13) Acetone	4.129	43	6218	5.098	ug/L	80
34) Trichloroethene	9.092	95	3400	0.531	ug/L #	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
Data File : VW024457.D
Acq On : 29 Aug 2022 20:06
Operator : SY/VA
Sample : N4362-06
Misc : 5.98g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Aug 30 00:25:37 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Aug 30 00:24:06 2022
Response via : Initial Calibration

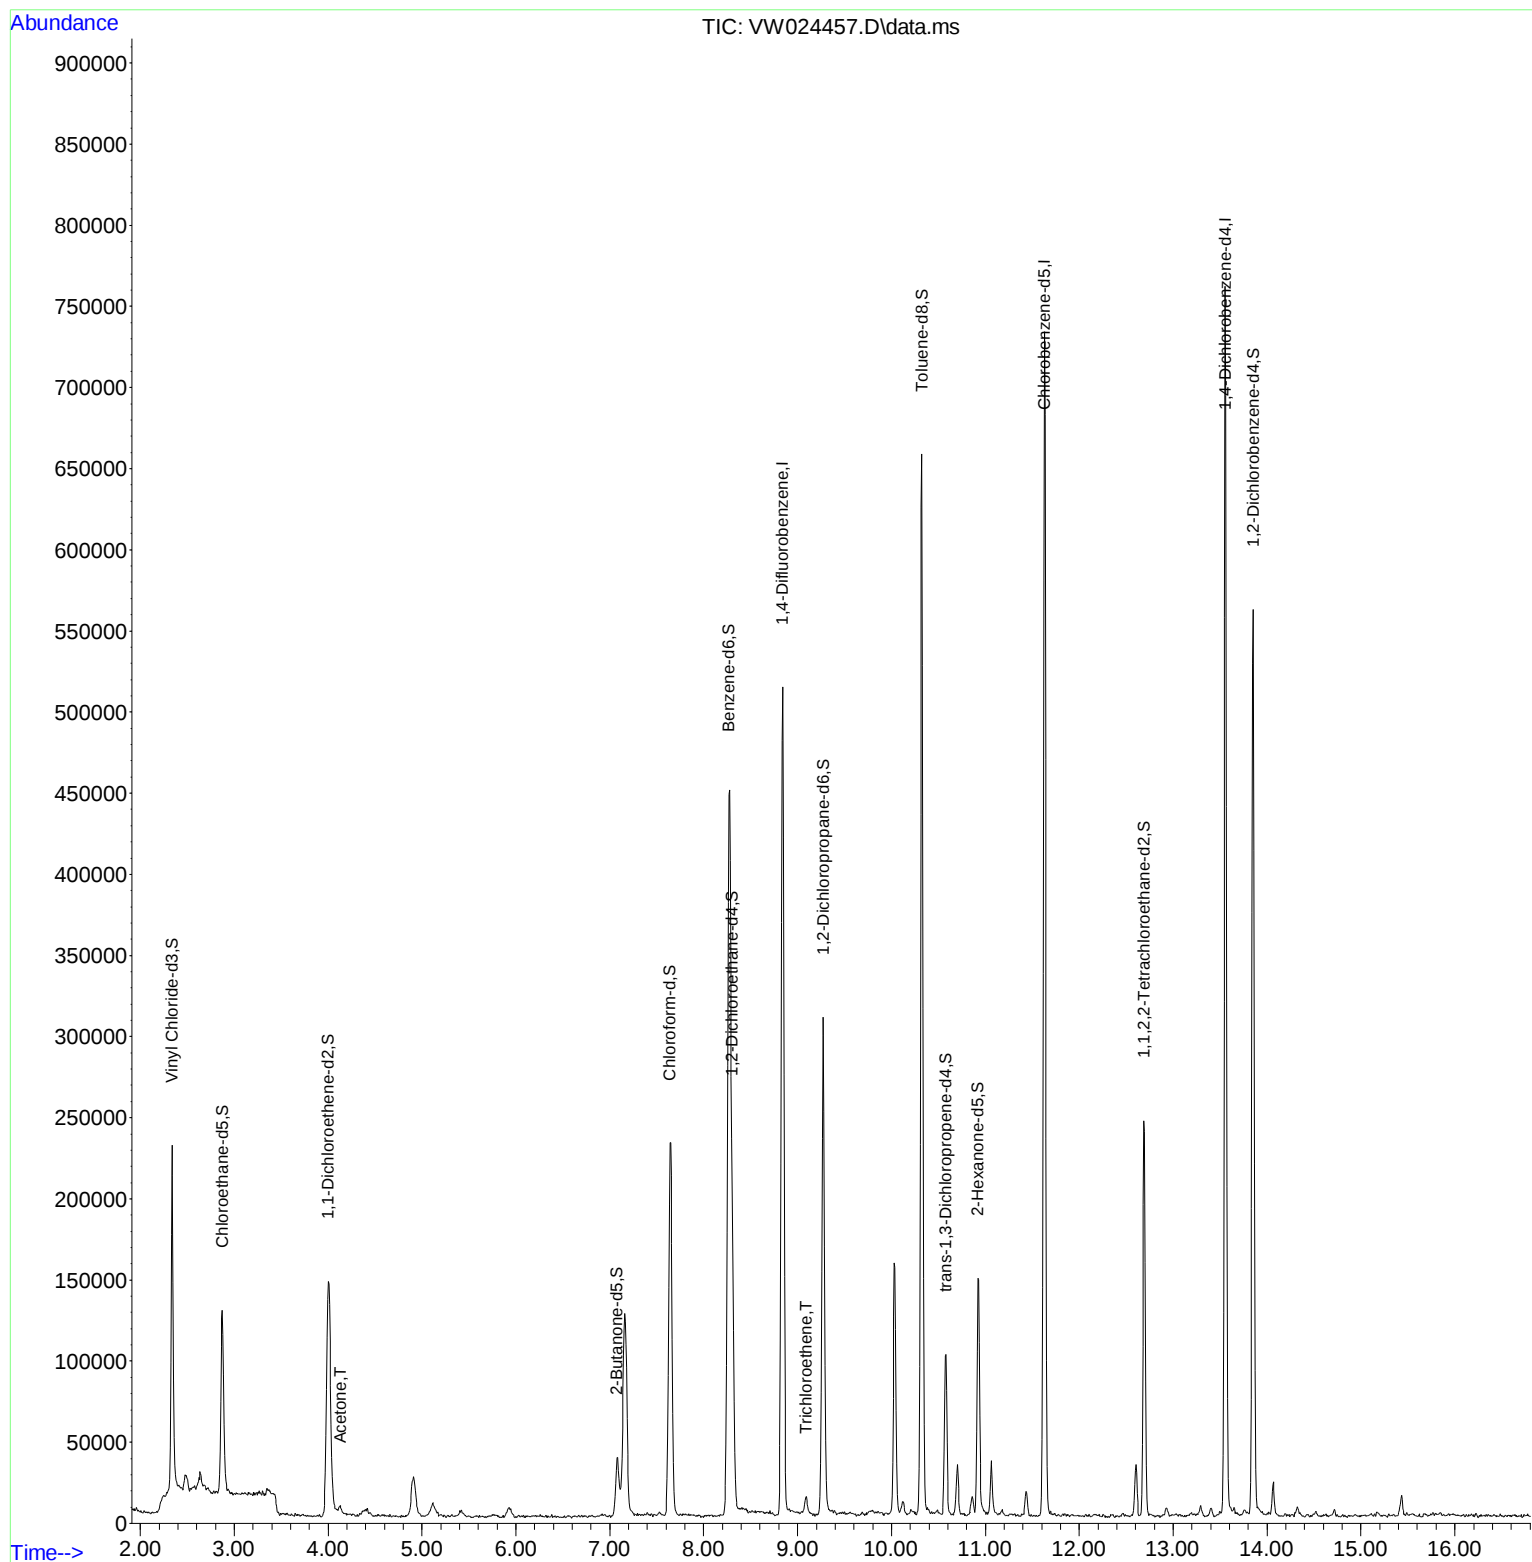

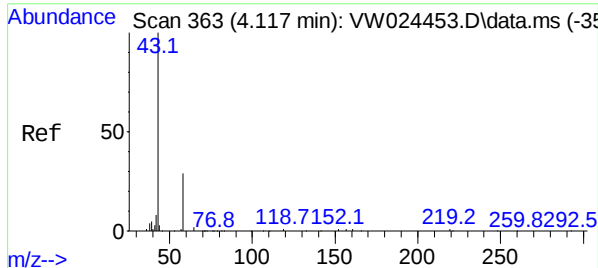

Acetone

Concen: 5.098 ug/L

RT: 4.129 min Scan#

Delta R.T. 0.012 min

Lab File: VW024457.D

Acq: 29 Aug 2022 20:06

Instrument :

MSVOA_W





ClientSampleId :

Tgt Ion: 43 Resp: 6218

Ion Ratio Lower Upper

43 100

58 39.8 0.0 58.4

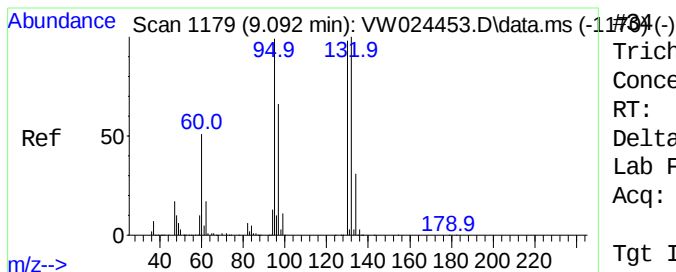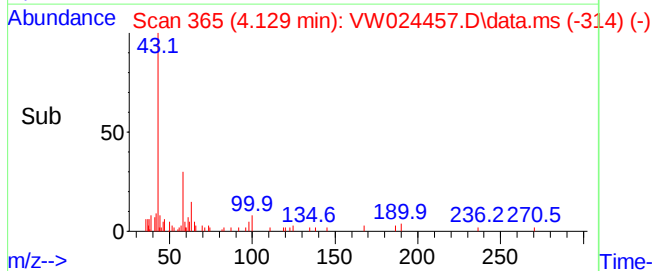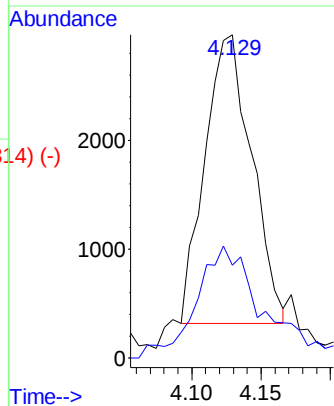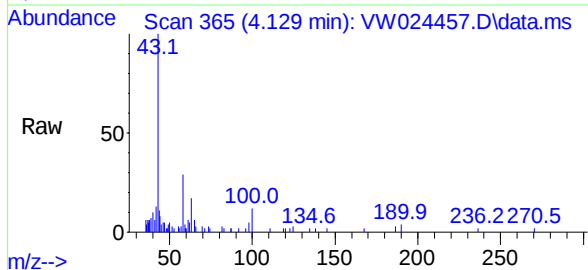

Trichloroethene

Concen: 0.531 ug/L

RT: 9.092 min Scan# 1179

Delta R.T. -0.000 min

Lab File: VW024457.D

Acq: 29 Aug 2022 20:06

Tgt Ion: 95 Resp: 3400

Ion Ratio Lower Upper

95 100

97 40.9 48.4 89.8#

132 66.5 68.6 127.4#

130 61.8 72.6 134.8#

