

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024501.D
 Acq On : 30 Aug 2022 19:39
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Aug 31 02:57:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 31 02:55:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	287798	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	289802	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	131166	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.337	65	162374	20.467	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	81.880%		
7) Chloroethane-d5	2.873	69	122725	20.647	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	82.600%		
11) 1,1-Dichloroethene-d2	4.007	63	104479	15.185	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	60.720%		
21) 2-Butanone-d5	6.982	46	188	0.129	ug/L	-0.09
Spiked Amount 50.000	Range 20 - 135		Recovery =	0.260%#		
24) Chloroform-d	7.647	84	217067	23.461	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	93.840%		
26) 1,2-Dichloroethane-d4	8.305	65	136566	24.339	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	97.360%		
32) Benzene-d6	8.268	84	379976	22.884	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	91.520%		
36) 1,2-Dichloropropane-d6	9.274	67	125024	24.211	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	96.840%		
41) Toluene-d8	10.323	98	321683	20.376	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	81.520%		
43) trans-1,3-Dichloroprop...	10.573	79	52298	21.642	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	86.560%		
47) 2-Hexanone-d5	10.920	63	65046	56.289	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	112.580%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	139642	23.885	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	95.520%		
66) 1,2-Dichlorobenzene-d4	13.853	152	133722	27.073	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	108.280%		
Target Compounds						
39) cis-1,3-Dichloropropene	10.036	75	4948	0.760	ug/L	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
Data File : VW024501.D
Acq On : 30 Aug 2022 19:39
Operator : SY/VA
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Aug 31 02:57:03 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 31 02:55:40 2022
Response via : Initial Calibration

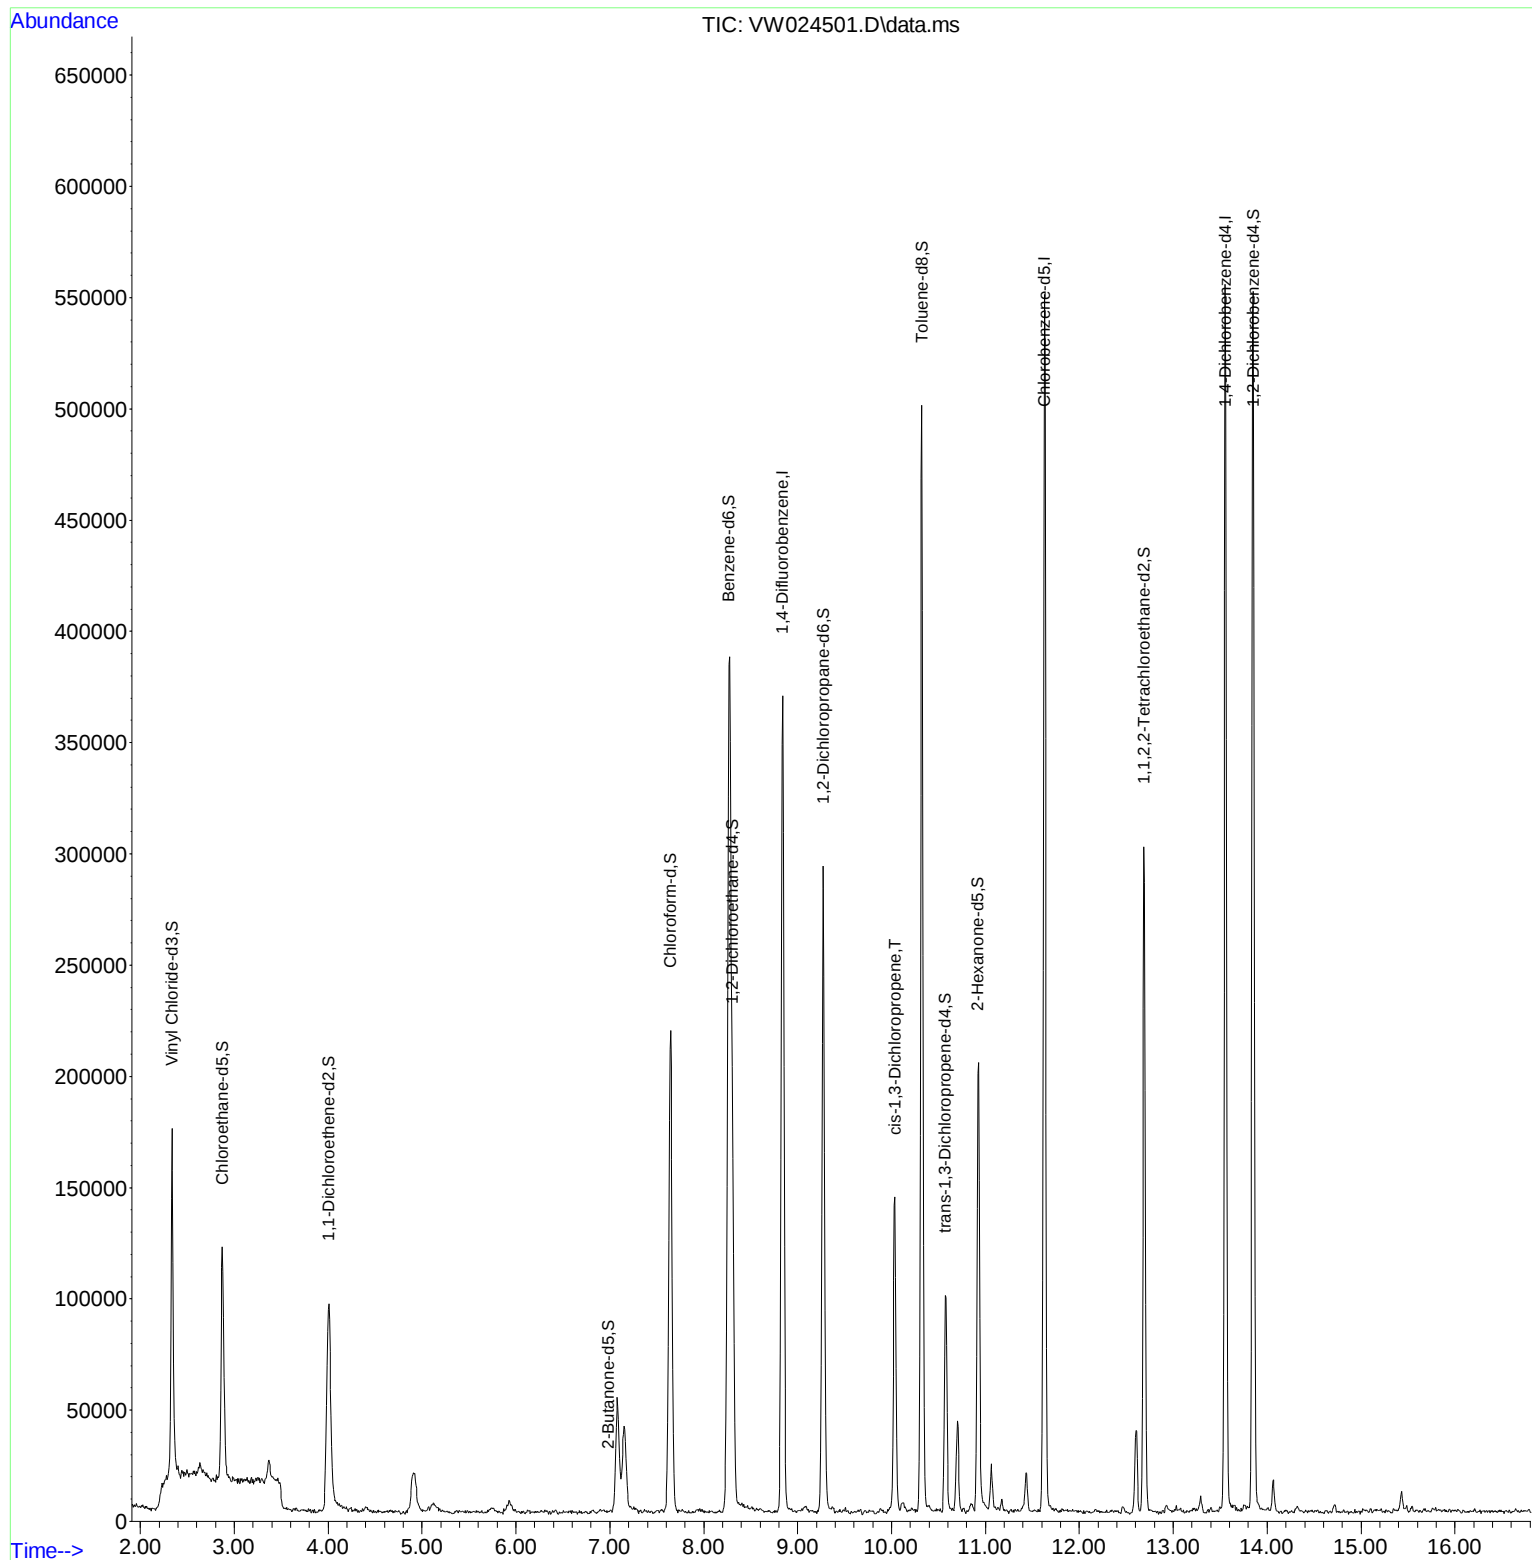

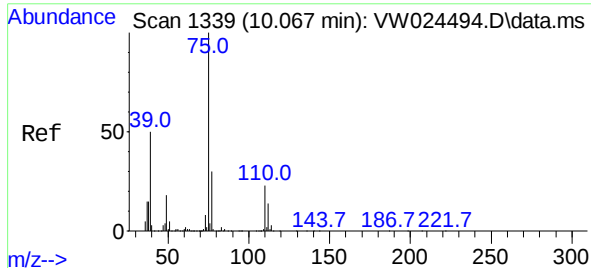

cis-1,3-Dichloropropene
 Concen: 0.760 ug/L
 RT: 10.036 min Scan# 1339
 Delta R.T. -0.031 min
 Lab File: VW024501.D
 Acq: 30 Aug 2022 19:39

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 4948
 Ion Ratio Lower Upper
 75 100
 77 34.6 21.8 40.6

