

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024503.D
 Acq On : 30 Aug 2022 20:29
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Aug 31 02:57:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 31 02:55:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	316848	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	303338	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	135969	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.337	65	168425	19.283	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	77.120%		
7) Chloroethane-d5	2.873	69	126321	19.303	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	77.200%		
11) 1,1-Dichloroethene-d2	4.001	63	105715	13.956	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	55.840%		
21) 2-Butanone-d5	7.080	46	82980	51.581	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	103.160%		
24) Chloroform-d	7.647	84	227813	22.364	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	89.440%		
26) 1,2-Dichloroethane-d4	8.305	65	140678	22.773	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	91.080%		
32) Benzene-d6	8.268	84	400363	23.036	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	92.160%		
36) 1,2-Dichloropropane-d6	9.274	67	130701	24.181	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	96.720%		
41) Toluene-d8	10.323	98	344920	20.873	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	83.480%		
43) trans-1,3-Dichloroprop...	10.579	79	55200	21.823	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	87.280%		
47) 2-Hexanone-d5	10.920	63	66697	55.142	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	110.280%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	141769	23.167	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	92.680%		
66) 1,2-Dichlorobenzene-d4	13.853	152	140502	27.440	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	109.760%		
Target Compounds						
39) cis-1,3-Dichloropropene	10.036	75	4825	0.708	ug/L #	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
Data File : VW024503.D
Acq On : 30 Aug 2022 20:29
Operator : SY/VA
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Aug 31 02:57:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 31 02:55:40 2022
Response via : Initial Calibration

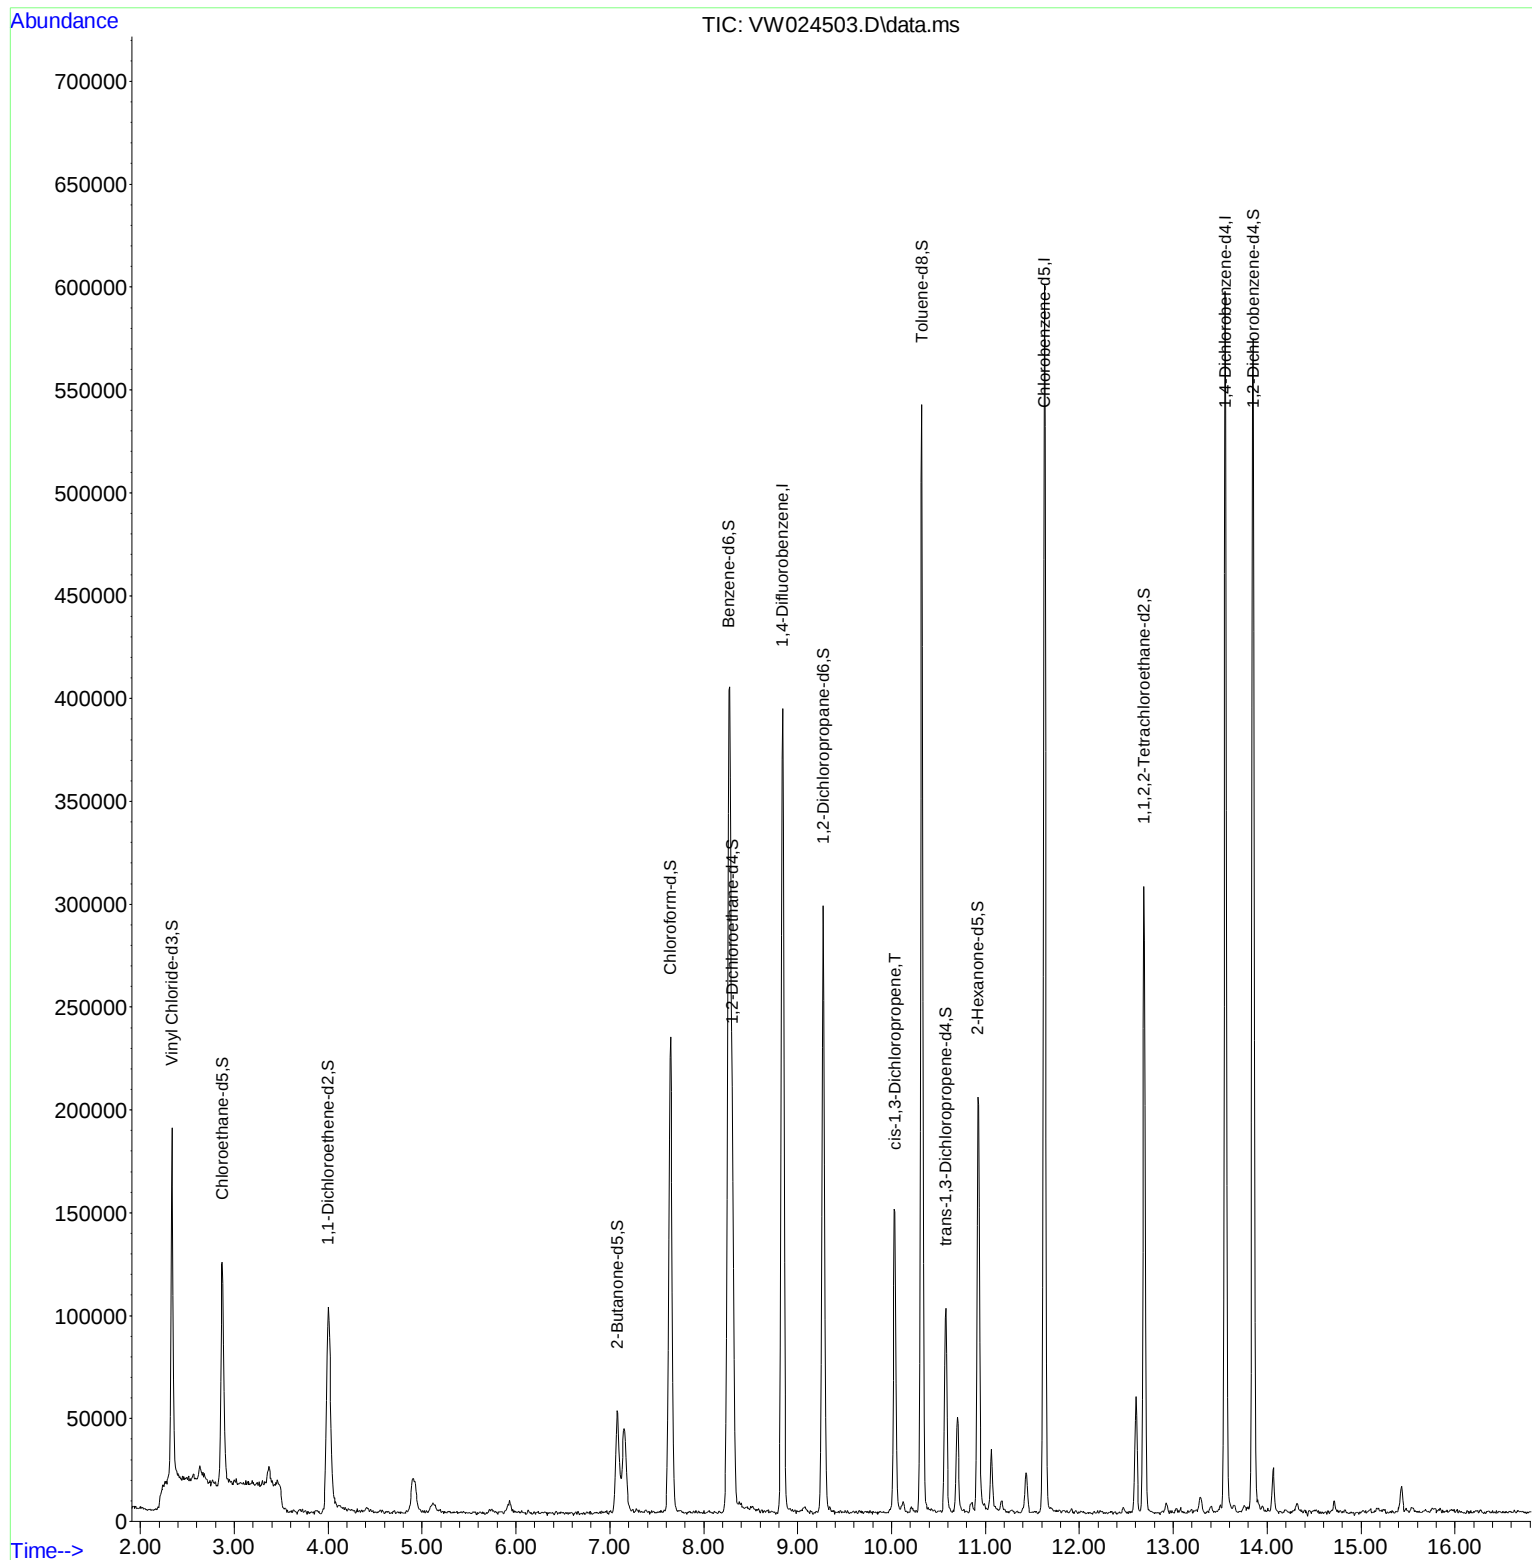

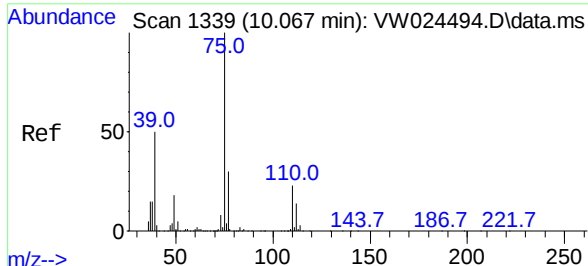

cis-1,3-Dichloropropene
 Concen: 0.708 ug/L
 RT: 10.036 min Scan# 1339
 Delta R.T. -0.031 min
 Lab File: VW024503.D
 Acq: 30 Aug 2022 20:29

Instrument : MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 4825
 Ion Ratio Lower Upper
 75 100
 77 48.8 21.8 40.6#

