

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024504.D
 Acq On : 30 Aug 2022 20:53
 Operator : SY/VA
 Sample : N4345-05RE
 Misc : 4.29g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Aug 31 02:57:24 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 31 02:55:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	401225	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	403601	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	180464	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.336	65	196115	17.732	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	70.920%	
7) Chloroethane-d5	2.873	69	124992	15.083	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	60.320%	
11) 1,1-Dichloroethene-d2	4.001	63	131703	13.730	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	54.920%	
21) 2-Butanone-d5	7.079	46	56265	27.619	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	55.240%	
24) Chloroform-d	7.646	84	219256	16.998	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	68.000%	
26) 1,2-Dichloroethane-d4	8.421	65	367	0.047	ug/L	0.12
Spiked Amount 25.000	Range 70	- 130	Recovery	=	0.200%#	
32) Benzene-d6	8.268	84	423422	18.311	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	73.240%	
36) 1,2-Dichloropropane-d6	9.268	67	126978	17.656	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	70.640%	
41) Toluene-d8	10.323	98	387142	17.608	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	70.440%	
43) trans-1,3-Dichloroprop...	10.573	79	47867	14.223	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	56.880%	
47) 2-Hexanone-d5	10.926	63	44986	27.953	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	55.900%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	108400	13.313	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	53.240%	
66) 1,2-Dichlorobenzene-d4	13.853	152	128338	18.885	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	75.520%	
Target Compounds						
39) cis-1,3-Dichloropropene	10.024	75	4581	0.505	ug/L	Qvalue 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
Data File : VW024504.D
Acq On : 30 Aug 2022 20:53
Operator : SY/VA
Sample : N4345-05RE
Misc : 4.29g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Aug 31 02:57:24 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 31 02:55:40 2022
Response via : Initial Calibration

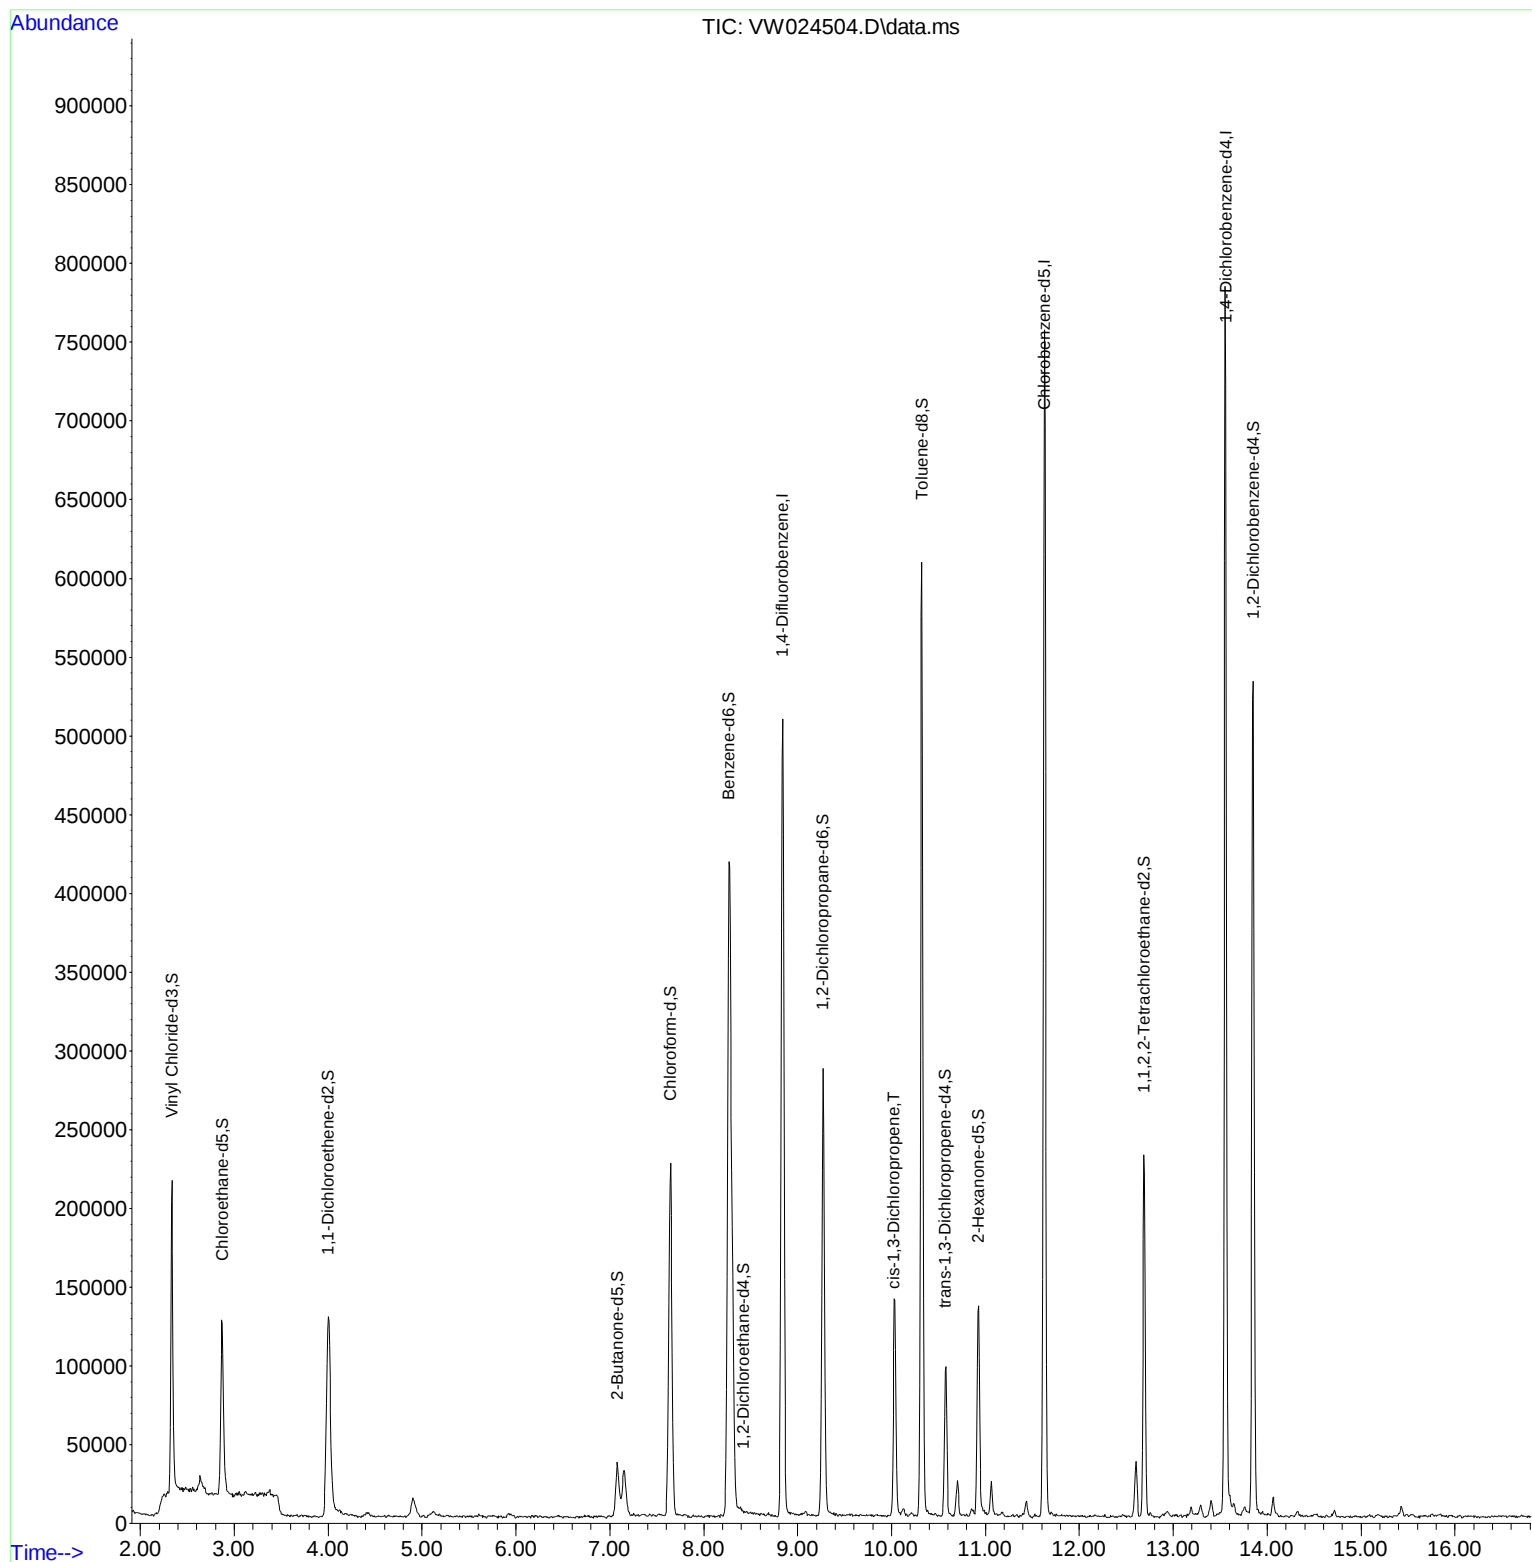

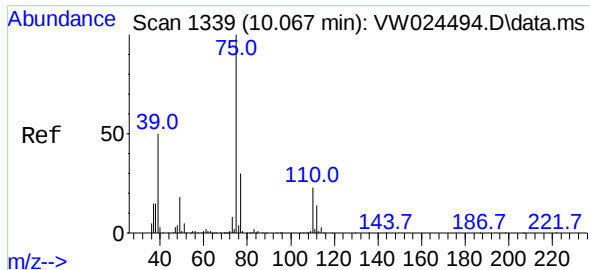

cis-1,3-Dichloropropene
 Concen: 0.505 ug/L
 RT: 10.024 min Scan# 1332
 Delta R.T. -0.043 min
 Lab File: VW024504.D
 Acq: 30 Aug 2022 20:53

Instrument : MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 4581
 Ion Ratio Lower Upper
 75 100
 77 37.8 21.8 40.6

