




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
Data File : VW024439.D
Acq On : 29 Aug 2022 11:35
Operator : SY/VA
Sample : N4346-11
Misc : 6.07g/10mL/MSVOA_W/soil
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBVU9

Manual IntegrationsAPPROVED

Quant Time: Aug 29 22:55:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Aug 29 22:53:57 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/30/2022
Supervised By :Mahesh Dadoda 08/31/2022

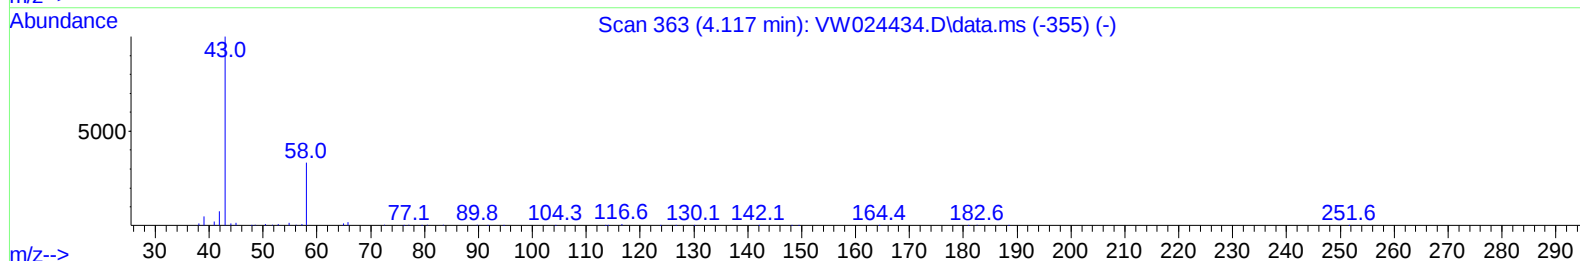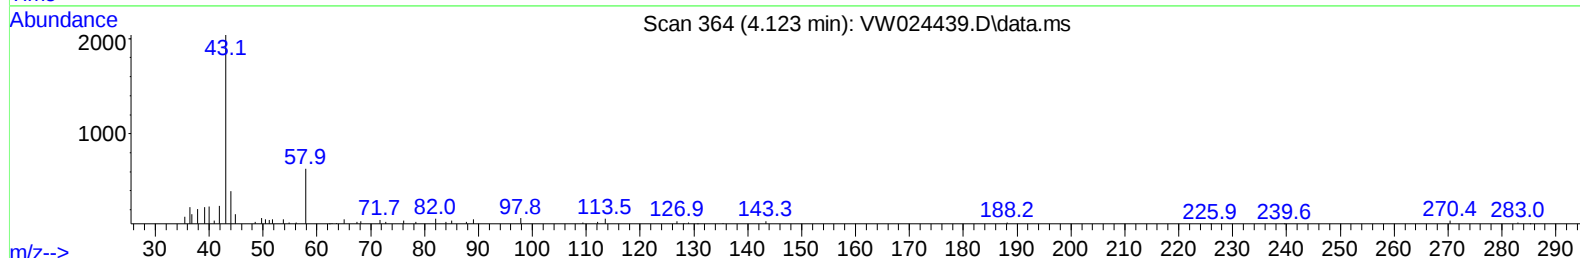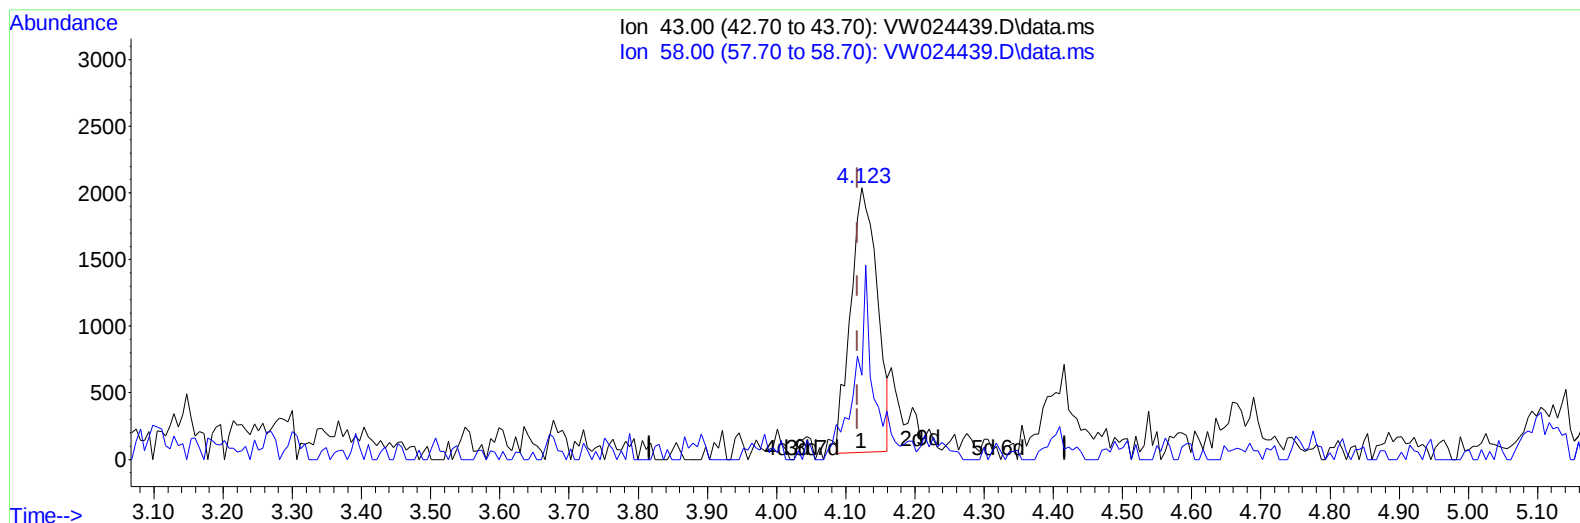

TIC: VW024439.D\data.ms

(13) Acetone (T)

4.123min (+ 0.006) 11.45 ug/L

response 5251

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	29.20	43.95
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024439.D
 Acq On : 29 Aug 2022 11:35
 Operator : SY/VA
 Sample : N4346-11
 Misc : 6.07g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVU9

Manual IntegrationsAPPROVED

Quant Time: Aug 29 22:55:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Aug 29 22:53:57 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/30/2022
 Supervised By :Mahesh Dadoda 08/31/2022

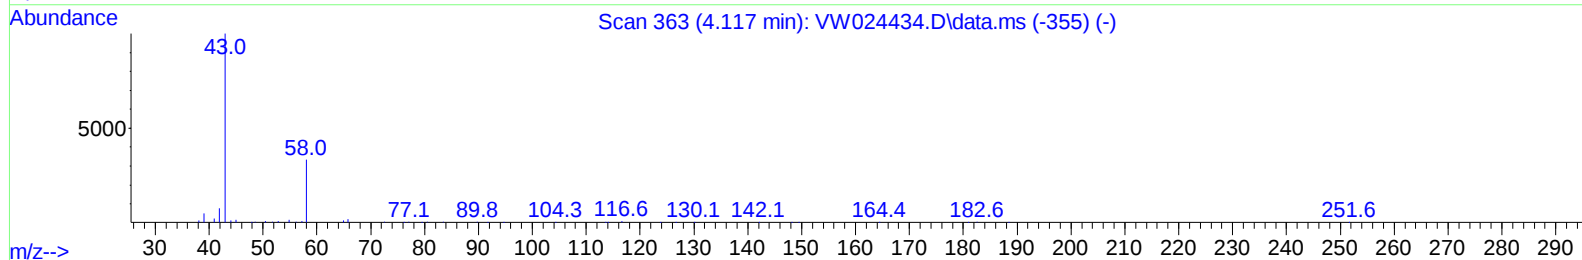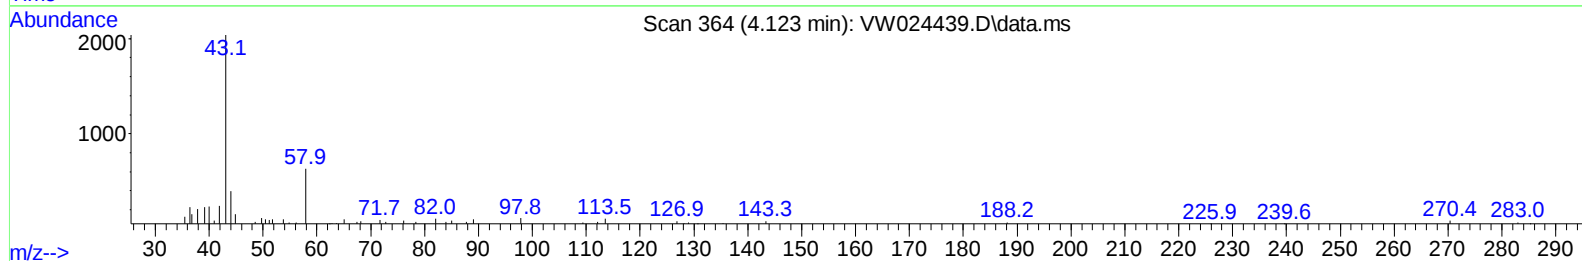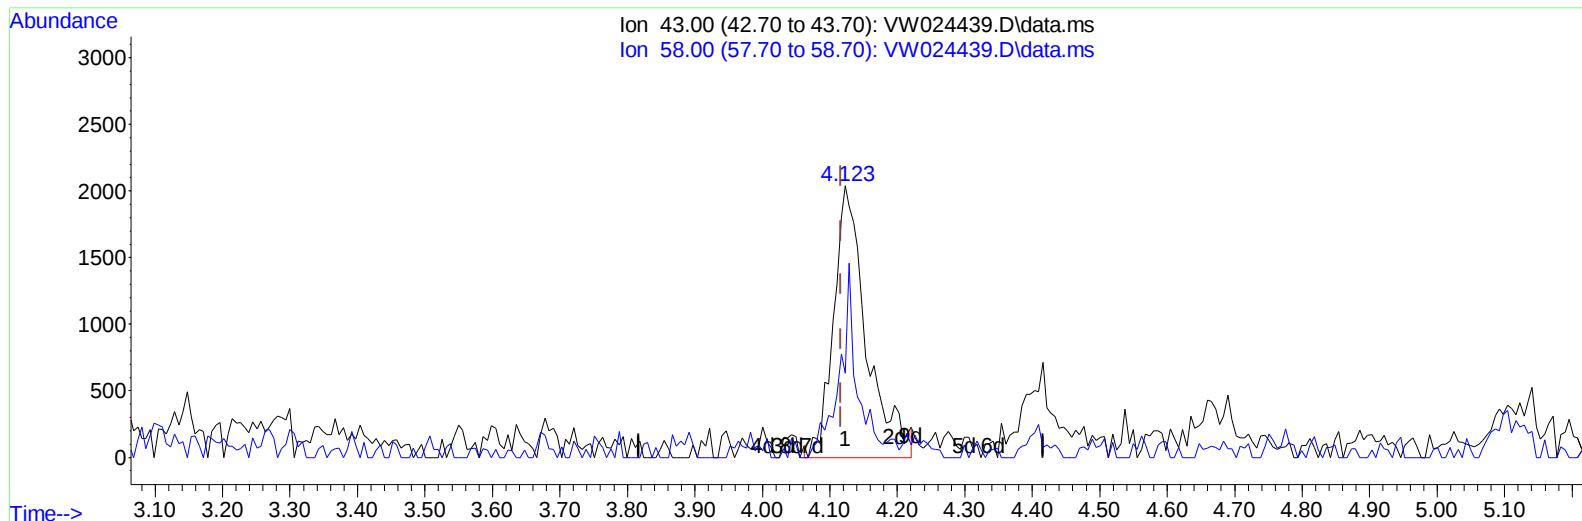

TIC: VW024439.D\data.ms

(13) Acetone (T)

4.123min (+ 0.006) 14.99 ug/L m

response 6878

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	29.20	33.56
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
Data File : VW024439.D
Acq On : 29 Aug 2022 11:35
Operator : SY/VA
Sample : N4346-11
Misc : 6.07g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBVU9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
Supervised By :Mahesh Dadoda 08/31/2022

Quant Time: Aug 29 22:55:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Aug 29 22:53:57 2022
Response via : Initial Calibration

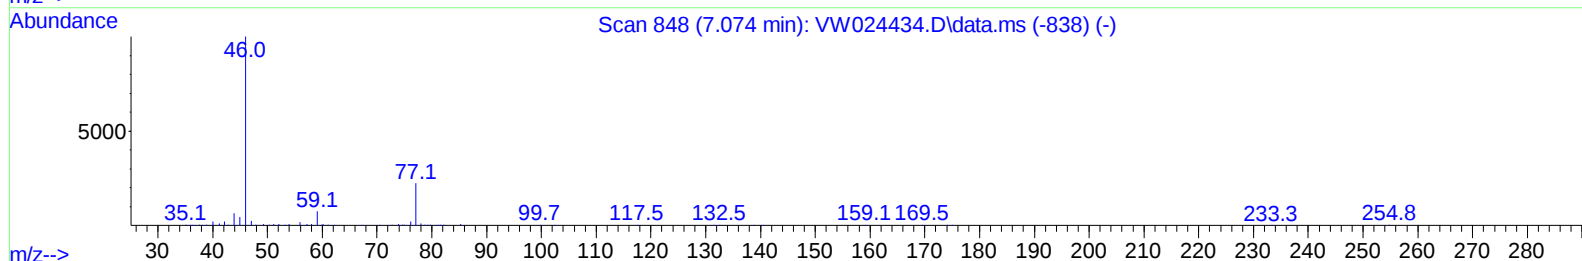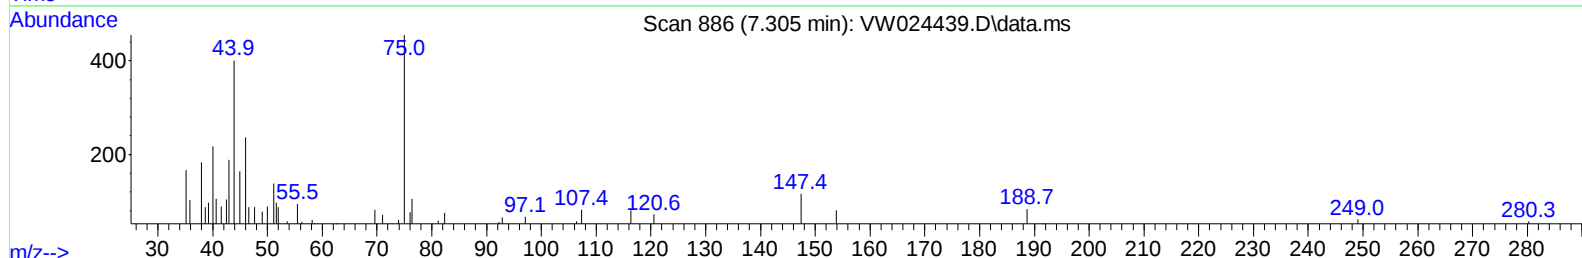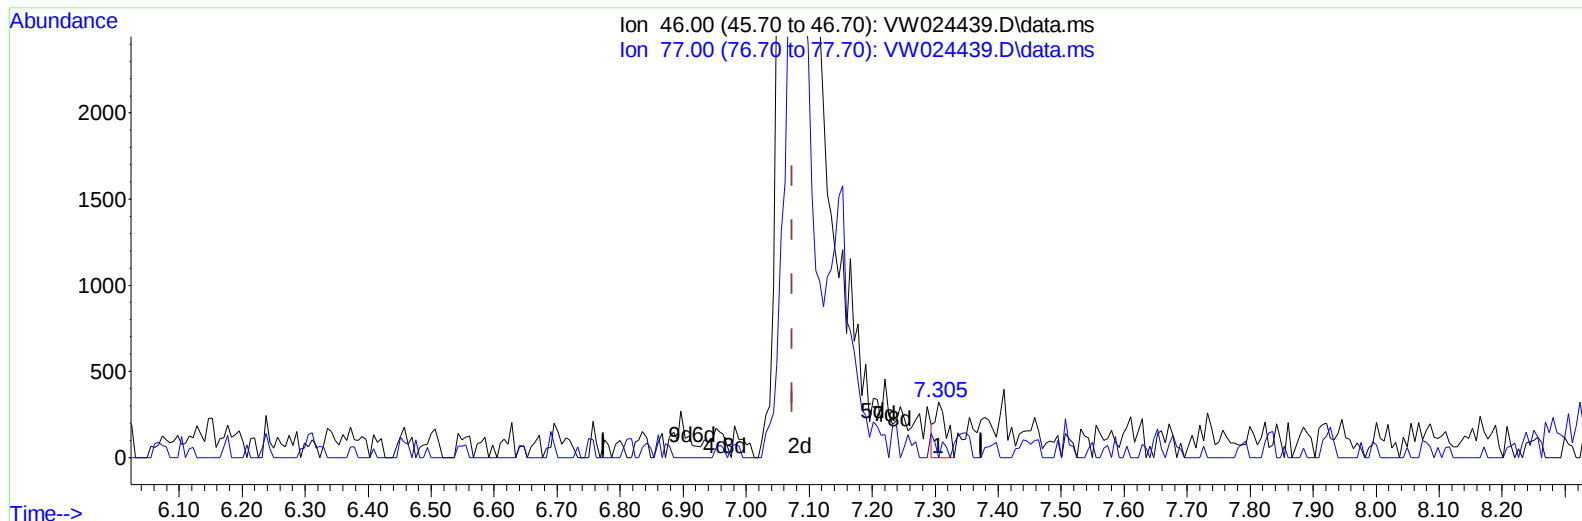

TIC: VW024439.D\data.ms

(21) 2-Butanone-d5 (S)

7.305min (+ 0.232) 0.52 ug/L

response 399

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	12.40	14.04
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
Data File : VW024439.D
Acq On : 29 Aug 2022 11:35
Operator : SY/VA
Sample : N4346-11
Misc : 6.07g/10mL/MSVOA_W/SoIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBVU9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
Supervised By :Mahesh Dadoda 08/31/2022

Quant Time: Aug 29 22:55:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Aug 29 22:53:57 2022
Response via : Initial Calibration

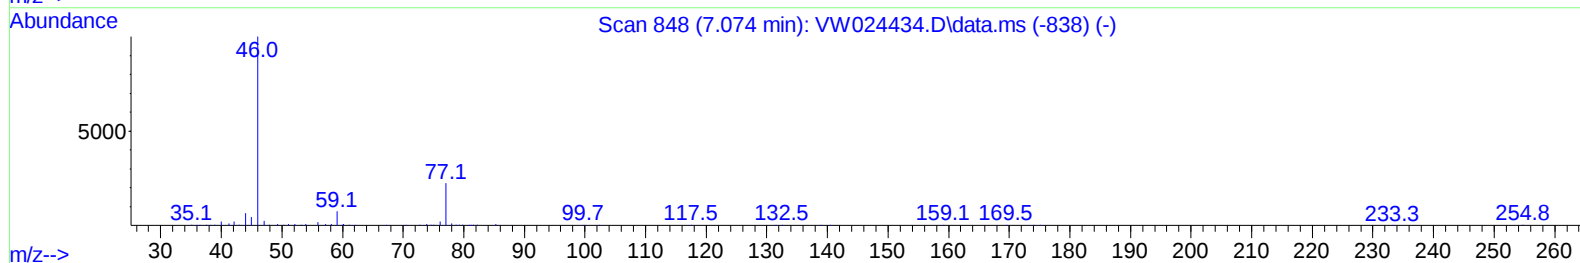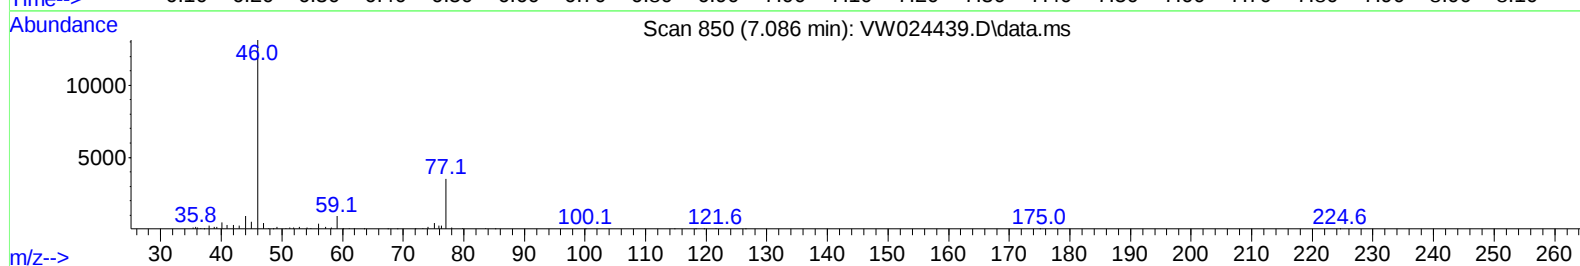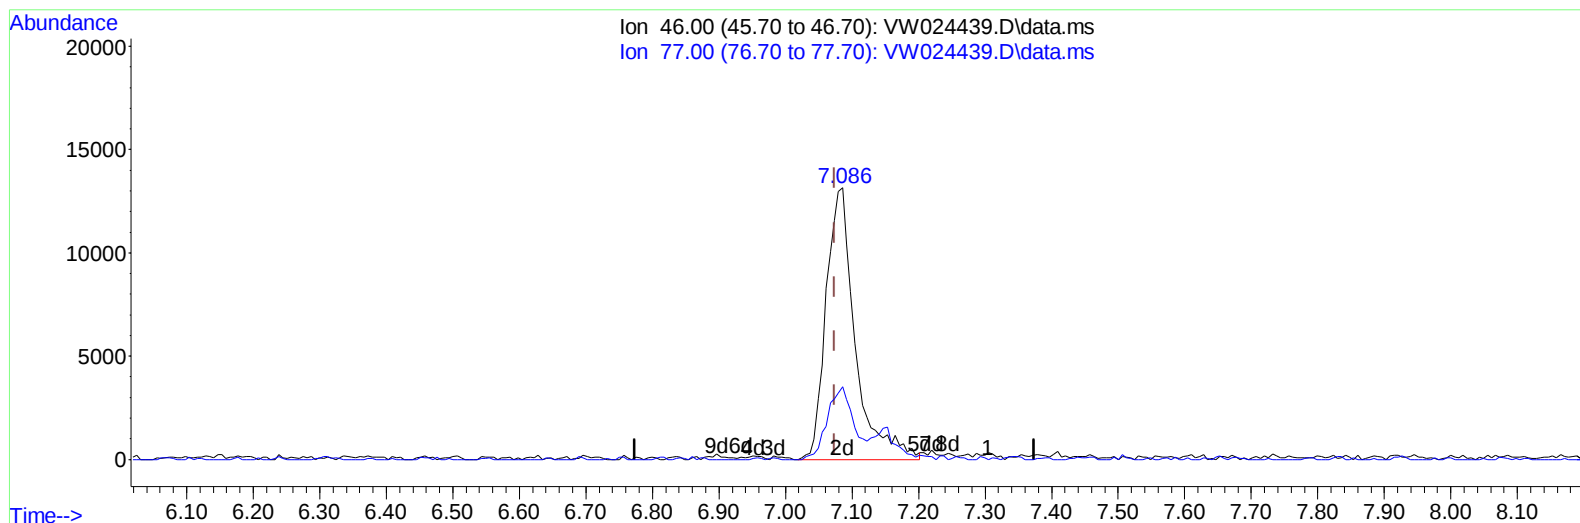

TIC: VW024439.D\data.ms

(21) 2-Butanone-d5 (S)

7.086min (+ 0.012) 52.00 ug/L m

response 39967

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	12.40	0.14#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024439.D
 Acq On : 29 Aug 2022 11:35
 Operator : SY/VA
 Sample : N4346-11
 Misc : 6.07g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVU9

Manual IntegrationsAPPROVED

Quant Time: Aug 29 22:55:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Aug 29 22:53:57 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/30/2022
 Supervised By :Mahesh Dadoda 08/31/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	151382	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	165433	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	93009	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	31904	7.645	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	30.600%	
7) Chloroethane-d5	2.873	69	32567	10.416	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	41.680%	
11) 1,1-Dichloroethene-d2	4.007	63	29606	8.180	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	32.720%#	
21) 2-Butanone-d5	7.086	46	39967m	51.999	ug/L	0.01
Spiked Amount 50.000	Range 20	- 135	Recovery	=	104.000%	
24) Chloroform-d	7.647	84	111348	22.879	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	91.520%	
26) 1,2-Dichloroethane-d4	8.305	65	93605	31.715	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	126.880%	
32) Benzene-d6	8.275	84	138100	14.570	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	58.280%	
36) 1,2-Dichloropropane-d6	9.274	67	77608	26.328	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	105.320%	
41) Toluene-d8	10.323	98	94551	10.492	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	41.960%	
43) trans-1,3-Dichloroprop...	10.579	79	28164	20.417	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	81.680%	
47) 2-Hexanone-d5	10.920	63	22225	33.692	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	67.380%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	97433	29.194	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	116.760%	
66) 1,2-Dichlorobenzene-d4	13.847	152	79866	22.803	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	91.200%	
Target Compounds						
					Qvalue	
13) Acetone	4.123	43	6878m	14.995	ug/L	
16) Methylene chloride	4.909	84	10397	4.095	ug/L	93
46) Tetrachloroethene	10.866	164	9697	4.599	ug/L	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
Data File : VW024439.D
Acq On : 29 Aug 2022 11:35
Operator : SY/VA
Sample : N4346-11
Misc : 6.07g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBVU9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
Supervised By :Mahesh Dadoda 08/31/2022

Quant Time: Aug 29 22:55:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Aug 29 22:53:57 2022
Response via : Initial Calibration

