




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024444.D
 Acq On : 29 Aug 2022 13:48
 Operator : SY/VA
 Sample : N4346-16
 Misc : 4.93g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVV4

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
 Supervised By :Mahesh Dadoda 08/31/2022

Quant Time: Aug 29 22:56:33 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Aug 29 22:53:57 2022
 Response via : Initial Calibration

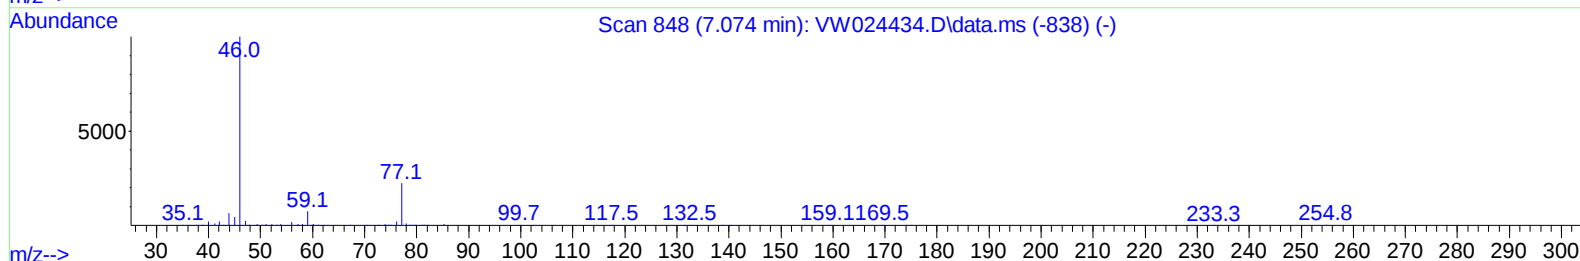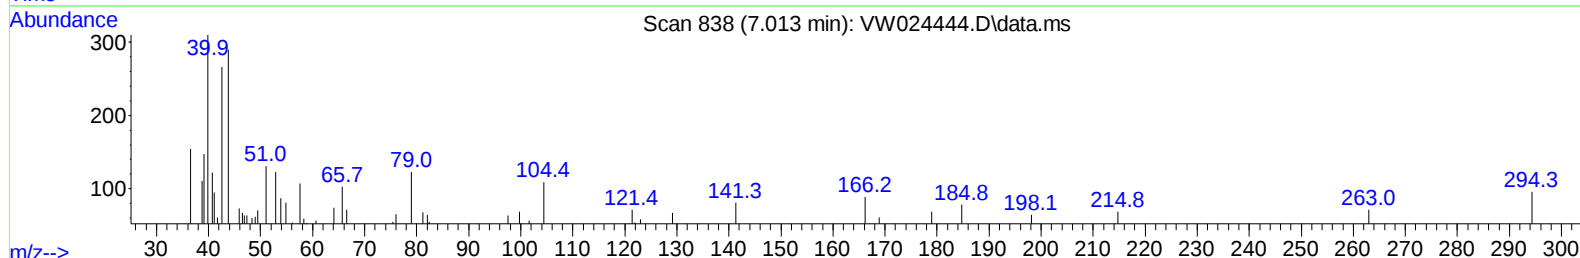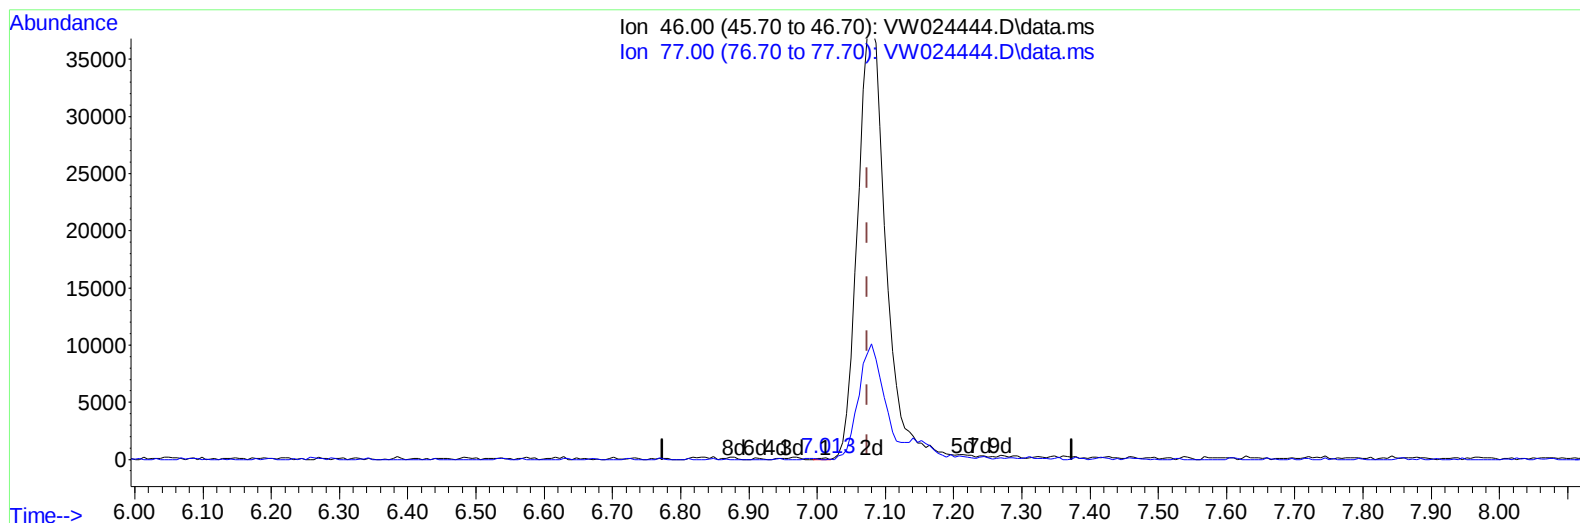

TIC: VW024444.D\data.ms

(21) 2-Butanone-d5 (S)

7.013min (-0.061) 0.07 ug/L

response	131	
Ion	Exp%	Act%
46.00	100.00	100.00
77.00	12.40	15.27
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024444.D
 Acq On : 29 Aug 2022 13:48
 Operator : SY/VA
 Sample : N4346-16
 Misc : 4.93g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVV4

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
 Supervised By :Mahesh Dadoda 08/31/2022

Quant Time: Aug 29 22:56:33 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Aug 29 22:53:57 2022
 Response via : Initial Calibration

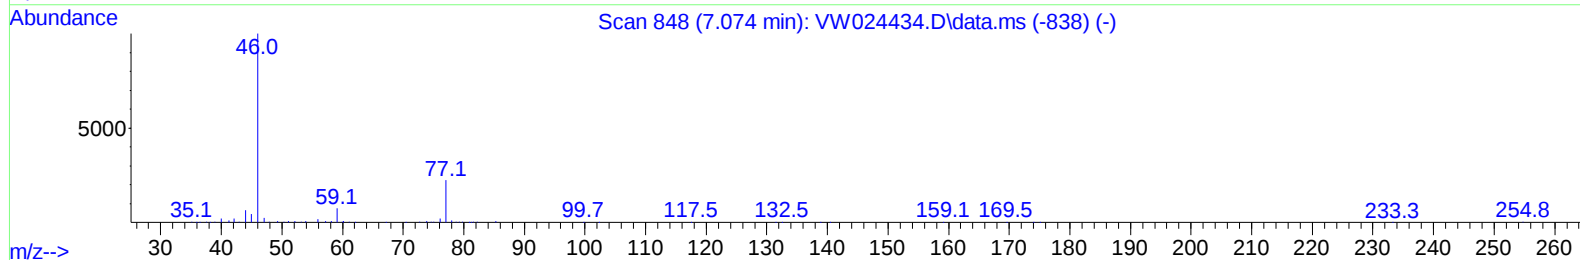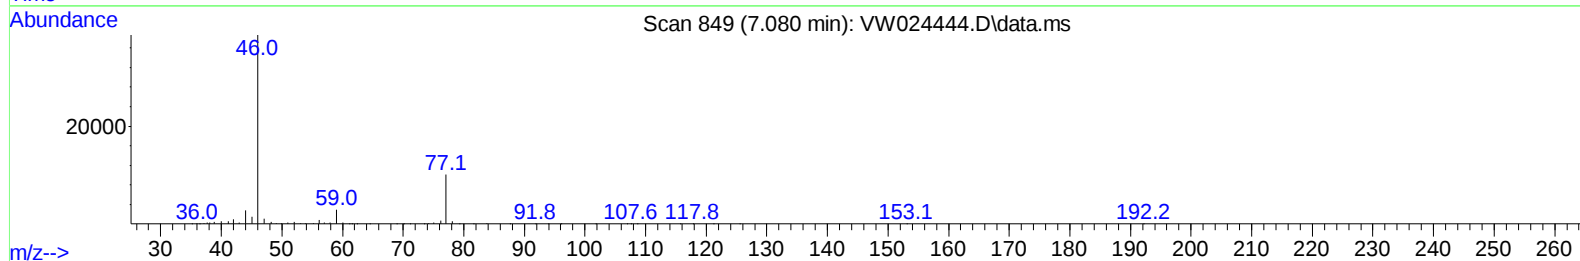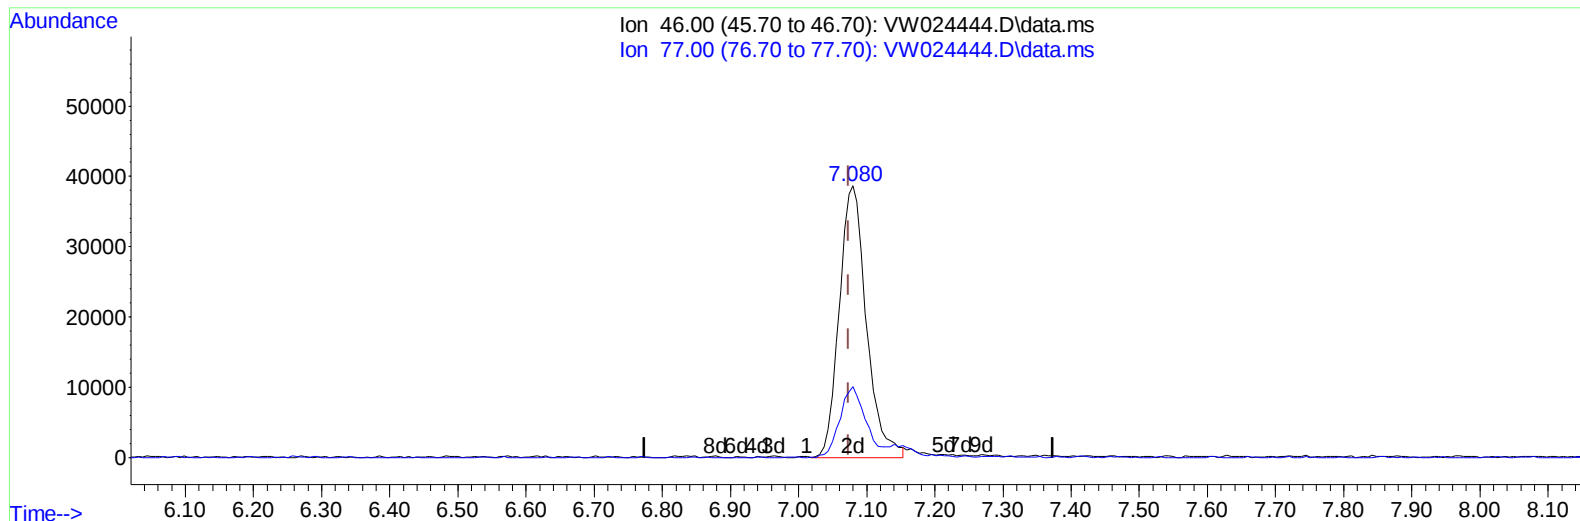

TIC: VW024444.D\data.ms

(21) 2-Butanone-d5 (S)

7.080min (+ 0.006) 54.12 ug/L m

response 107581

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	12.40	0.02#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024444.D
 Acq On : 29 Aug 2022 13:48
 Operator : SY/VA
 Sample : N4346-16
 Misc : 4.93g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVV4

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
 Supervised By :Mahesh Dadoda 08/31/2022

Quant Time: Aug 29 22:56:33 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Aug 29 22:53:57 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	391504	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	377277	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	169100	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	226672	21.003	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	84.000%	
7) Chloroethane-d5	2.873	69	165448	20.461	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	81.840%	
11) 1,1-Dichloroethene-d2	4.007	63	155377	16.601	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	66.400%	
21) 2-Butanone-d5	7.080	46	107581m	54.121	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	108.240%	
24) Chloroform-d	7.641	84	301844	23.982	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	95.920%	
26) 1,2-Dichloroethane-d4	8.305	65	185507	24.304	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	97.200%	
32) Benzene-d6	8.275	84	552784	25.573	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	102.280%	
36) 1,2-Dichloropropane-d6	9.274	67	175958	26.174	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	104.680%	
41) Toluene-d8	10.323	98	488521	23.770	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	95.080%	
43) trans-1,3-Dichloroprop...	10.579	79	75484	23.994	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	95.960%	
47) 2-Hexanone-d5	10.921	63	86929	57.784	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	115.560%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	184756	24.274	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	97.080%	
66) 1,2-Dichlorobenzene-d4	13.853	152	181606	28.519	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	114.080%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
Data File : VW024444.D
Acq On : 29 Aug 2022 13:48
Operator : SY/VA
Sample : N4346-16
Misc : 4.93g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBVV4

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
Supervised By :Mahesh Dadoda 08/31/2022

Quant Time: Aug 29 22:56:33 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Aug 29 22:53:57 2022
Response via : Initial Calibration

