




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
Data File : VW024451.D
Acq On : 29 Aug 2022 17:02
Operator : SY/VA
Sample : N4365-04
Misc : 5.71g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBVY2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
Supervised By :Mahesh Dadoda 08/31/2022

Quant Time: Aug 29 22:58:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Aug 29 22:53:57 2022
Response via : Initial Calibration

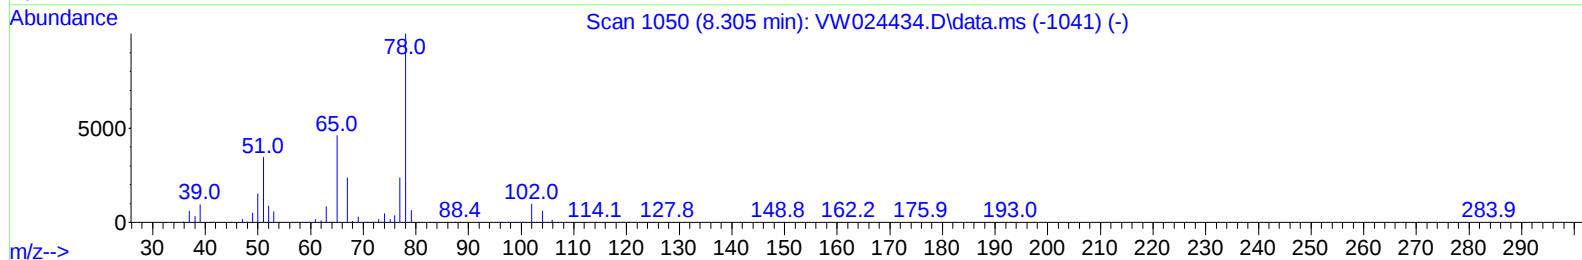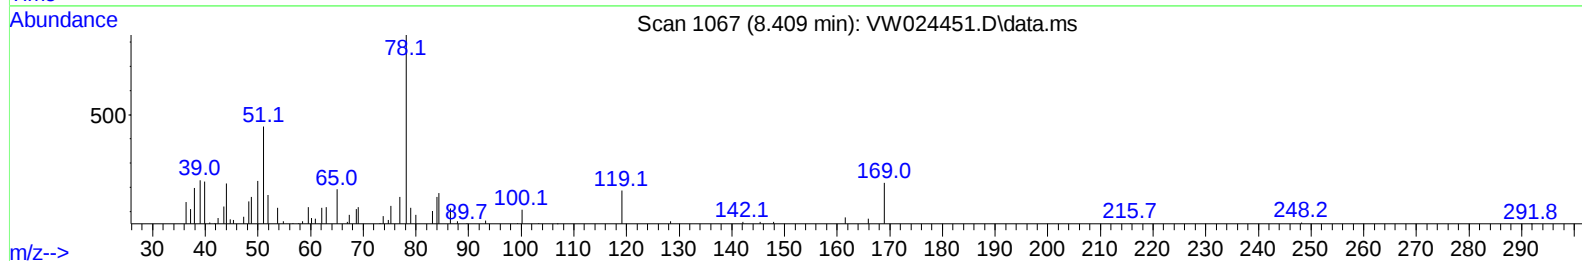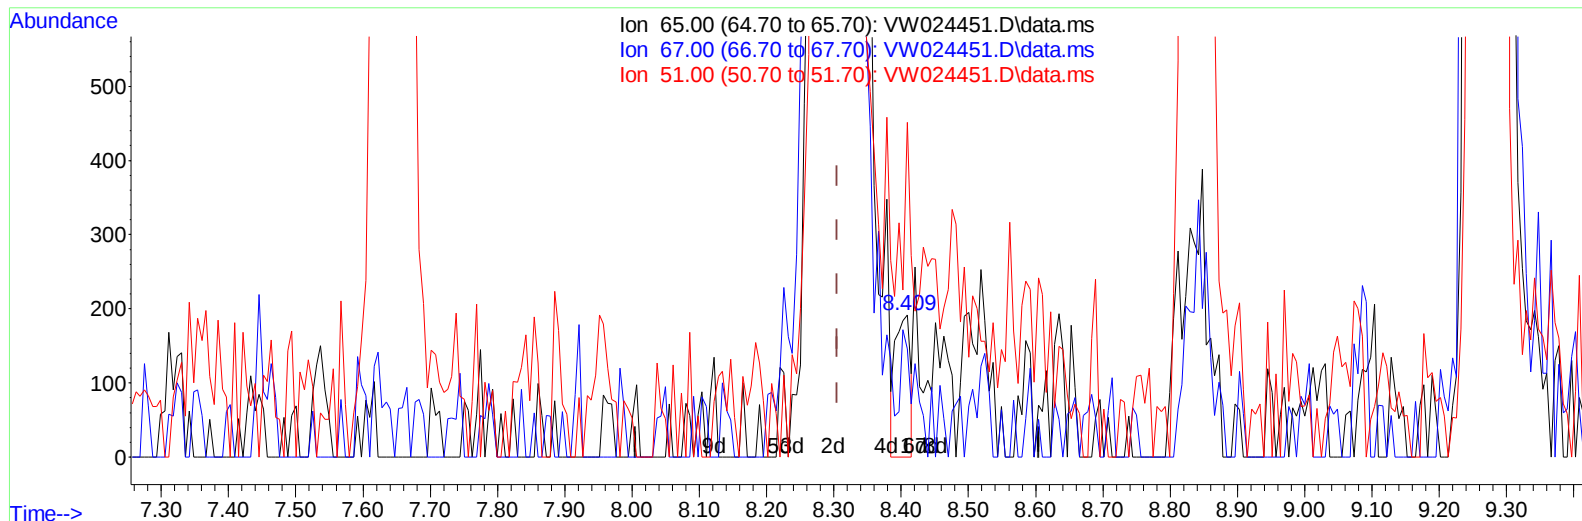

TIC: VW024451.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.409min (+ 0.104) 0.04 ug/L

response 298

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.10	55.37
51.00	96.50	87.25
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024451.D
 Acq On : 29 Aug 2022 17:02
 Operator : SY/VA
 Sample : N4365-04
 Misc : 5.71g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVY2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
 Supervised By :Mahesh Dadoda 08/31/2022

Quant Time: Aug 29 22:58:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Aug 29 22:53:57 2022
 Response via : Initial Calibration

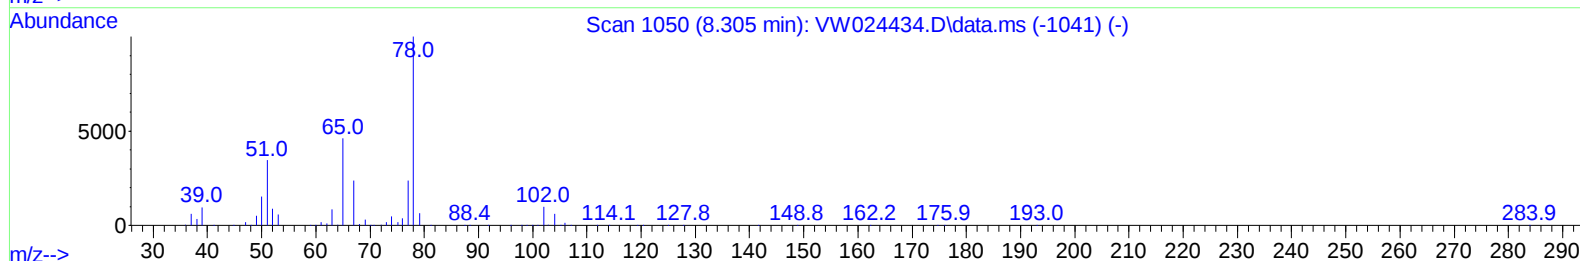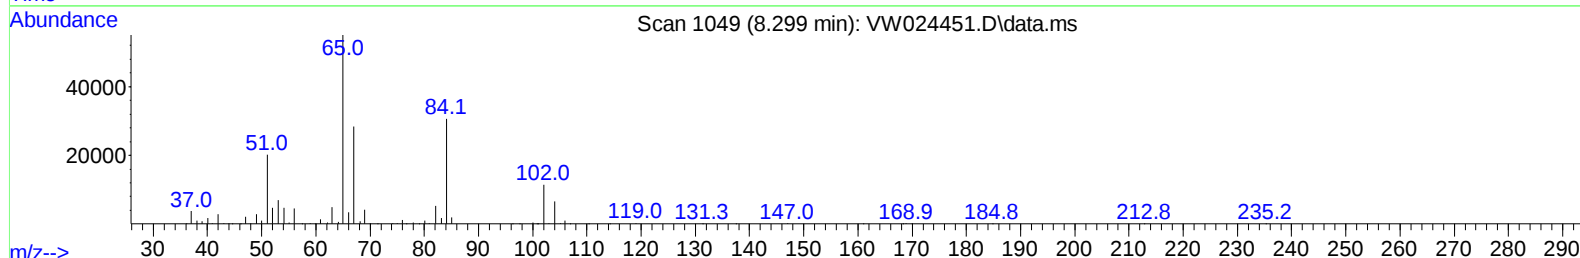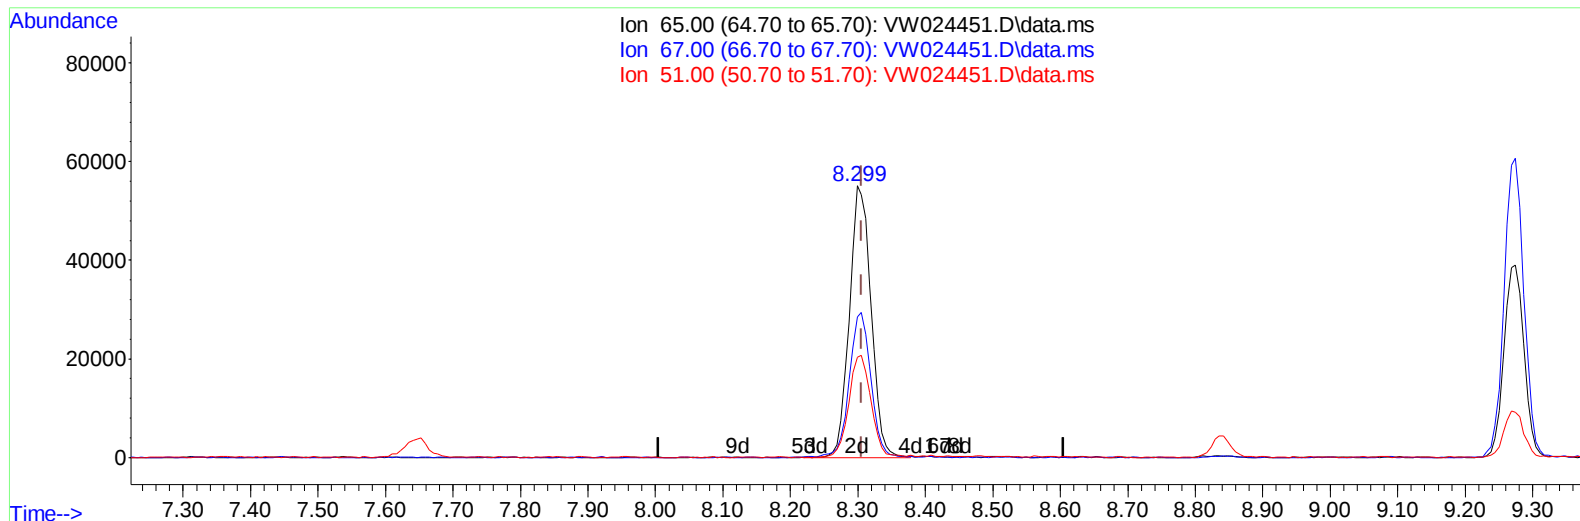

TIC: VW024451.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.299min (-0.006) 16.13 ug/L m

response 122540

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.10	0.13#
51.00	96.50	0.21#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024451.D
 Acq On : 29 Aug 2022 17:02
 Operator : SY/VA
 Sample : N4365-04
 Misc : 5.71g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVY2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
 Supervised By :Mahesh Dadoda 08/31/2022

Quant Time: Aug 29 22:58:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Aug 29 22:53:57 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	389729	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	370398	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	155975	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	198371	18.465	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	73.840%	
7) Chloroethane-d5	2.873	69	133544	16.591	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	66.360%	
11) 1,1-Dichloroethene-d2	4.001	63	144540	15.513	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110	Recovery	=	62.040%	
21) 2-Butanone-d5	7.080	46	56154	28.378	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	56.760%	
24) Chloroform-d	7.647	84	208289	16.624	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	66.480%	
26) 1,2-Dichloroethane-d4	8.299	65	122540m	16.127	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	64.520%#	
32) Benzene-d6	8.269	84	427911	20.163	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	80.640%	
36) 1,2-Dichloropropane-d6	9.275	67	123632	18.732	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	74.920%	
41) Toluene-d8	10.323	98	390311	19.344	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	77.360%	
43) trans-1,3-Dichloroprop...	10.579	79	49771	16.115	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	64.440%	
47) 2-Hexanone-d5	10.921	63	45635	30.898	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	61.800%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	103991	13.917	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	55.680%	
66) 1,2-Dichlorobenzene-d4	13.853	152	120724	20.554	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	82.200%	
Target Compounds						
					Qvalue	
13) Acetone	4.123	43	11105	9.404	ug/L	88
34) Trichloroethene	9.092	95	2851	0.469	ug/L	90
46) Tetrachloroethene	10.860	164	20558	4.355	ug/L	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
Data File : VW024451.D
Acq On : 29 Aug 2022 17:02
Operator : SY/VA
Sample : N4365-04
Misc : 5.71g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBVY2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
Supervised By :Mahesh Dadoda 08/31/2022

Quant Time: Aug 29 22:58:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Aug 29 22:53:57 2022
Response via : Initial Calibration

