




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024464.D
 Acq On : 29 Aug 2022 22:59
 Operator : SY/VA
 Sample : N4344-06
 Misc : 4.62g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVQ5

Manual IntegrationsAPPROVED

Quant Time: Aug 30 00:26:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 30 00:24:06 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/30/2022
 Supervised By :Mahesh Dadoda 08/31/2022

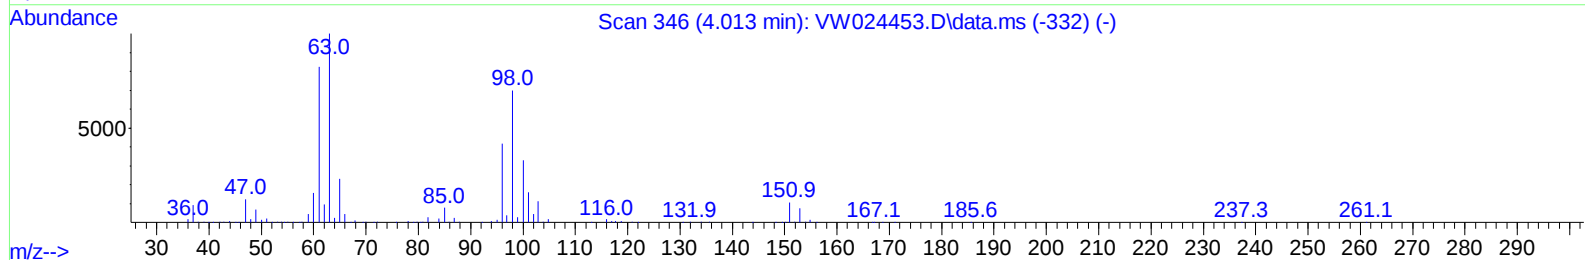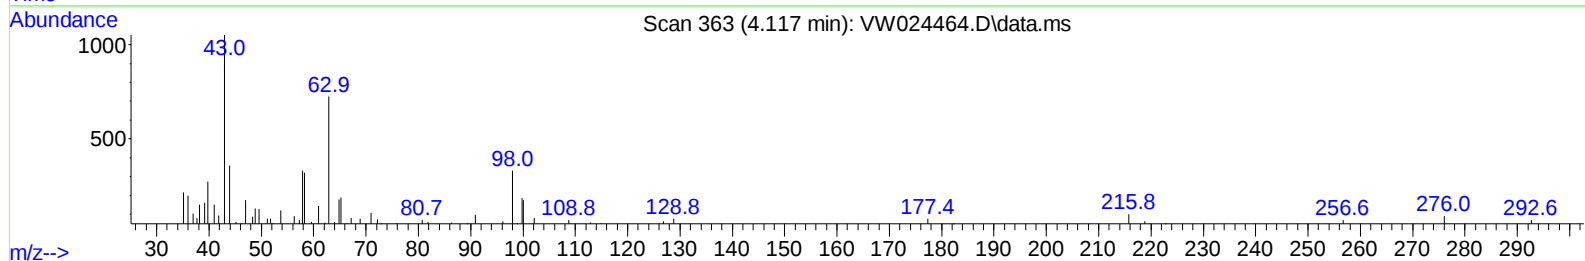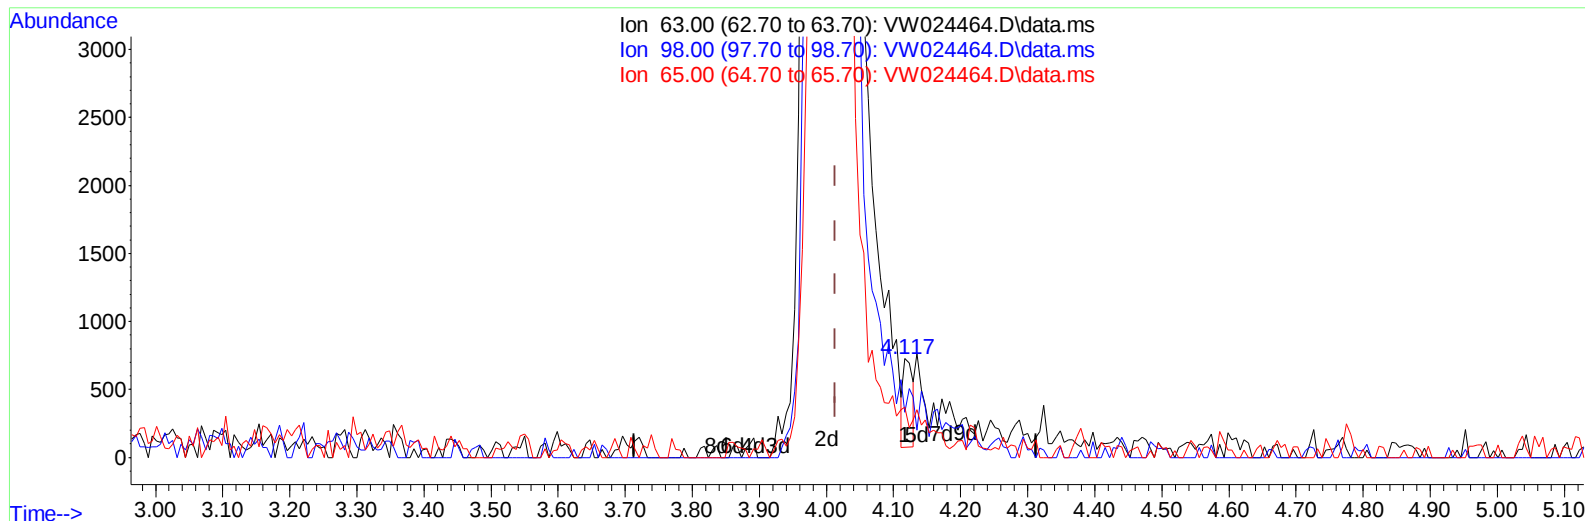

TIC: VW024464.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.117min (+ 0.104) 0.06 ug/L

response 641

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	70.50	65.68
65.00	22.70	26.05
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
Data File : VW024464.D
Acq On : 29 Aug 2022 22:59
Operator : SY/VA
Sample : N4344-06
Misc : 4.62g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBVQ5

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
Supervised By :Mahesh Dadoda 08/31/2022

Quant Time: Aug 30 00:26:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Aug 30 00:24:06 2022
Response via : Initial Calibration

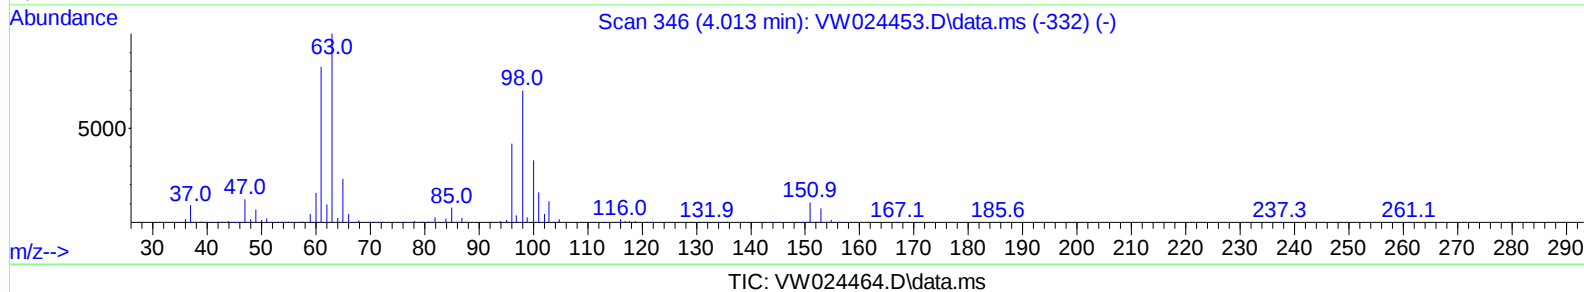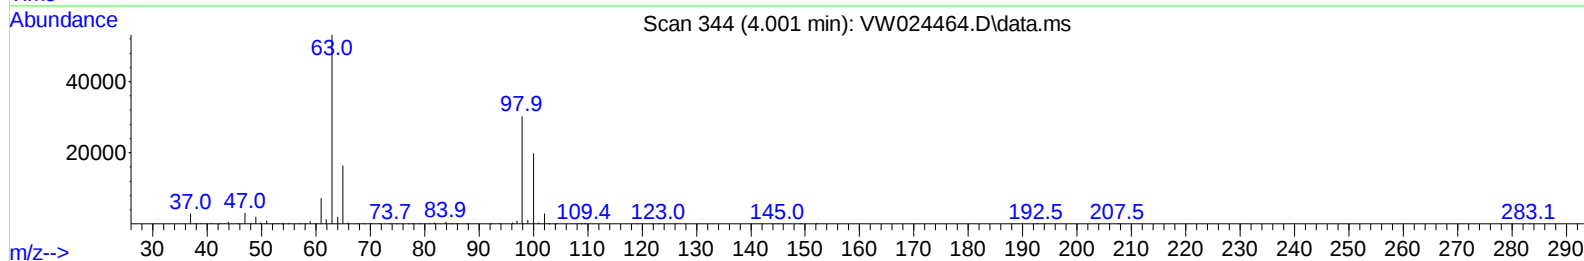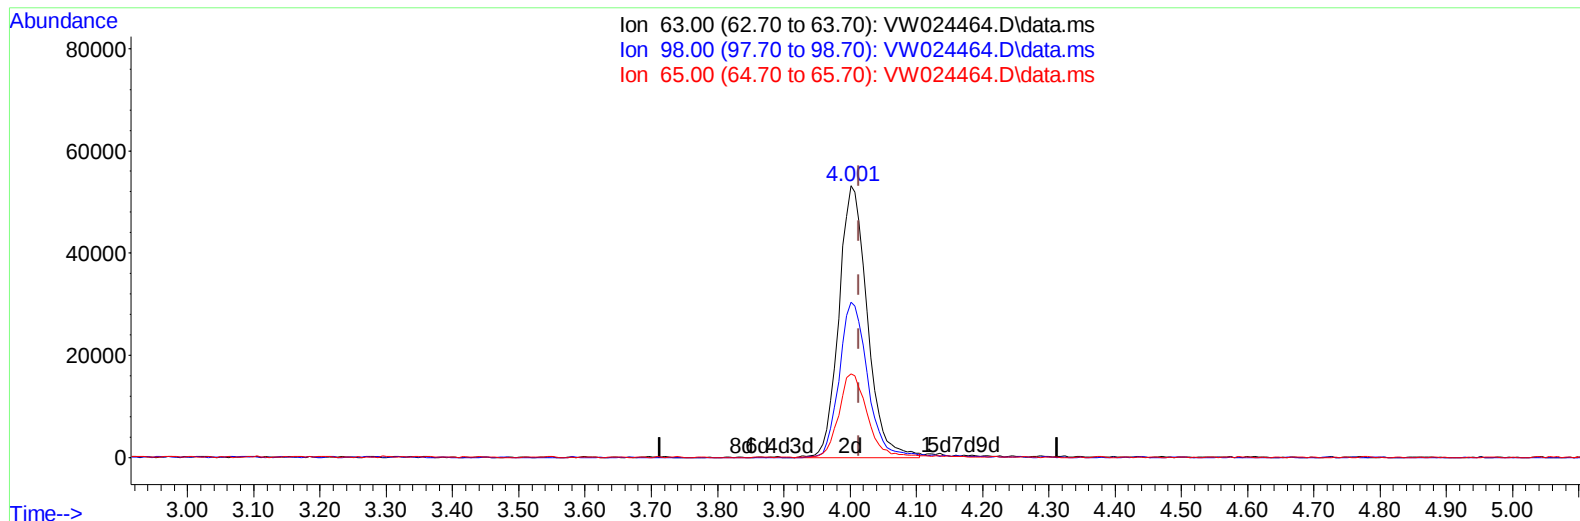

(11) 1,1-Dichloroethene-d2 (S)

4.001min (-0.012) 15.77 ug/L m

response 158469

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	70.50	0.27#
65.00	22.70	0.11#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024464.D
 Acq On : 29 Aug 2022 22:59
 Operator : SY/VA
 Sample : N4344-06
 Misc : 4.62g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVQ5

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
 Supervised By :Mahesh Dadoda 08/31/2022

Quant Time: Aug 30 00:26:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 30 00:24:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	420354	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	398649	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	179324	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.337	65	219631	18.954	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	75.800%	
7) Chloroethane-d5	2.873	69	136872	15.765	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	63.080%	
11) 1,1-Dichloroethene-d2	4.001	63	158469m	15.769	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110	Recovery	=	63.080%	
21) 2-Butanone-d5	7.074	46	64110	30.038	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	60.080%	
24) Chloroform-d	7.647	84	251182	18.587	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	74.360%	
26) 1,2-Dichloroethane-d4	8.299	65	141082	17.215	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	68.840%#	
32) Benzene-d6	8.269	84	480719	21.047	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	84.200%	
36) 1,2-Dichloropropane-d6	9.268	67	139599	19.652	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	78.600%	
41) Toluene-d8	10.323	98	449870	20.716	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	82.880%	
43) trans-1,3-Dichloroprop...	10.573	79	55238	16.617	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	66.480%	
47) 2-Hexanone-d5	10.921	63	52815	33.226	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	66.460%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	120009	14.922	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	59.680%	
66) 1,2-Dichlorobenzene-d4	13.847	152	141205	20.910	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	83.640%	
Target Compounds						
						Qvalue
25) Chloroform	7.671	83	7900	0.634	ug/L	83
34) Trichloroethene	9.092	95	3666	0.560	ug/L	89
46) Tetrachloroethene	10.860	164	1052652	207.195	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
Data File : VW024464.D
Acq On : 29 Aug 2022 22:59
Operator : SY/VA
Sample : N4344-06
Misc : 4.62g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBVQ5

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
Supervised By :Mahesh Dadoda 08/31/2022

Quant Time: Aug 30 00:26:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Aug 30 00:24:06 2022
Response via : Initial Calibration

