




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
Data File : VW024466.D
Acq On : 29 Aug 2022 23:48
Operator : SY/VA
Sample : N4344-12
Misc : 5.19g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBVR1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
Supervised By :Mahesh Dadoda 08/31/2022

Quant Time: Aug 30 00:26:46 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Aug 30 00:24:06 2022
Response via : Initial Calibration

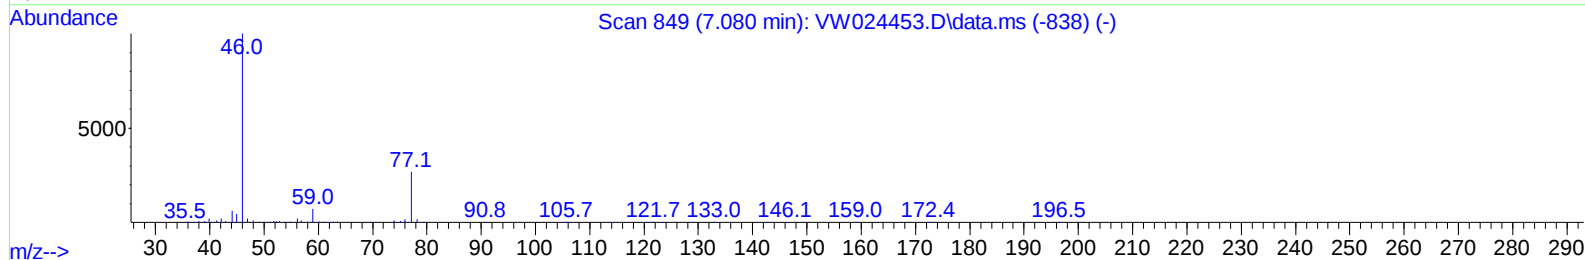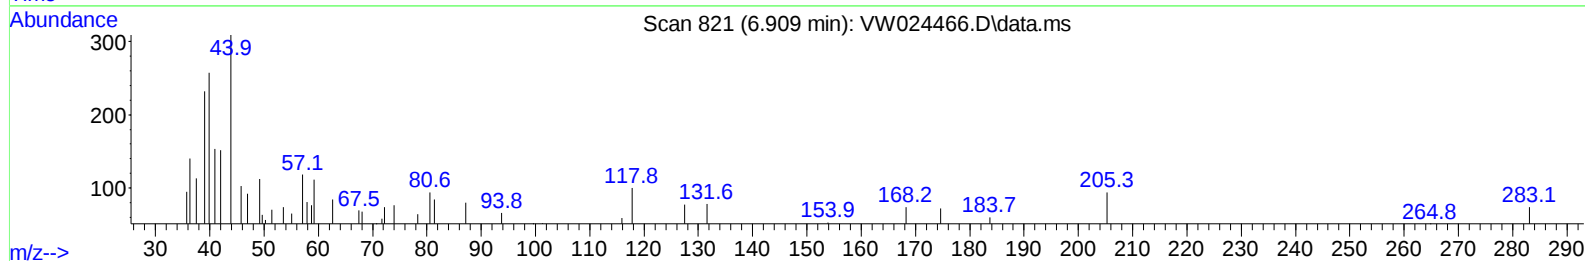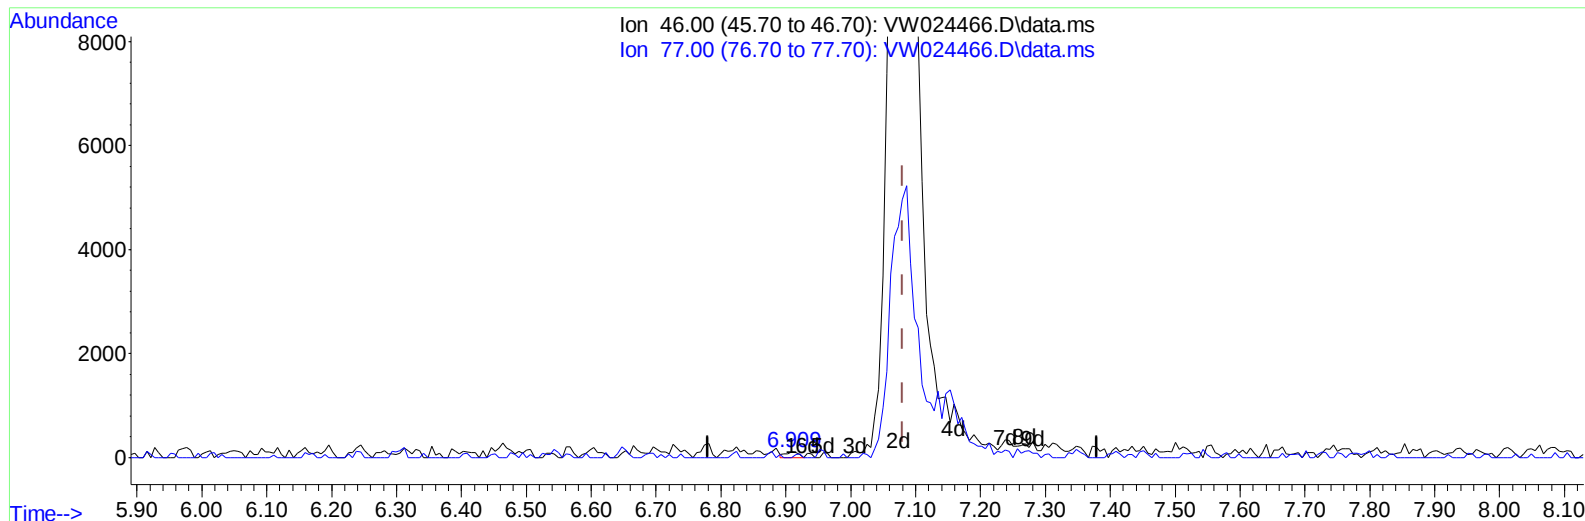

TIC: VW024466.D\data.ms

(21) 2-Butanone-d5 (S)

6.909min (-0.171) 0.08 ug/L

response 142

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	12.40	14.79
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024466.D
 Acq On : 29 Aug 2022 23:48
 Operator : SY/VA
 Sample : N4344-12
 Misc : 5.19g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVR1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
 Supervised By :Mahesh Dadoda 08/31/2022

Quant Time: Aug 30 00:26:46 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 30 00:24:06 2022
 Response via : Initial Calibration

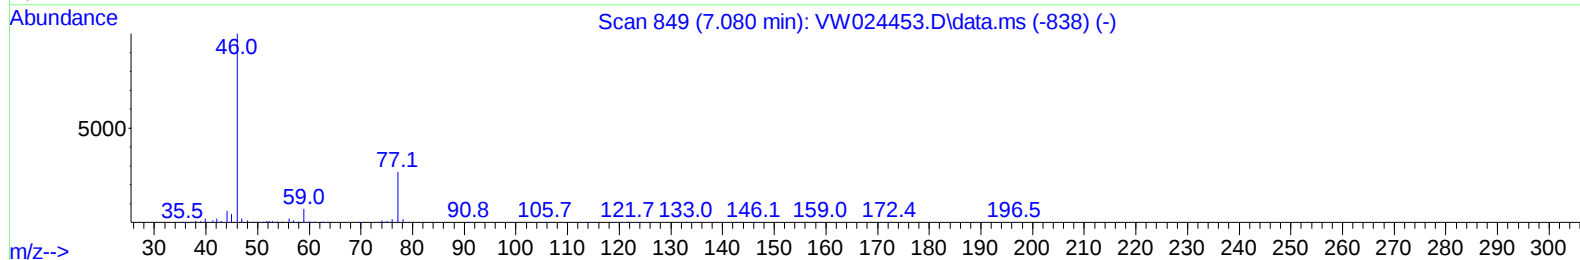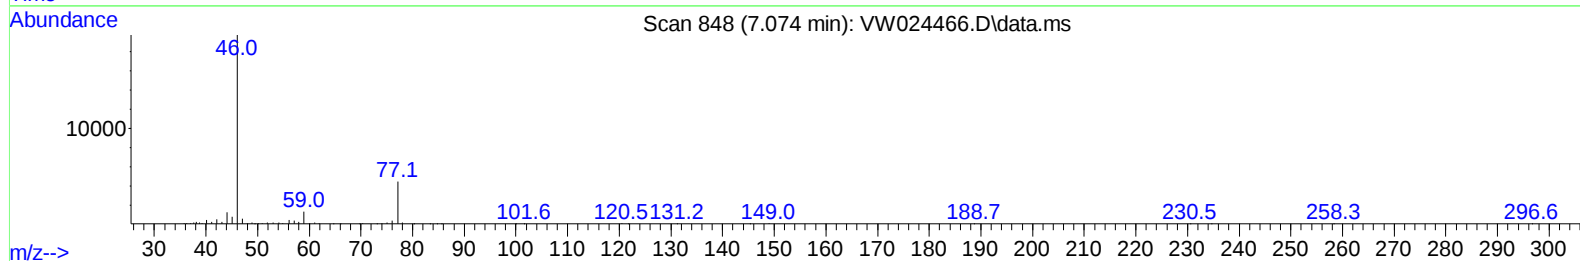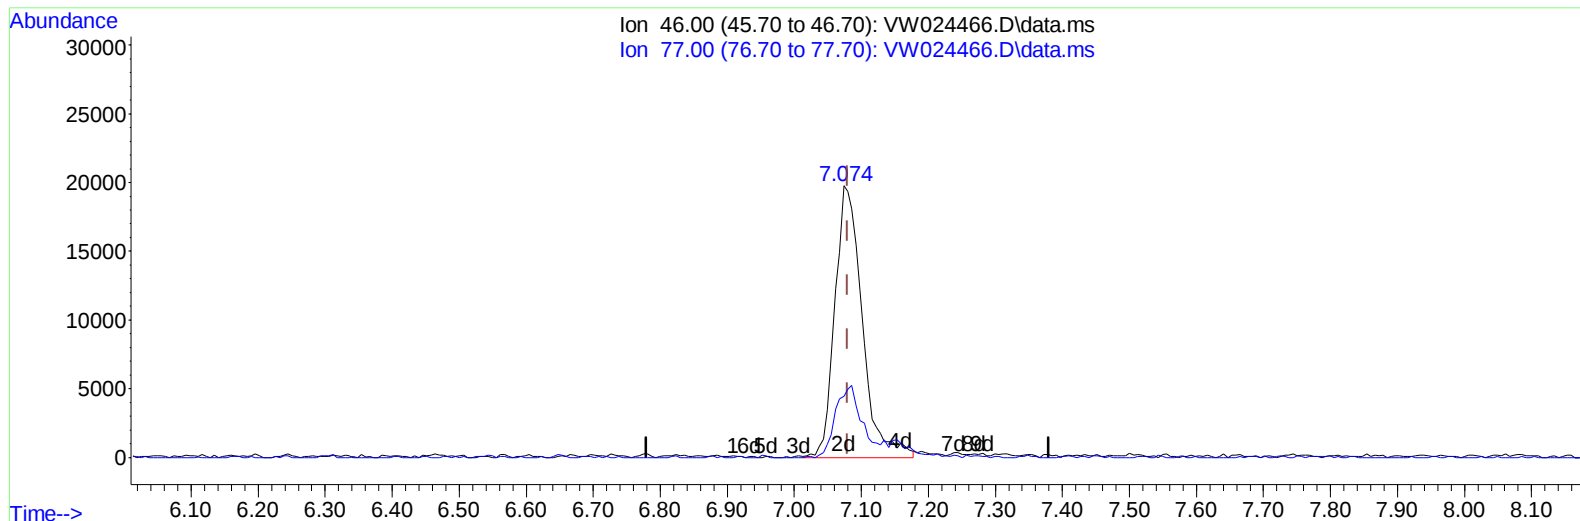

TIC: VW024466.D\data.ms

(21) 2-Butanone-d5 (S)

7.074min (-0.006) 30.35 ug/L m

response 55864

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	12.40	0.04#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024466.D
 Acq On : 29 Aug 2022 23:48
 Operator : SY/VA
 Sample : N4344-12
 Misc : 5.19g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVR1

Manual IntegrationsAPPROVED

Quant Time: Aug 30 00:26:46 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 30 00:24:06 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/30/2022
 Supervised By :Mahesh Dadoda 08/31/2022

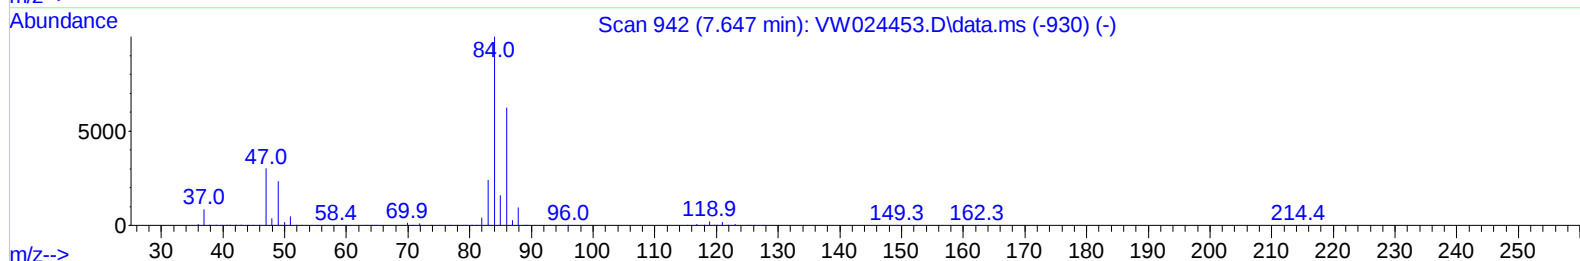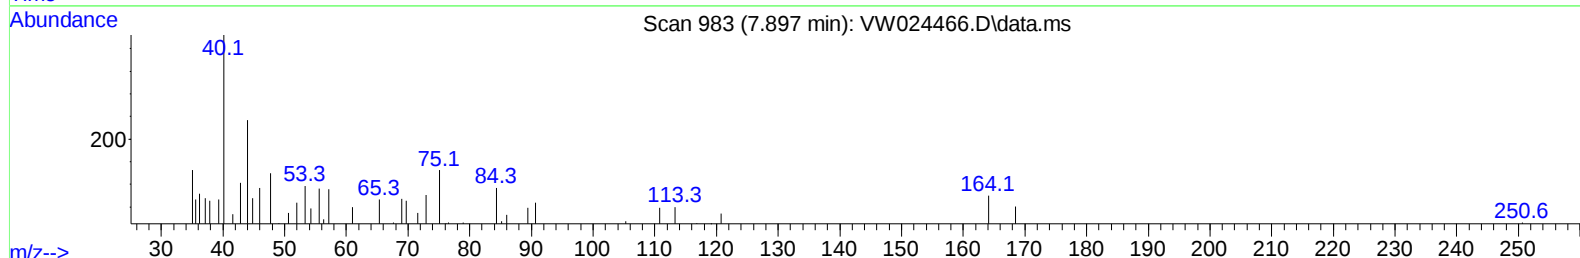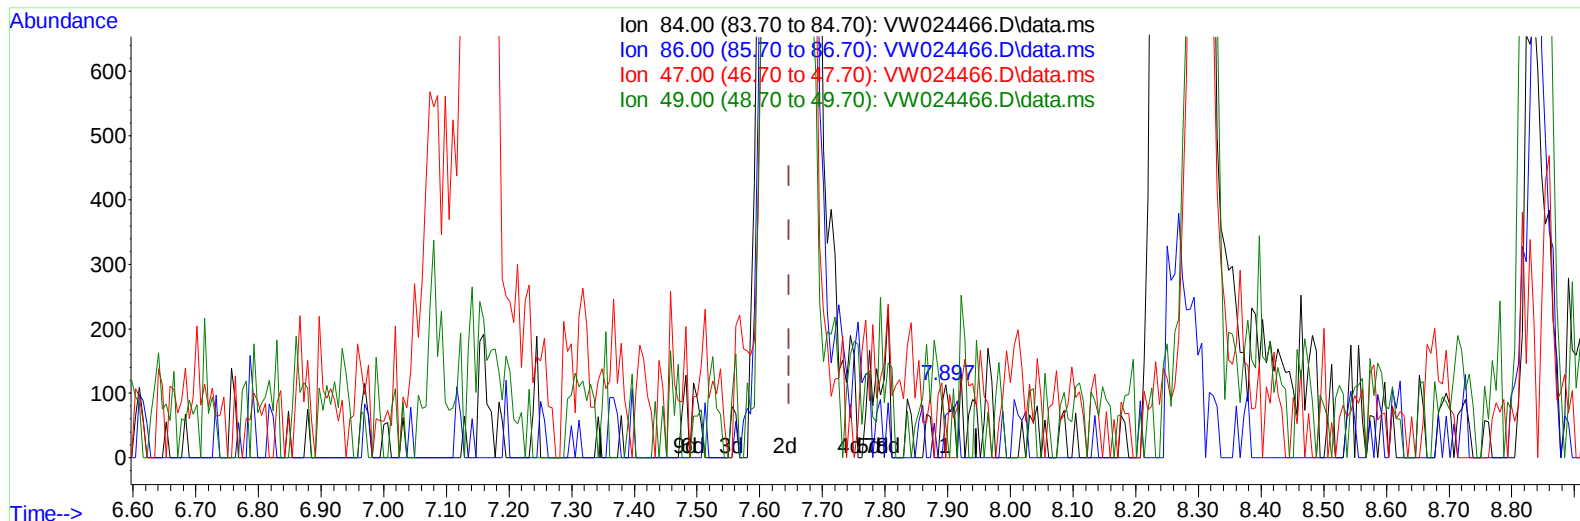

TIC: VW024466.D\data.ms

(24) Chloroform-d (S)

7.897min (+ 0.250) 0.01 ug/L

response 126

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.30	46.83
47.00	49.80	46.03
49.00	30.40	30.95




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024466.D
 Acq On : 29 Aug 2022 23:48
 Operator : SY/VA
 Sample : N4344-12
 Misc : 5.19g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVR1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
 Supervised By :Mahesh Dadoda 08/31/2022

Quant Time: Aug 30 00:26:46 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 30 00:24:06 2022
 Response via : Initial Calibration

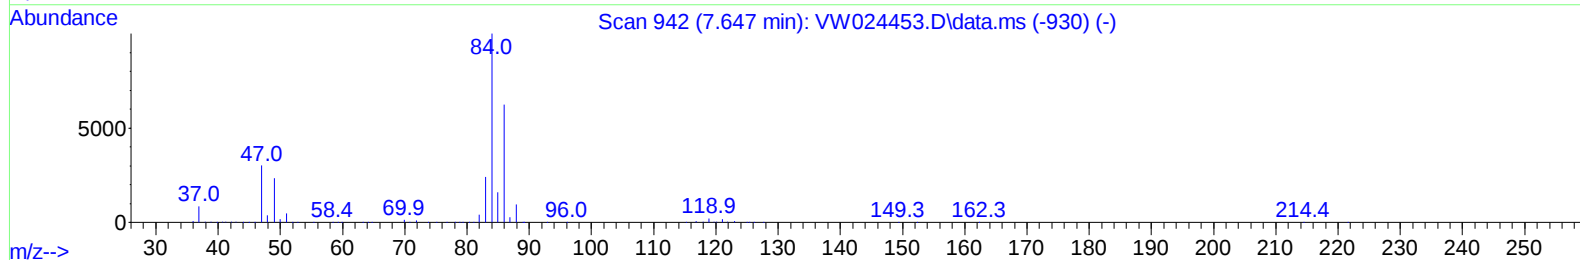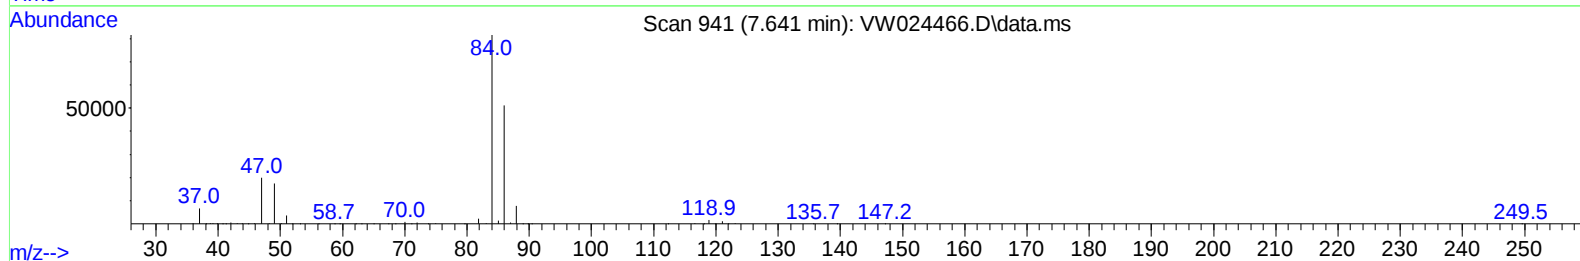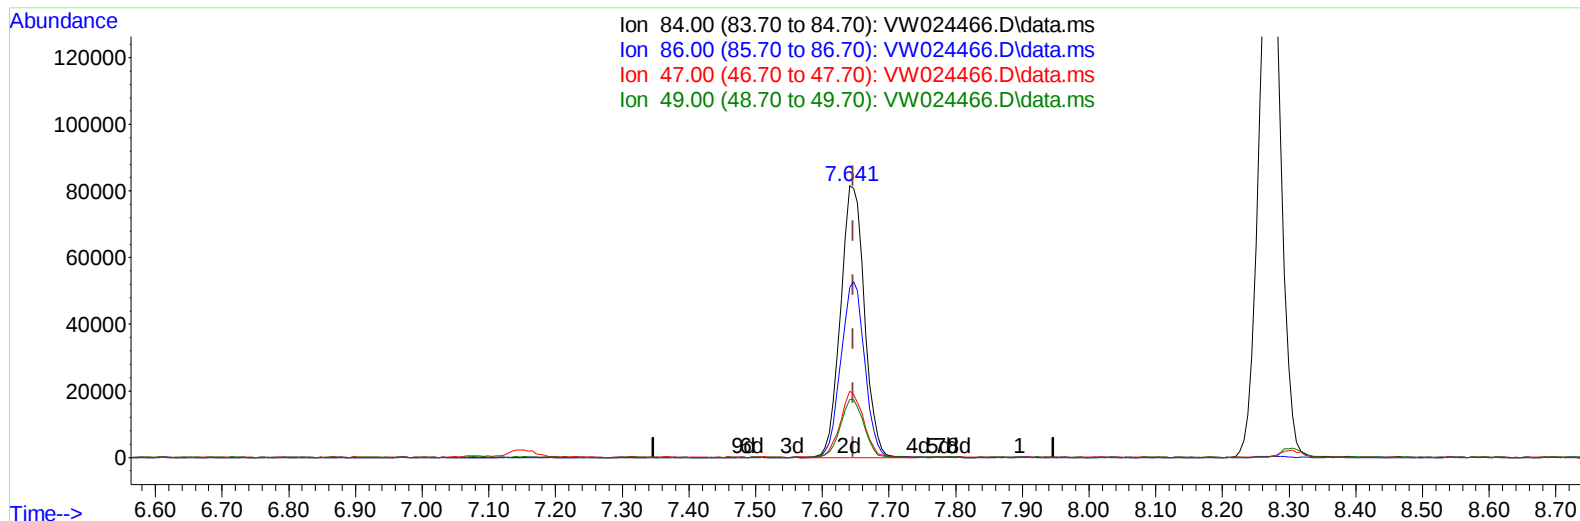

TIC: VW024466.D\data.ms

(24) Chloroform-d (S)

7.641min (-0.006) 17.33 ug/L m

response 202030

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.30	0.03#
47.00	49.80	0.03#
49.00	30.40	0.02#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024466.D
 Acq On : 29 Aug 2022 23:48
 Operator : SY/VA
 Sample : N4344-12
 Misc : 5.19g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVR1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
 Supervised By :Mahesh Dadoda 08/31/2022

Quant Time: Aug 30 00:26:46 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 30 00:24:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	362578	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	338496	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	147997	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.337	65	180675	18.077	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	72.320%	
7) Chloroethane-d5	2.873	69	108916	14.544	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	58.160%	
11) 1,1-Dichloroethene-d2	4.007	63	130795	15.089	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	60.360%	
21) 2-Butanone-d5	7.074	46	55864m	30.346	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	60.700%	
24) Chloroform-d	7.641	84	202030m	17.332	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	69.320%	
26) 1,2-Dichloroethane-d4	8.299	65	118046	16.699	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	66.800%#	
32) Benzene-d6	8.269	84	388461	20.030	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	80.120%	
36) 1,2-Dichloropropane-d6	9.274	67	116151	19.257	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	77.040%	
41) Toluene-d8	10.323	98	360548	19.553	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	78.200%	
43) trans-1,3-Dichloroprop...	10.573	79	45154	15.998	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	64.000%	
47) 2-Hexanone-d5	10.921	63	45487	33.701	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	67.400%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	106710	15.626	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	62.520%	
66) 1,2-Dichlorobenzene-d4	13.853	152	114251	20.500	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	82.000%	
Target Compounds					Qvalue	
13) Acetone	4.123	43	4479	4.077	ug/L	93
46) Tetrachloroethene	10.860	164	96677	22.411	ug/L	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
Data File : VW024466.D
Acq On : 29 Aug 2022 23:48
Operator : SY/VA
Sample : N4344-12
Misc : 5.19g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBVR1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
Supervised By :Mahesh Dadoda 08/31/2022

Quant Time: Aug 30 00:26:46 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Aug 30 00:24:06 2022
Response via : Initial Calibration

