




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
Data File : VW024478.D
Acq On : 30 Aug 2022 06:22
Operator : SY/VA
Sample : N4365-09
Misc : 6.14g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBVY7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
Supervised By :Mahesh Dadoda 08/31/2022

Quant Time: Aug 30 07:08:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Aug 30 07:05:43 2022
Response via : Initial Calibration

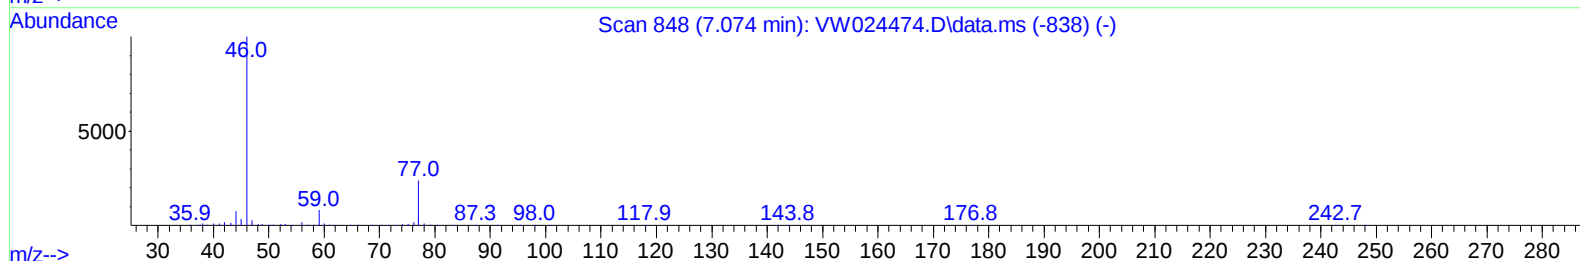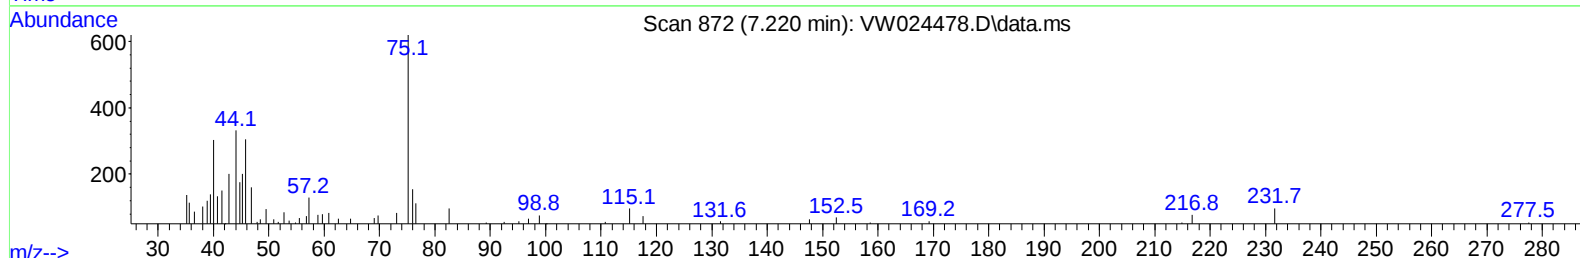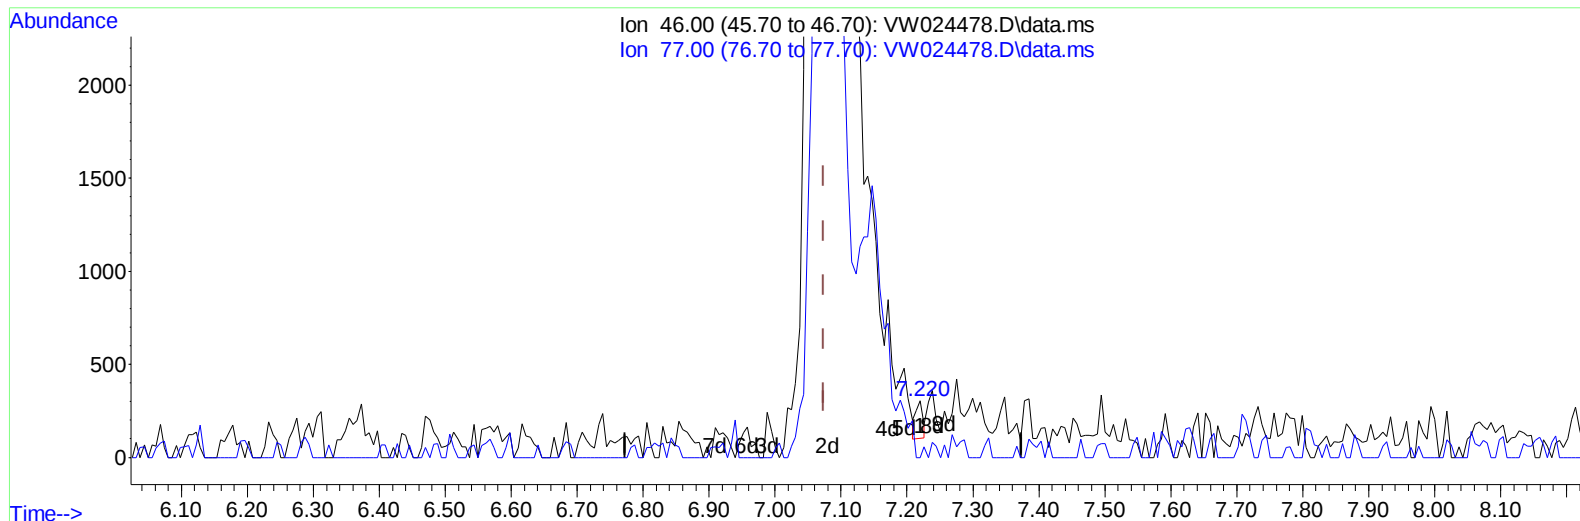

TIC: VW024478.D\data.ms

(21) 2-Butanone-d5 (S)

7.220min (+ 0.147) 0.09 ug/L

response 158

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	12.40	12.66
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024478.D
 Acq On : 30 Aug 2022 06:22
 Operator : SY/VA
 Sample : N4365-09
 Misc : 6.14g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVY7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
 Supervised By :Mahesh Dadoda 08/31/2022

Quant Time: Aug 30 07:08:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 30 07:05:43 2022
 Response via : Initial Calibration

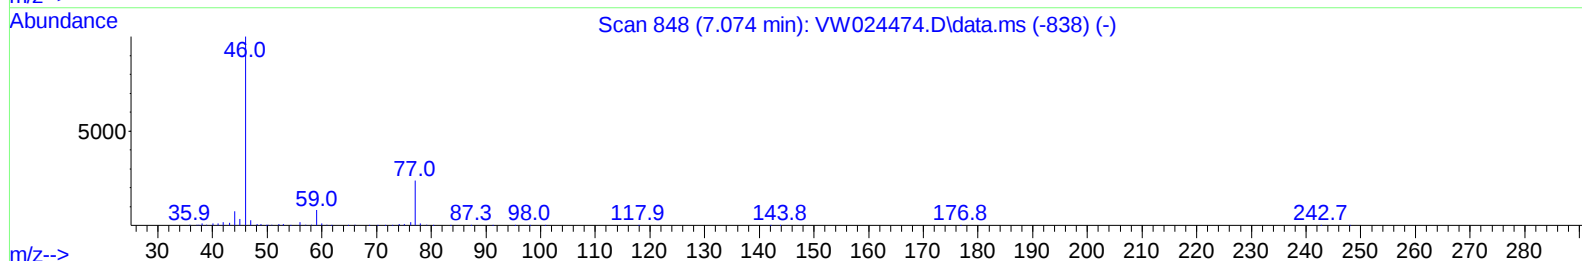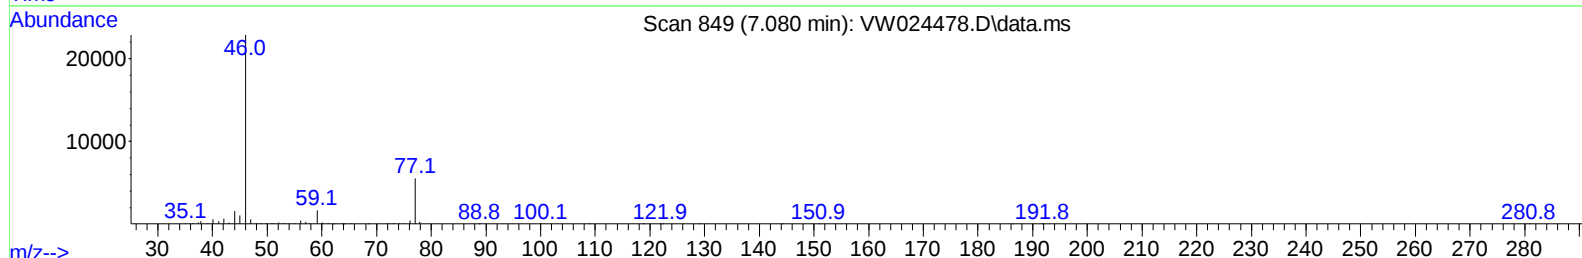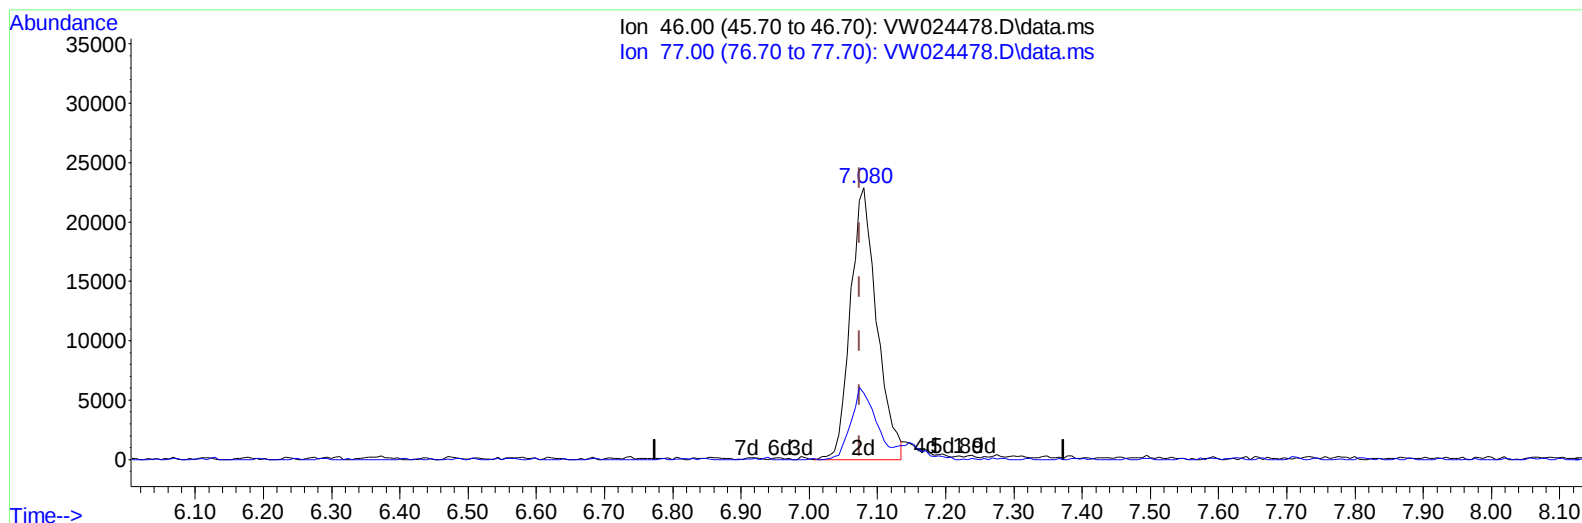

TIC: VW024478.D\data.ms

(21) 2-Butanone-d5 (S)

7.080min (+ 0.006) 34.24 ug/L m

response 61290

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	12.40	0.03#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024478.D
 Acq On : 30 Aug 2022 06:22
 Operator : SY/VA
 Sample : N4365-09
 Misc : 6.14g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVY7

Manual IntegrationsAPPROVED

Quant Time: Aug 30 07:08:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 30 07:05:43 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/30/2022
 Supervised By :Mahesh Dadoda 08/31/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	352534	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	335700	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	151053	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	163468	16.821	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	67.280%	
7) Chloroethane-d5	2.873	69	113590	15.601	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	62.400%	
11) 1,1-Dichloroethene-d2	4.013	63	132528	15.725	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	62.880%	
21) 2-Butanone-d5	7.080	46	61290m	34.242	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	68.480%	
24) Chloroform-d	7.647	84	201713	17.798	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	71.200%	
26) 1,2-Dichloroethane-d4	8.305	65	117809	17.141	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	68.560%#	
32) Benzene-d6	8.275	84	392010	20.381	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	81.520%	
36) 1,2-Dichloropropane-d6	9.275	67	116194	19.425	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	77.680%	
41) Toluene-d8	10.323	98	362546	19.825	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	79.280%	
43) trans-1,3-Dichloroprop...	10.579	79	43246	15.449	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	61.800%	
47) 2-Hexanone-d5	10.921	63	48389	36.149	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	72.300%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	111272	16.430	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	65.720%	
66) 1,2-Dichlorobenzene-d4	13.853	152	116492	20.479	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	81.920%	
Target Compounds						
46) Tetrachloroethene	10.860	164	88304	20.640	ug/L	Qvalue 94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
Data File : VW024478.D
Acq On : 30 Aug 2022 06:22
Operator : SY/VA
Sample : N4365-09
Misc : 6.14g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBVY7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
Supervised By :Mahesh Dadoda 08/31/2022

Quant Time: Aug 30 07:08:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Aug 30 07:05:43 2022
Response via : Initial Calibration

