

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024480.D
 Acq On : 30 Aug 2022 07:11
 Operator : SY/VA
 Sample : N4365-11
 Misc : 5.42g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 DBVY9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/31/2022
 Supervised By :Mahesh Dadoda 08/31/2022

Quant Time: Aug 31 01:18:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 30 07:05:43 2022
 Response via : Initial Calibration

08/31/2022
 Supervised By :Mahesh
 Dadoda
 08/31/2022

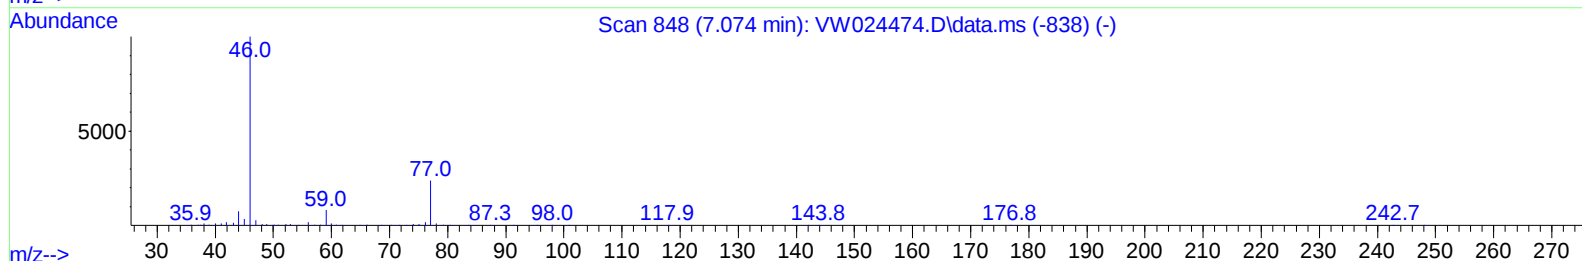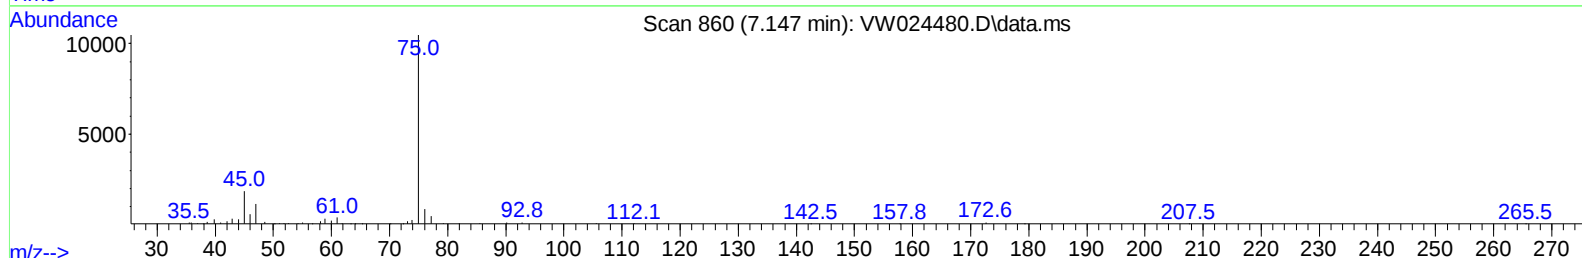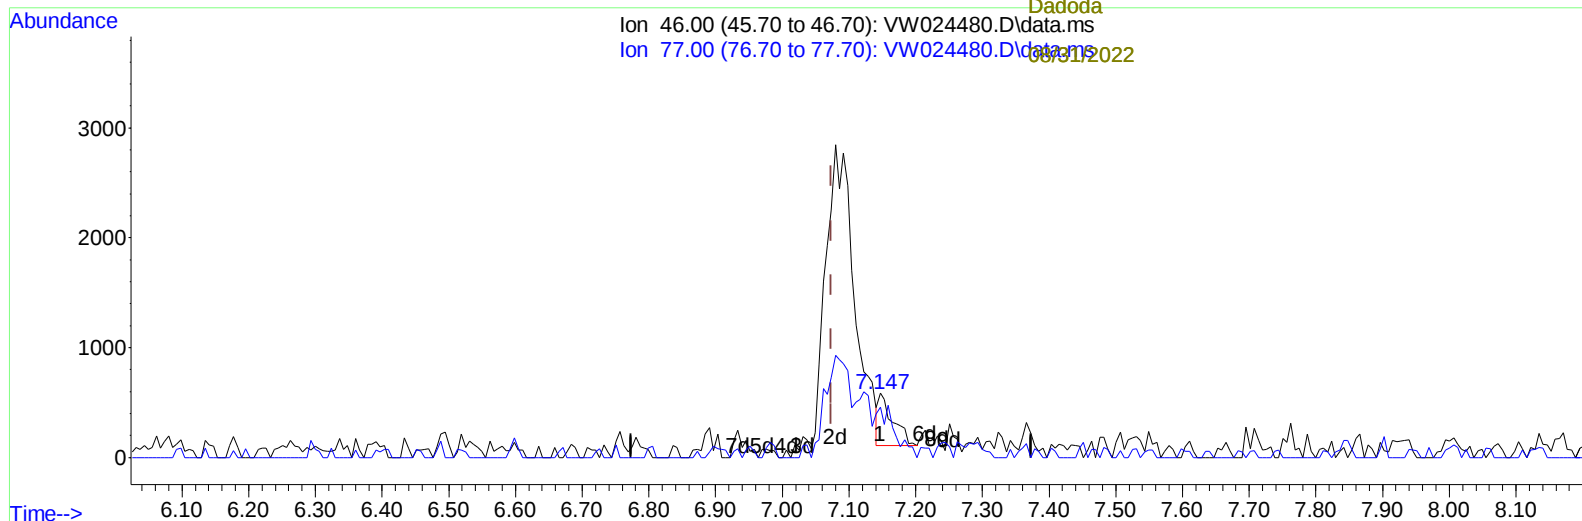

TIC: VW024480.D\data.ms

(21) 2-Butanone-d5 (S)

7.147min (+ 0.073) 4.89 ug/L

response 713

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	12.40	15.99
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024480.D
 Acq On : 30 Aug 2022 07:11
 Operator : SY/VA
 Sample : N4365-11
 Misc : 5.42g/10mL/MSVOA_W/SoIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 DBVY9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/31/2022
 Supervised By :Mahesh Dadoda 08/31/2022

Quant Time: Aug 31 01:18:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 30 07:05:43 2022
 Response via : Initial Calibration

08/31/2022
 Supervised By :Mahesh
 Dadoda
 08/31/2022

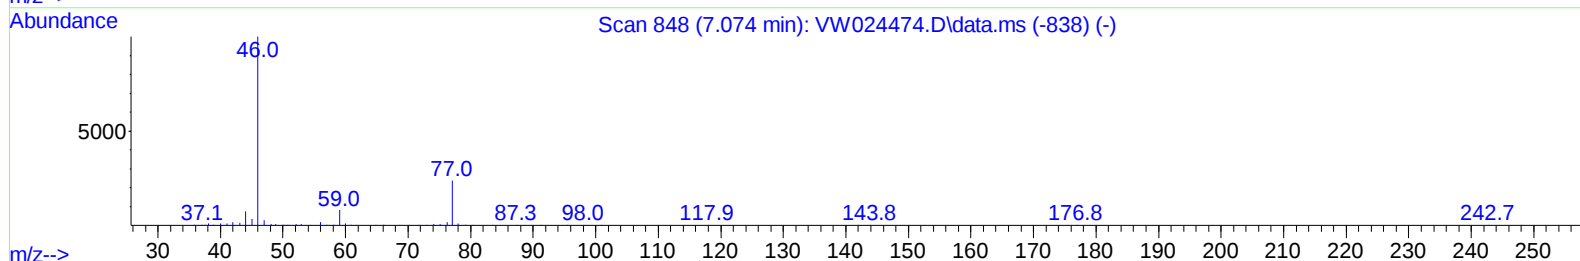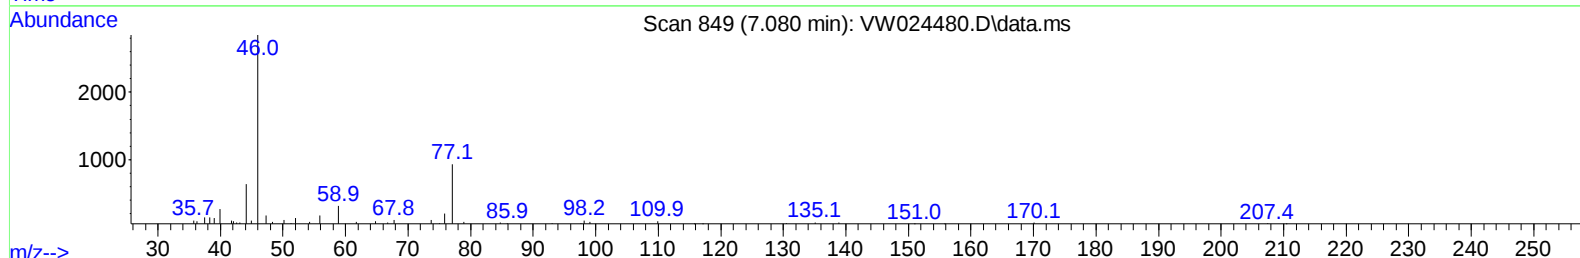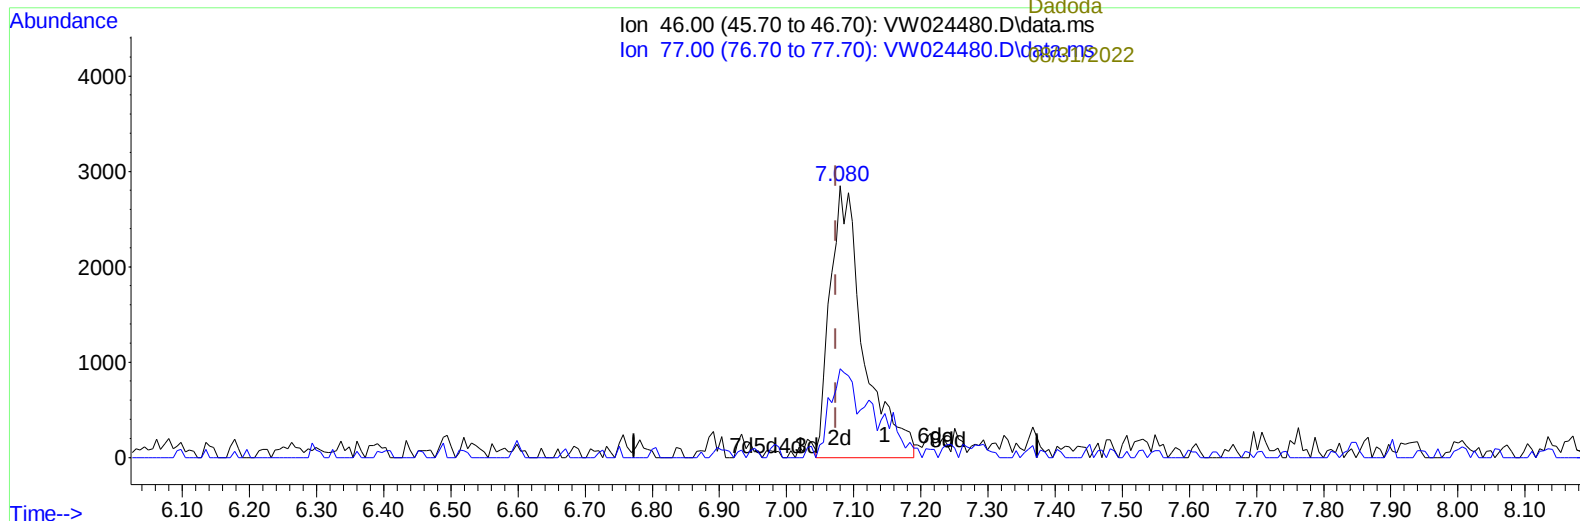

TIC: VW024480.D\data.ms

(21) 2-Butanone-d5 (S)

7.080min (+ 0.006) 67.03 ug/L m

response 9774

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	12.40	1.17#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024480.D
 Acq On : 30 Aug 2022 07:11
 Operator : SY/VA
 Sample : N4365-11
 Misc : 5.42g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 DBVY9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/31/2022
 Supervised By :Mahesh Dadoda 08/31/2022

08/31/2022
 Supervised By :Mahesh
 Dadoda

Quant Time: Aug 31 01:18:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 30 07:05:43 2022
 Response via : Initial Calibration

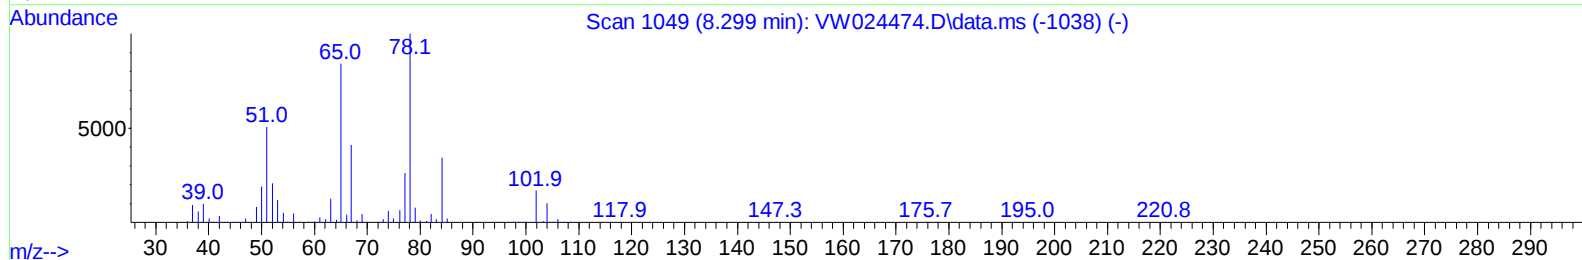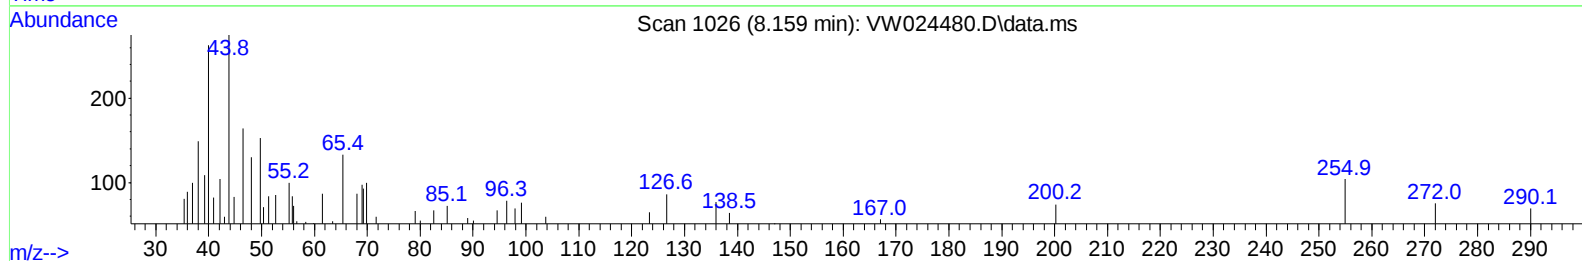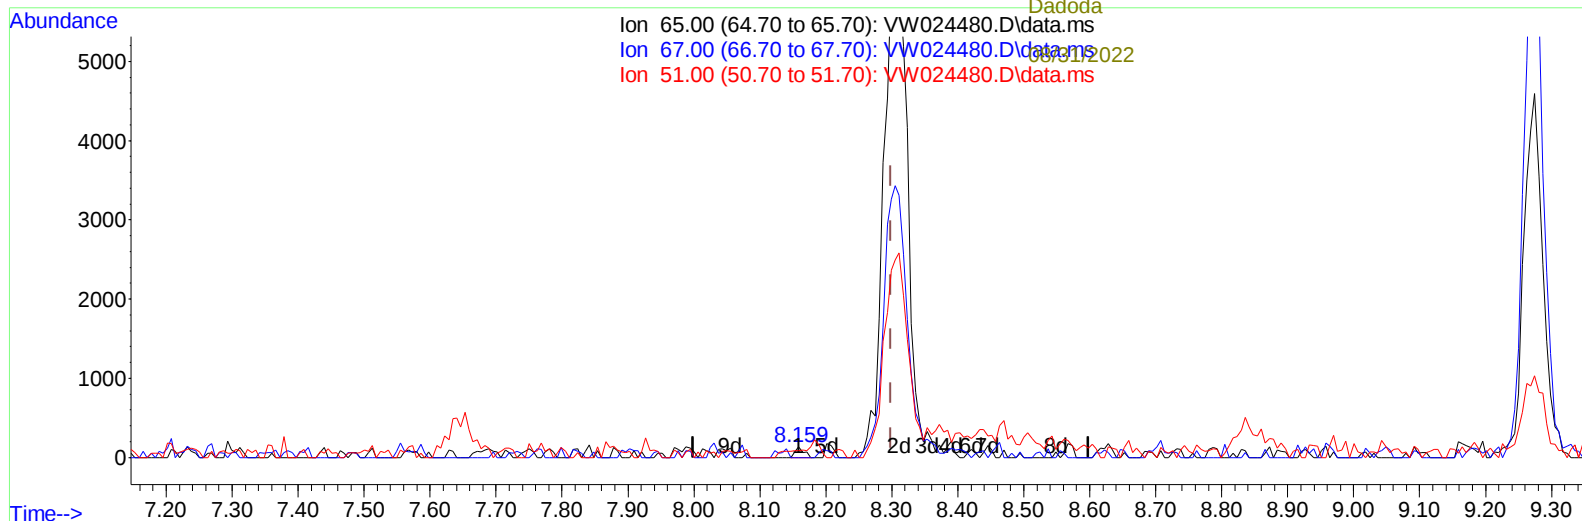

TIC: VW024480.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.159min (-0.140) 0.22 ug/L

response 123

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.10	52.03
51.00	96.50	86.99
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024480.D
 Acq On : 30 Aug 2022 07:11
 Operator : SY/VA
 Sample : N4365-11
 Misc : 5.42g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 DBVY9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/31/2022
 Supervised By :Mahesh Dadoda 08/31/2022

Quant Time: Aug 31 01:18:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 30 07:05:43 2022
 Response via : Initial Calibration

08/31/2022
 Supervised By :Mahesh
 Dadoda

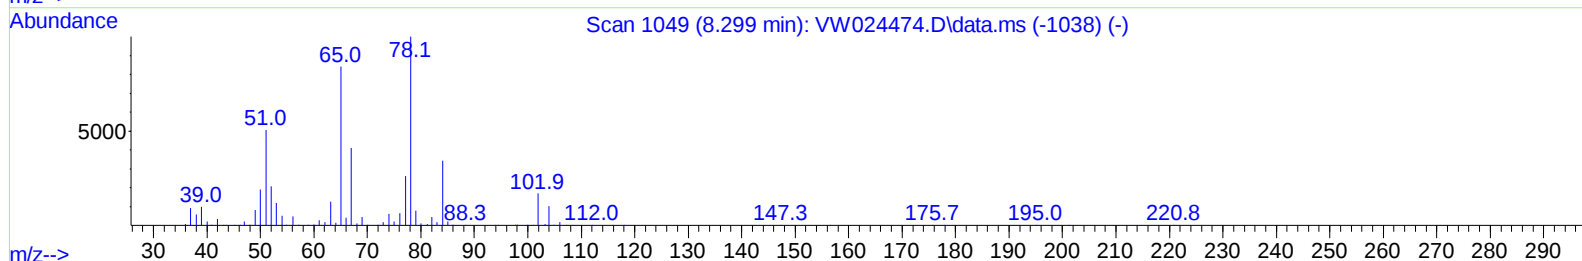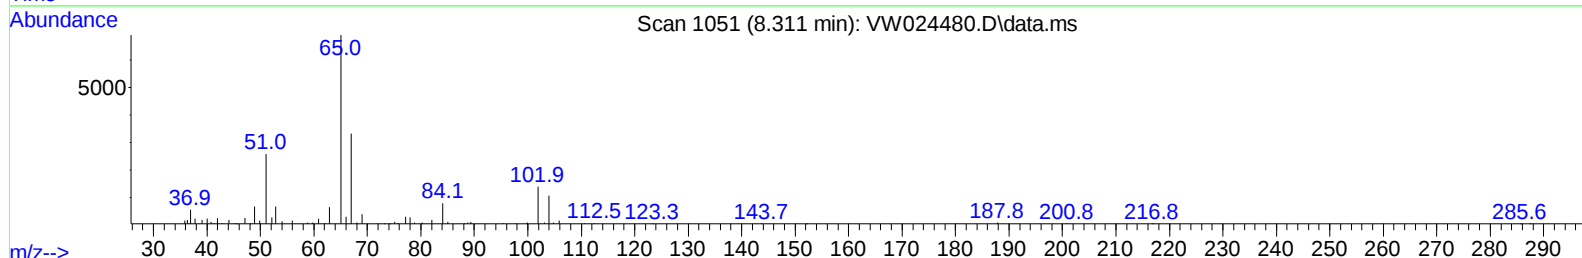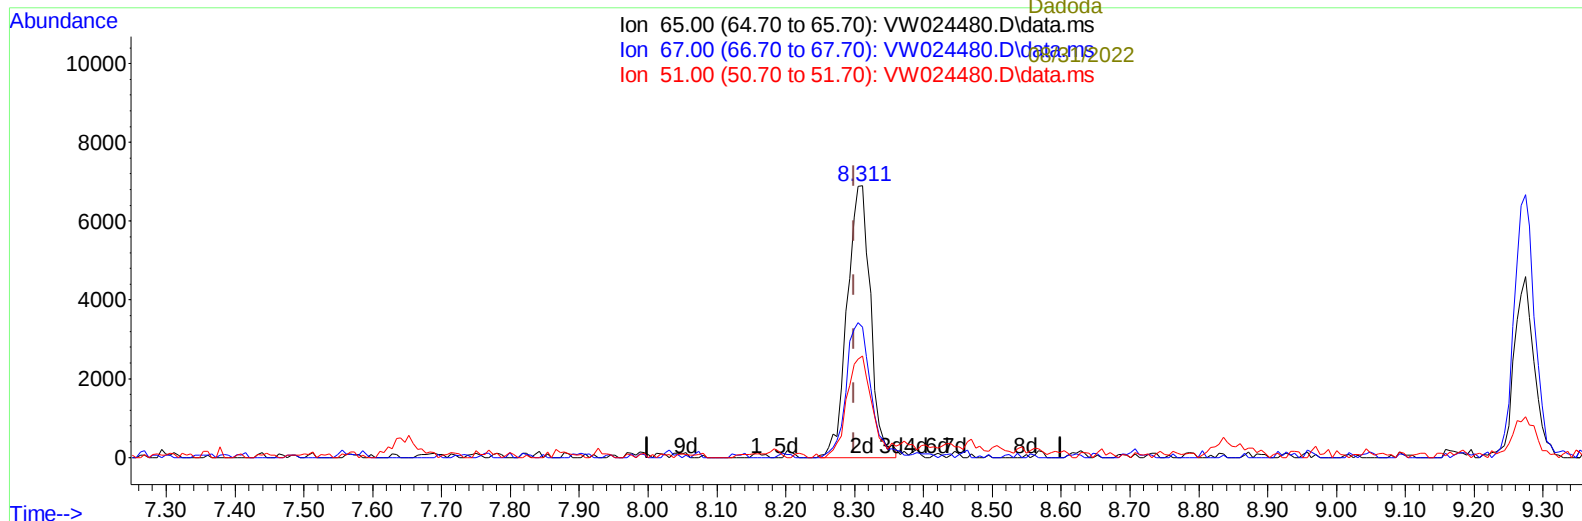

TIC: VW024480.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.311min (+ 0.012) 29.01 ug/L m

response 16243

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.10	0.39#
51.00	96.50	0.66#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024480.D
 Acq On : 30 Aug 2022 07:11
 Operator : SY/VA
 Sample : N4365-11
 Misc : 5.42g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVY9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/31/2022
 Supervised By :Mahesh Dadoda 08/31/2022

Quant Time: Aug 31 01:18:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 30 07:05:43 2022
 Response via : Initial Calibration

08/31/2022
 Supervised By :Mahesh
 Dadoda

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----08/31/2022						
Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	28719	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	31966	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	12167	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	10299	13.009	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery =	52.040%		
7) Chloroethane-d5	2.879	69	11005	18.553	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery =	74.200%		
11) 1,1-Dichloroethene-d2	4.007	63	10204	14.862	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery =	59.440%		
21) 2-Butanone-d5	7.080	46	9774m	67.030	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery =	134.060%		
24) Chloroform-d	7.647	84	23149	25.072	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery =	100.280%		
26) 1,2-Dichloroethane-d4	8.311	65	16243m	29.010	ug/L	0.01
Spiked Amount 25.000	Range 70	- 130	Recovery =	116.040%		
32) Benzene-d6	8.275	84	36440	19.896	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery =	79.600%		
36) 1,2-Dichloropropane-d6	9.274	67	13791	24.212	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery =	96.840%		
41) Toluene-d8	10.323	98	28666	16.462	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery =	65.840%		
43) trans-1,3-Dichloroprop...	10.579	79	5034	18.886	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery =	75.560%		
47) 2-Hexanone-d5	10.927	63	4606	36.136	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery =	72.280%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	15188	23.552	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery =	94.200%		
66) 1,2-Dichlorobenzene-d4	13.847	152	10029	21.889	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery =	87.560%		
Target Compounds						
46) Tetrachloroethene	10.860	164	797	1.956	ug/L	Qvalue 92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
Data File : VW024480.D
Acq On : 30 Aug 2022 07:11
Operator : SY/VA
Sample : N4365-11
Misc : 5.42g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBVY9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/31/2022
Supervised By :Mahesh Dadoda 08/31/2022

08/31/2022
Supervised By :Mahesh
Dadoda

08/31/2022

