

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024481.D
 Acq On : 30 Aug 2022 08:50
 Operator : SY/VA
 Sample : N4319-11
 Misc : 4.67g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 COZJ5

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/31/2022
 Supervised By :Mahesh Dadoda 08/31/2022

Supervised By :Mahesh
 Dadoda
 08/31/2022

Quant Time: Aug 31 01:18:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 30 07:05:43 2022
 Response via : Initial Calibration

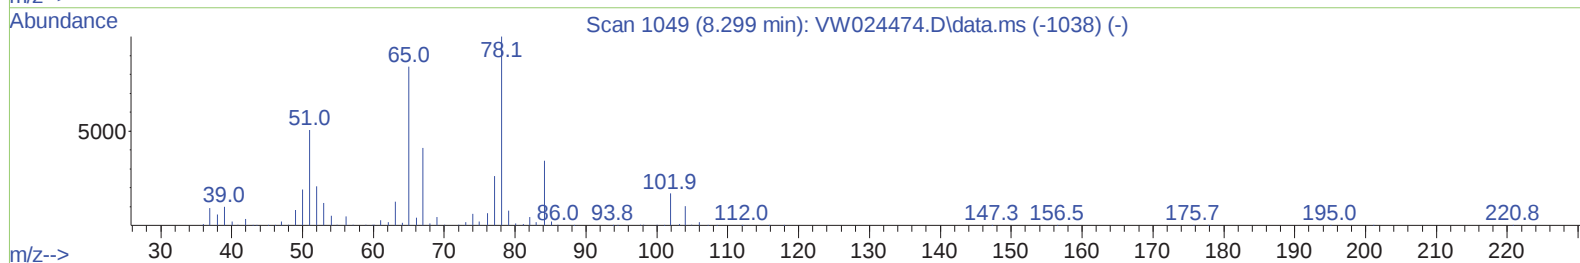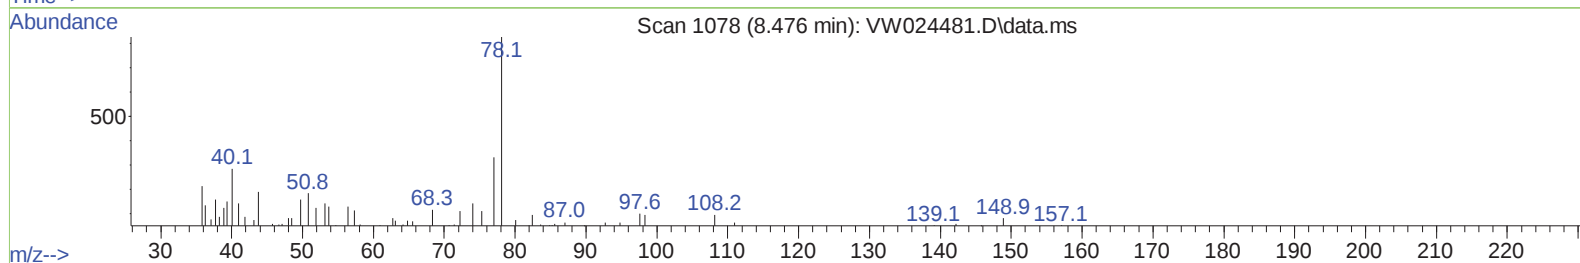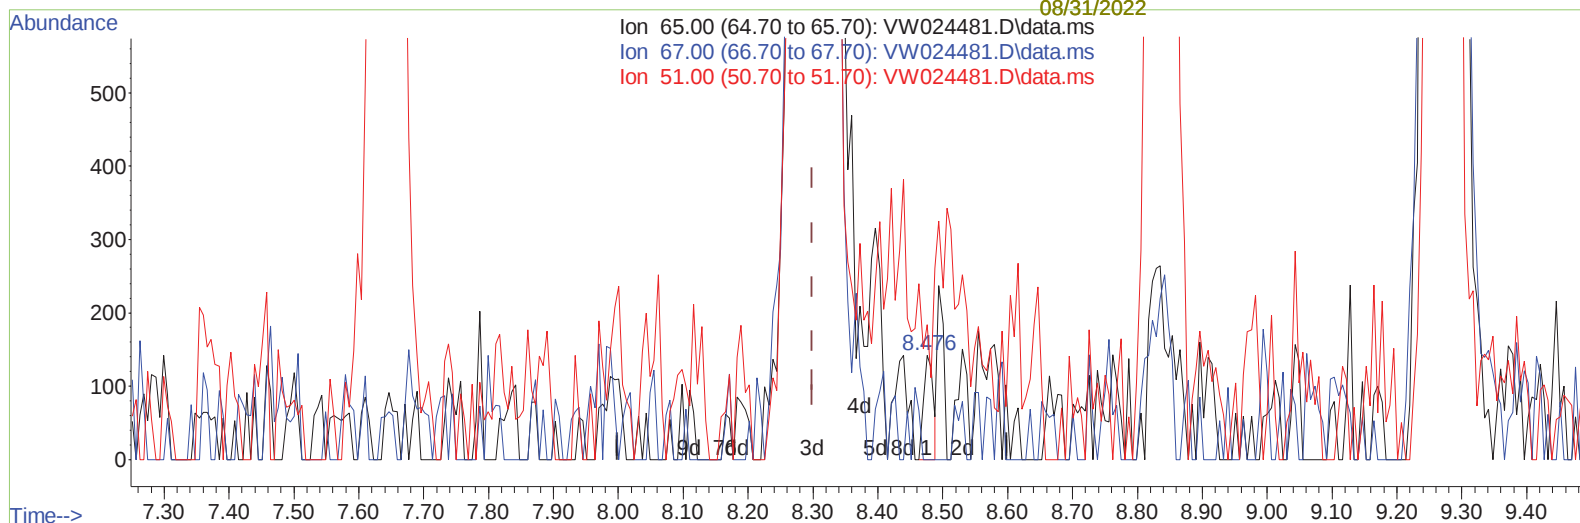

TIC: VW024481.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.476min (+ 0.177) 0.02 ug/L

response 148

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.10	40.54
51.00	96.50	91.89
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
Data File : VW024481.D
Acq On : 30 Aug 2022 08:50
Operator : SY/VA
Sample : N4319-11
Misc : 4.67g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1




Instrument :
MSVOA_W
ClientSampleId :
C0ZJ5

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/31/2022
Supervised By :Mahesh Dadoda 08/31/2022

Supervised By :Mahesh
Dadoda
08/31/2022

Quant Time: Aug 31 01:18:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Aug 30 07:05:43 2022
Response via : Initial Calibration

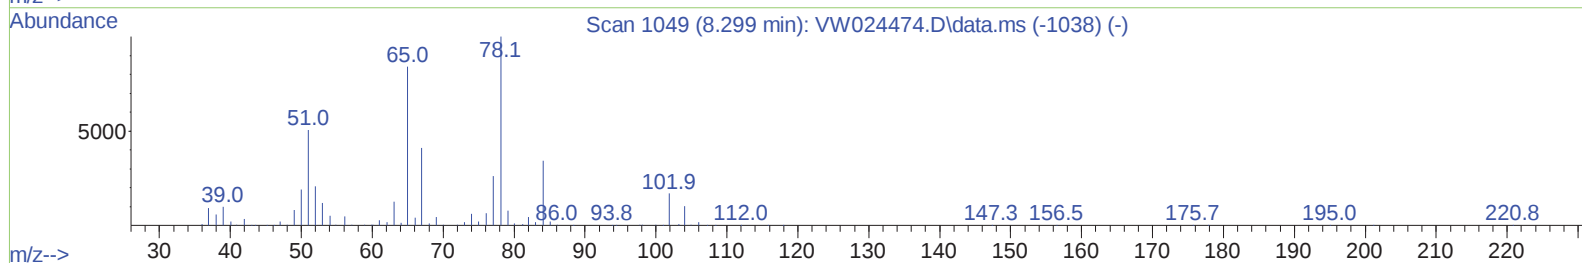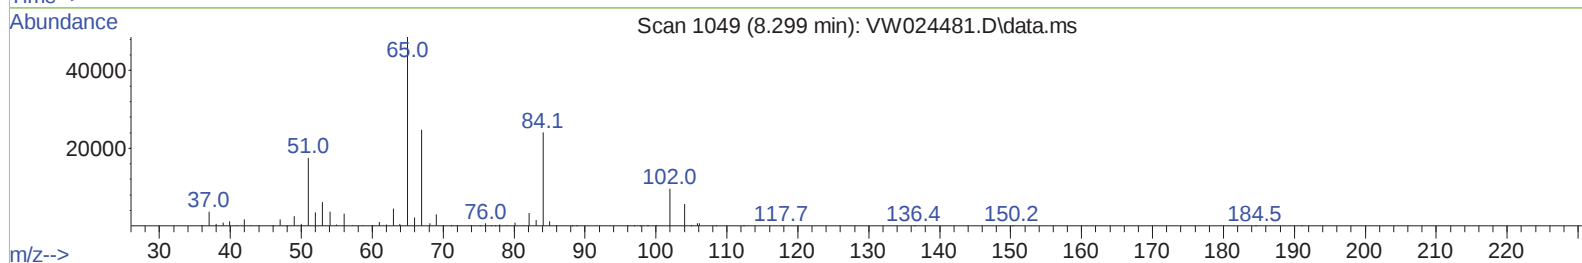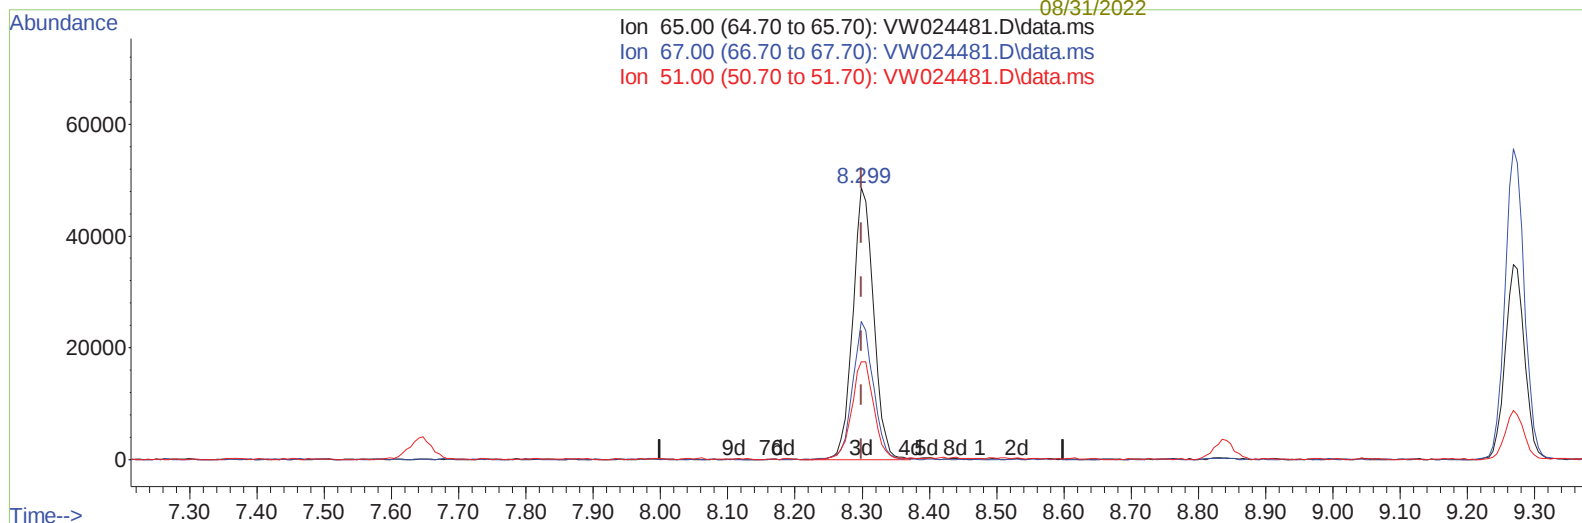

TIC: VW024481.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.299min (+ 0.000) 16.14 ug/L m

response 104299

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.10	0.06#
51.00	96.50	0.13#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024481.D
 Acq On : 30 Aug 2022 08:50
 Operator : SY/VA
 Sample : N4319-11
 Misc : 4.67g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0ZJ5

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/31/2022
 Supervised By :Mahesh Dadoda 08/31/2022

Supervised By :Mahesh
 Dadoda
 08/31/2022

Quant Time: Aug 31 01:18:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 30 07:05:43 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		331419	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		310085	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		123092	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.343	65		169408	18.543	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	74.160%		
7) Chloroethane-d5	2.873	69		101835	14.877	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	59.520%		
11) 1,1-Dichloroethene-d2	4.001	63		137206	17.317	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110		Recovery =	69.280%		
21) 2-Butanone-d5	7.080	46		37647	22.373	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	44.740%		
24) Chloroform-d	7.647	84		198493	18.629	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	74.520%		
26) 1,2-Dichloroethane-d4	8.299	65		104299m	16.142	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	64.560%#		
32) Benzene-d6	8.268	84		390252	21.966	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	87.880%		
36) 1,2-Dichloropropane-d6	9.268	67		111110	20.109	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	80.440%		
41) Toluene-d8	10.323	98		347923	20.597	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	82.400%		
43) trans-1,3-Dichloroprop...	10.573	79		41485	16.044	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	64.160%		
47) 2-Hexanone-d5	10.920	63		28915	23.386	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	46.780%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84		78027	12.473	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	49.880%		
66) 1,2-Dichlorobenzene-d4	13.853	152		92677	19.994	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	79.960%		
Target Compounds							
13) Acetone	4.123	43		9500	9.460	ug/L	Qvalue 89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
Data File : VW024481.D
Acq On : 30 Aug 2022 08:50
Operator : SY/VA
Sample : N4319-11
Misc : 4.67g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0ZJ5

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/31/2022
Supervised By :Mahesh Dadoda 08/31/2022

Supervised By :Mahesh
Dadoda
08/31/2022

Quant Time: Aug 31 01:18:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Aug 30 07:05:43 2022
Response via : Initial Calibration

