




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024482.D
 Acq On : 30 Aug 2022 09:15
 Operator : SY/VA
 Sample : N4363-18
 Misc : 5.52g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVX2

Manual IntegrationsAPPROVED

Quant Time: Aug 31 01:18:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 30 07:05:43 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/12/2022
 Supervised By :Mahesh Dadoda 09/12/2022

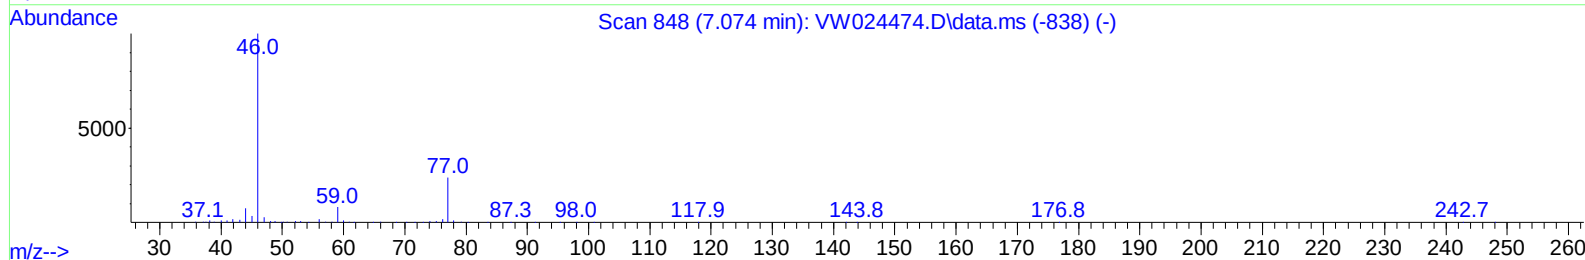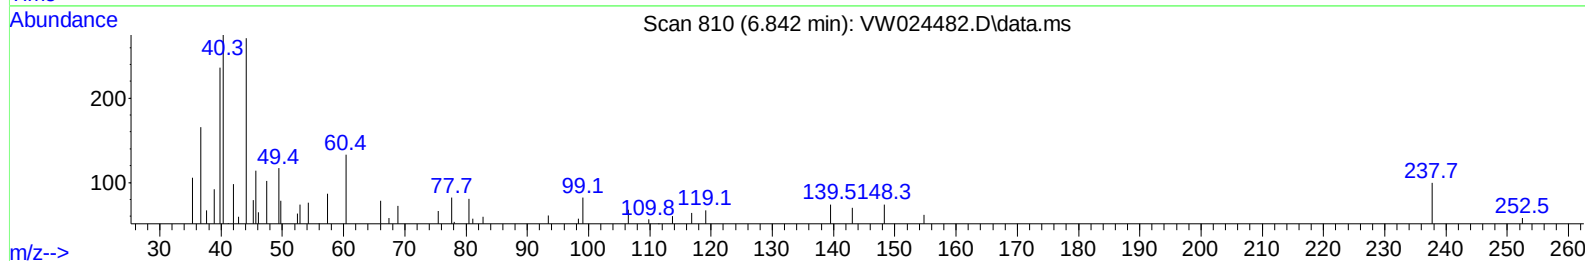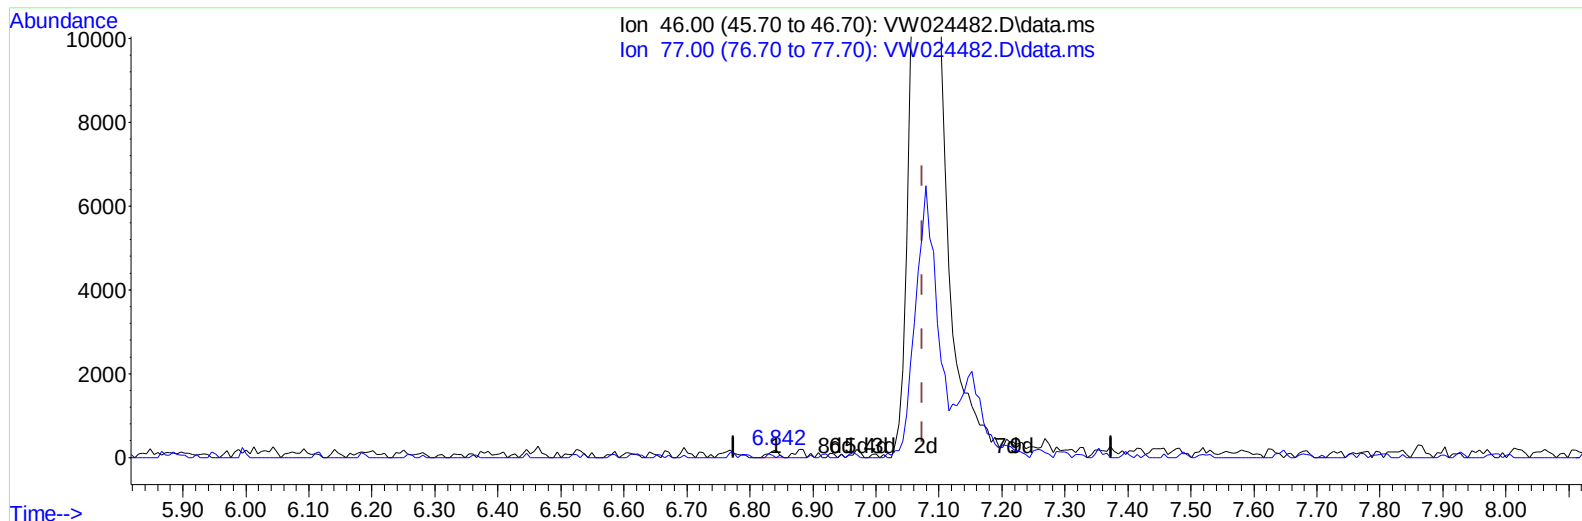

TIC: VW024482.D\data.ms

(21) 2-Butanone-d5 (S)

6.842min (-0.232) 0.10 ug/L

response 195

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	12.40	10.26
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024482.D
 Acq On : 30 Aug 2022 09:15
 Operator : SY/VA
 Sample : N4363-18
 Misc : 5.52g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVX2

Manual IntegrationsAPPROVED

Quant Time: Aug 31 01:18:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 30 07:05:43 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/12/2022
 Supervised By :Mahesh Dadoda 09/12/2022

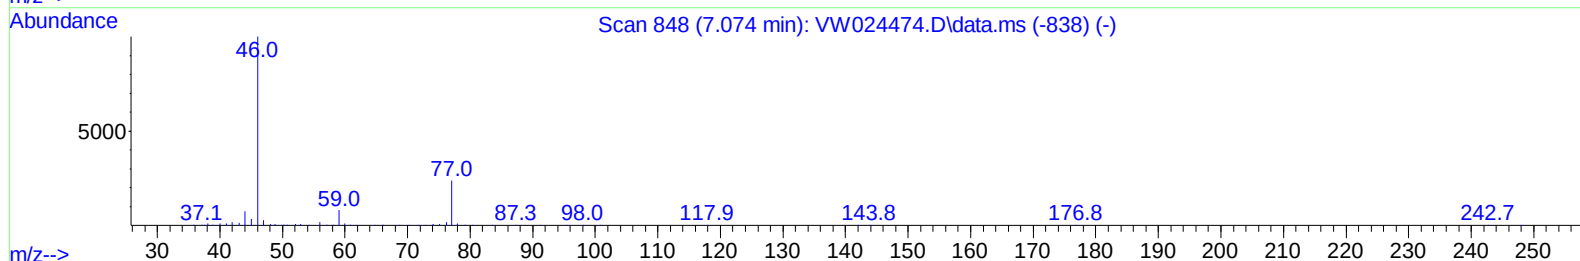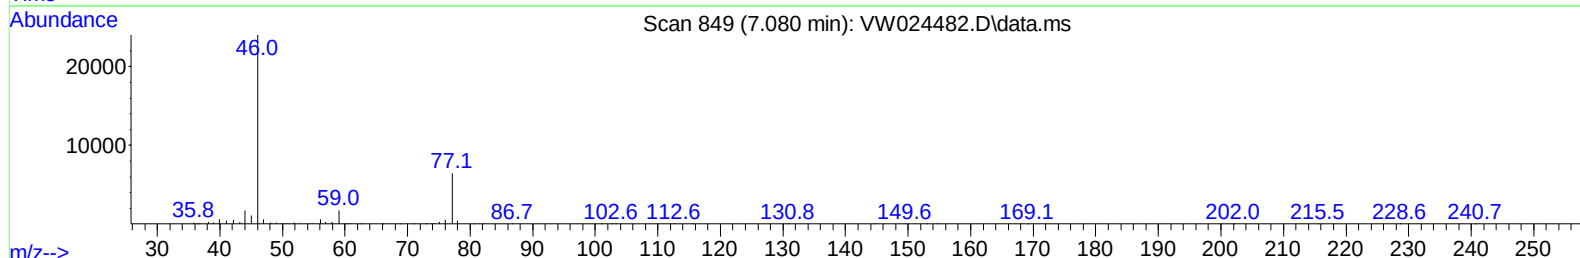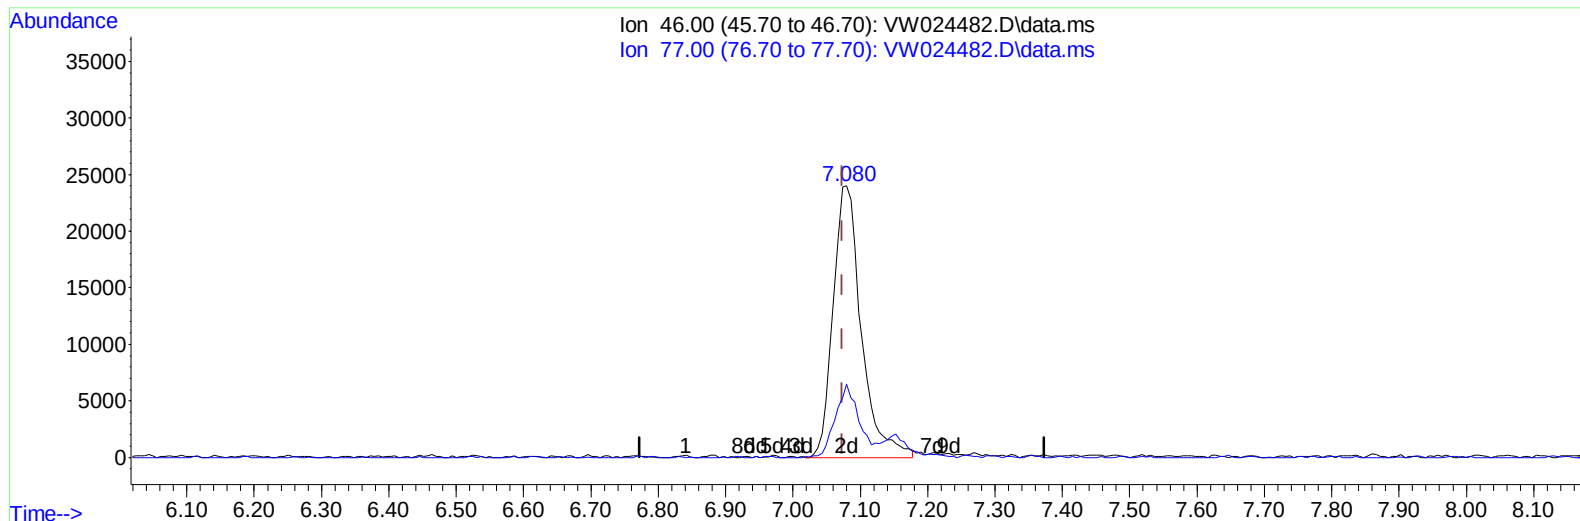

TIC: VW024482.D\data.ms

(21) 2-Butanone-d5 (S)

7.080min (+ 0.006) 35.51 ug/L m

response 69555

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	12.40	0.03#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024482.D
 Acq On : 30 Aug 2022 09:15
 Operator : SY/VA
 Sample : N4363-18
 Misc : 5.52g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVX2

Manual IntegrationsAPPROVED

Quant Time: Aug 31 01:18:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 30 07:05:43 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/12/2022
 Supervised By :Mahesh Dadoda 09/12/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.841	114		385791	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		364117	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		164898	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.343	65		189621	17.831	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	71.320%		
7) Chloroethane-d5	2.873	69		133659	16.774	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	67.080%		
11) 1,1-Dichloroethene-d2	4.007	63		149523	16.212	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	64.840%		
21) 2-Butanone-d5	7.080	46		69555m	35.509	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	71.020%		
24) Chloroform-d	7.647	84		225674	18.195	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	72.800%		
26) 1,2-Dichloroethane-d4	8.305	65		132989	17.681	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	70.720%		
32) Benzene-d6	8.268	84		435036	20.853	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	83.400%		
36) 1,2-Dichloropropane-d6	9.274	67		127512	19.653	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	78.600%		
41) Toluene-d8	10.323	98		406339	20.486	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	81.960%		
43) trans-1,3-Dichloroprop...	10.579	79		54436	17.929	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	71.720%		
47) 2-Hexanone-d5	10.927	63		52601	36.229	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	72.460%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84		122511	16.678	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	66.720%		
66) 1,2-Dichlorobenzene-d4	13.853	152		132682	21.367	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	85.480%		
Target Compounds							
13) Acetone	4.129	43		3749	3.207	ug/L	Qvalue 87

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
Data File : VW024482.D
Acq On : 30 Aug 2022 09:15
Operator : SY/VA
Sample : N4363-18
Misc : 5.52g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBVX2

Manual IntegrationsAPPROVED

Quant Time: Aug 31 01:18:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Aug 30 07:05:43 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 09/12/2022
Supervised By :Mahesh Dadoda 09/12/2022

