




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024484.D
 Acq On : 30 Aug 2022 10:04
 Operator : SY/VA
 Sample : N4365-07
 Misc : 5.92g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVY5

Manual IntegrationsAPPROVED

Quant Time: Aug 31 01:19:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 30 07:05:43 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/31/2022
 Supervised By :Mahesh Dadoda 08/31/2022

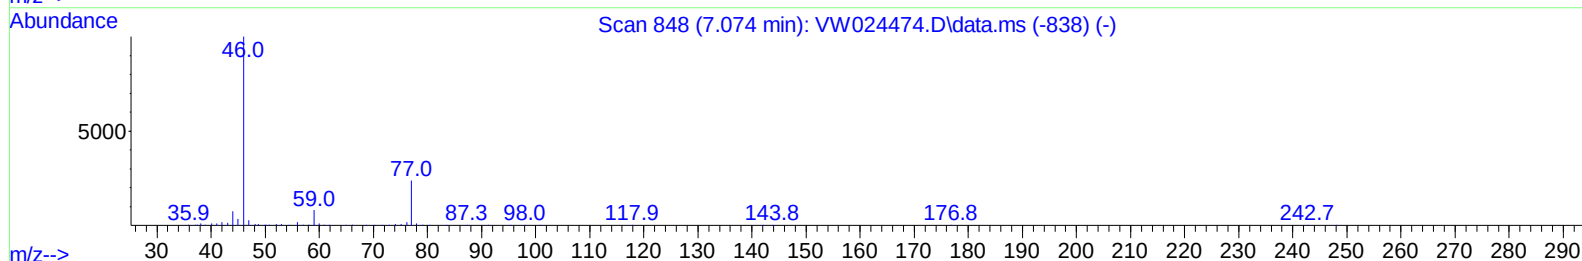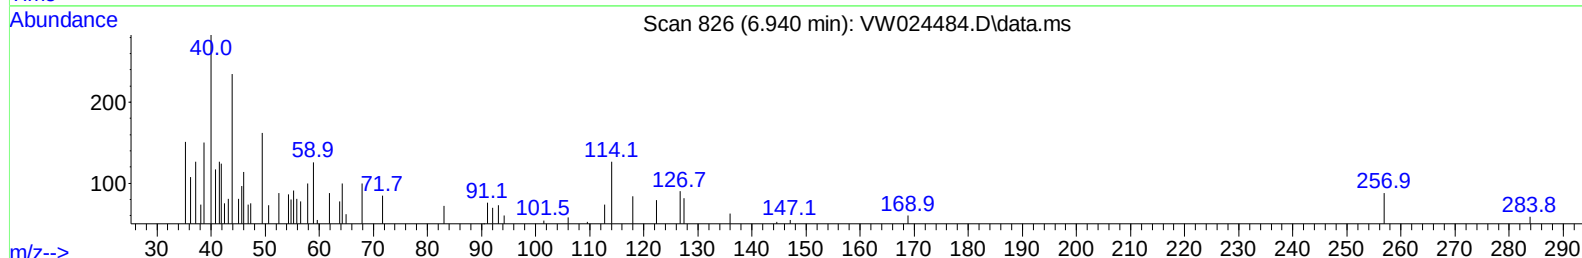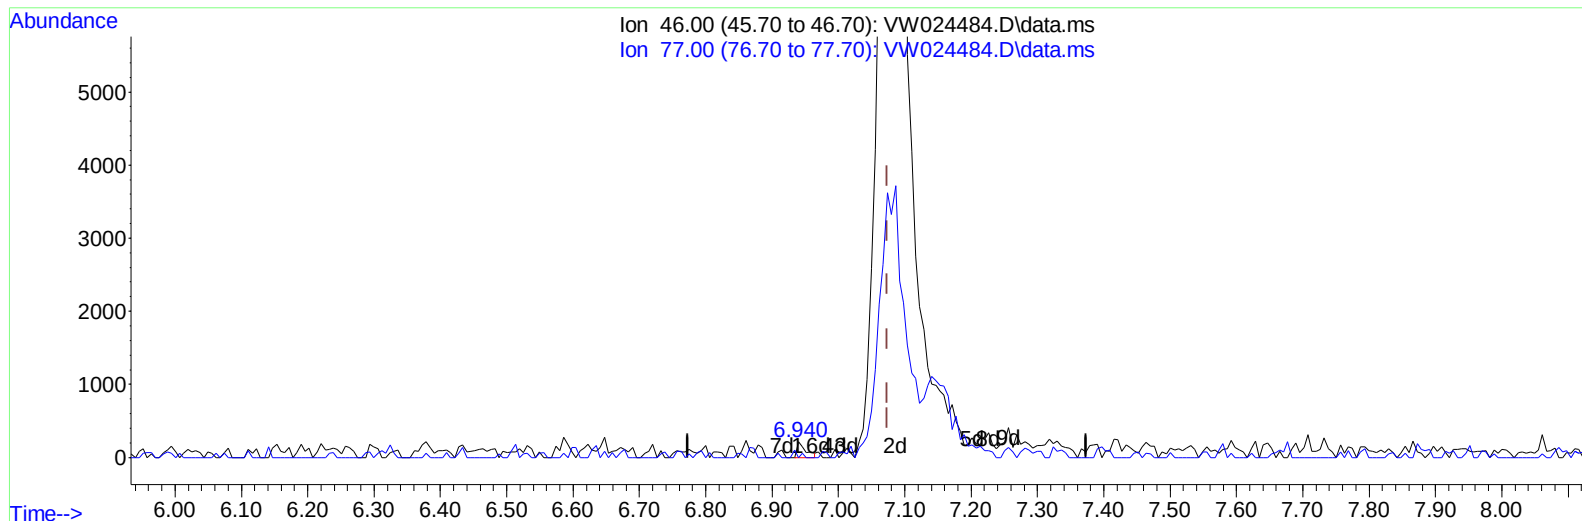

TIC: VW024484.D\data.ms

(21) 2-Butanone-d5 (S)

6.940min (-0.134) 0.16 ug/L

response 200

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	12.40	11.00
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024484.D
 Acq On : 30 Aug 2022 10:04
 Operator : SY/VA
 Sample : N4365-07
 Misc : 5.92g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVY5

Manual IntegrationsAPPROVED

Quant Time: Aug 31 01:19:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 30 07:05:43 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/31/2022
 Supervised By :Mahesh Dadoda 08/31/2022

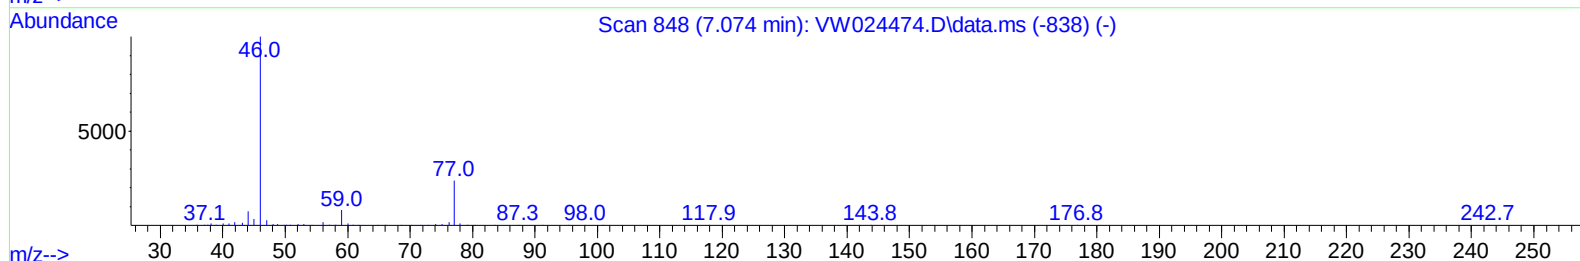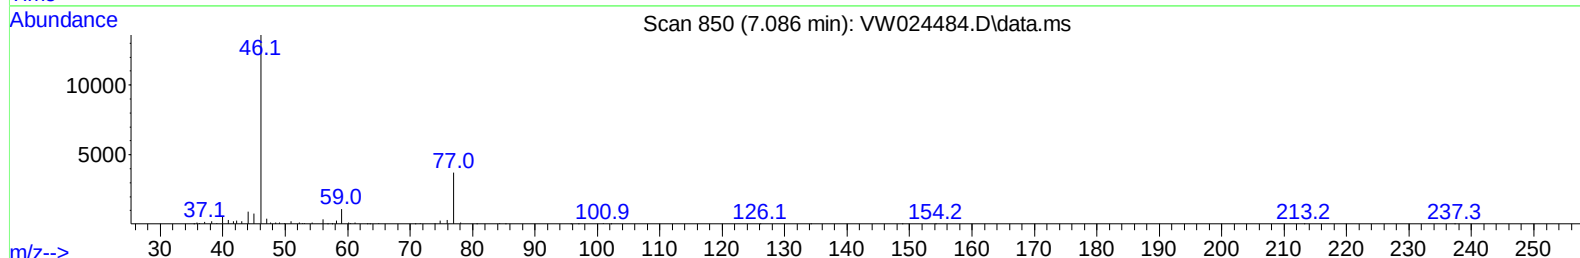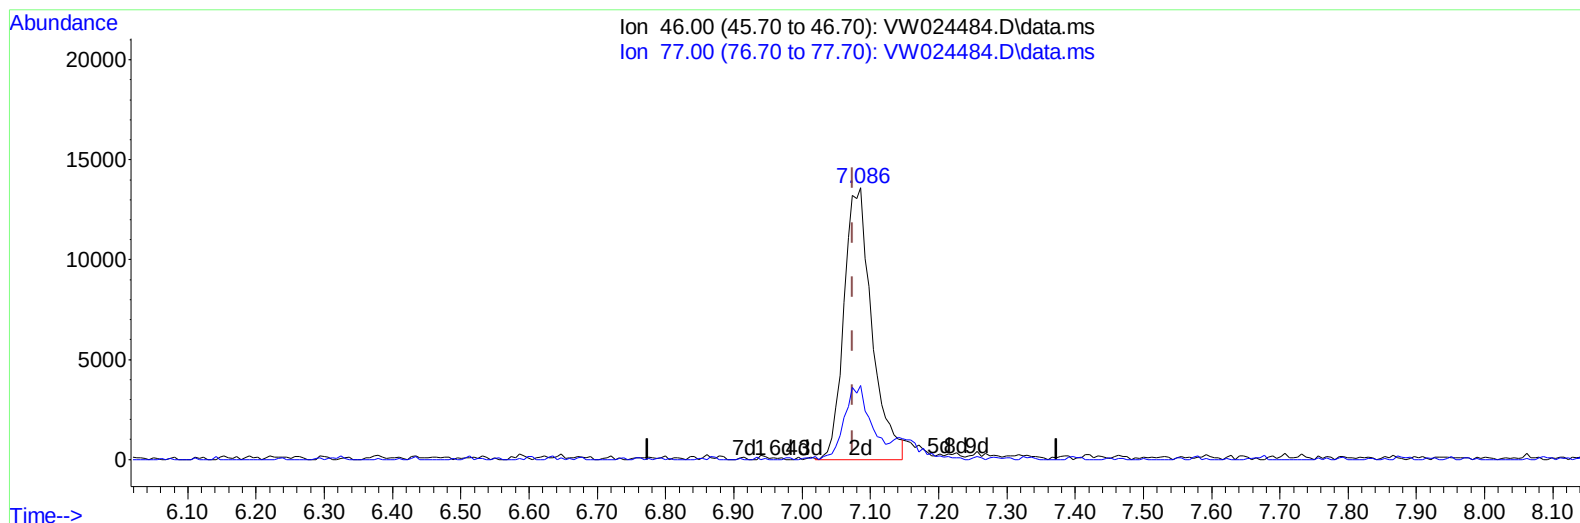

TIC: VW024484.D\data.ms

(21) 2-Butanone-d5 (S)

7.086min (+ 0.012) 29.98 ug/L m

response 38587

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	12.40	0.06#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024484.D
 Acq On : 30 Aug 2022 10:04
 Operator : SY/VA
 Sample : N4365-07
 Misc : 5.92g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVY5

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/31/2022
 Supervised By :Mahesh Dadoda 08/31/2022

Quant Time: Aug 31 01:19:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 30 07:05:43 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	253524	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	243505	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	103518	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	133798	19.145	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	76.600%	
7) Chloroethane-d5	2.873	69	74483	14.225	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	56.880%	
11) 1,1-Dichloroethene-d2	4.007	63	103675	17.105	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	68.440%	
21) 2-Butanone-d5	7.086	46	38587m	29.977	ug/L	0.01
Spiked Amount 50.000	Range 20	- 135	Recovery	=	59.960%	
24) Chloroform-d	7.647	84	144984	17.788	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	71.160%	
26) 1,2-Dichloroethane-d4	8.305	65	82456	16.682	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	66.720%#	
32) Benzene-d6	8.275	84	274806	19.697	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	78.800%	
36) 1,2-Dichloropropane-d6	9.275	67	81866	18.868	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	75.480%	
41) Toluene-d8	10.323	98	251682	18.973	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	75.880%	
43) trans-1,3-Dichloroprop...	10.573	79	32463	15.988	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	63.960%	
47) 2-Hexanone-d5	10.921	63	28261	29.106	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	58.220%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	72339	14.726	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	58.920%	
66) 1,2-Dichlorobenzene-d4	13.853	152	81691	20.956	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	83.840%	
Target Compounds						
46) Tetrachloroethene	10.860	164	2257	0.727	ug/L #	Qvalue 68

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
Data File : VW024484.D
Acq On : 30 Aug 2022 10:04
Operator : SY/VA
Sample : N4365-07
Misc : 5.92g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBVY5

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/31/2022
Supervised By :Mahesh Dadoda 08/31/2022

Quant Time: Aug 31 01:19:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Aug 30 07:05:43 2022
Response via : Initial Calibration

