




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
Data File : VW024496.D
Acq On : 30 Aug 2022 17:35
Operator : SY/VA
Sample : N4440-03
Misc : 5.13g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0ZJ9

Manual IntegrationsAPPROVED

Quant Time: Aug 31 02:56:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 31 02:55:40 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/31/2022
Supervised By :Mahesh Dadoda 08/31/2022

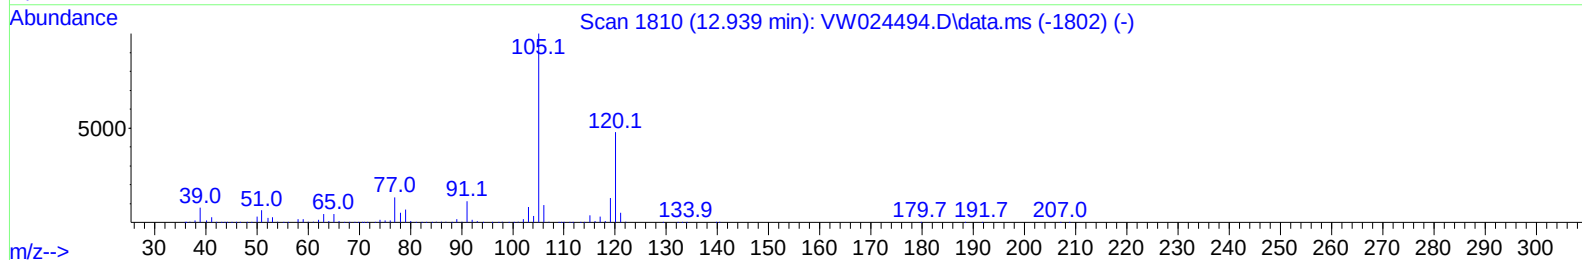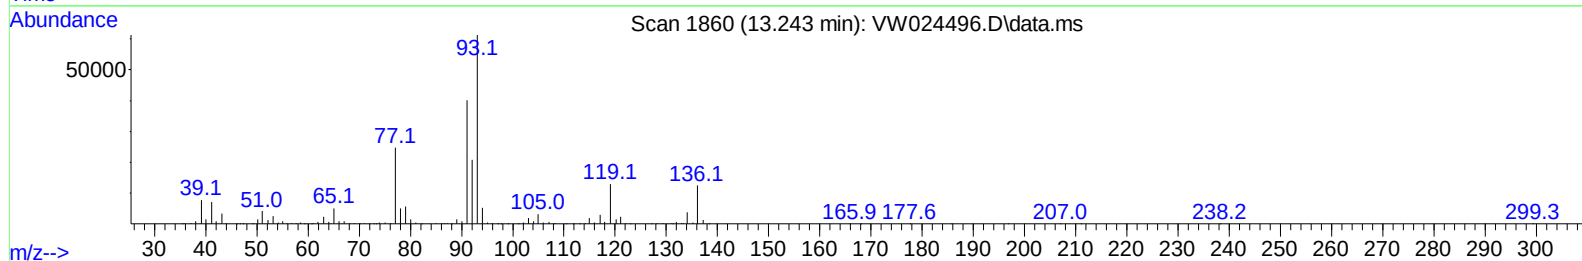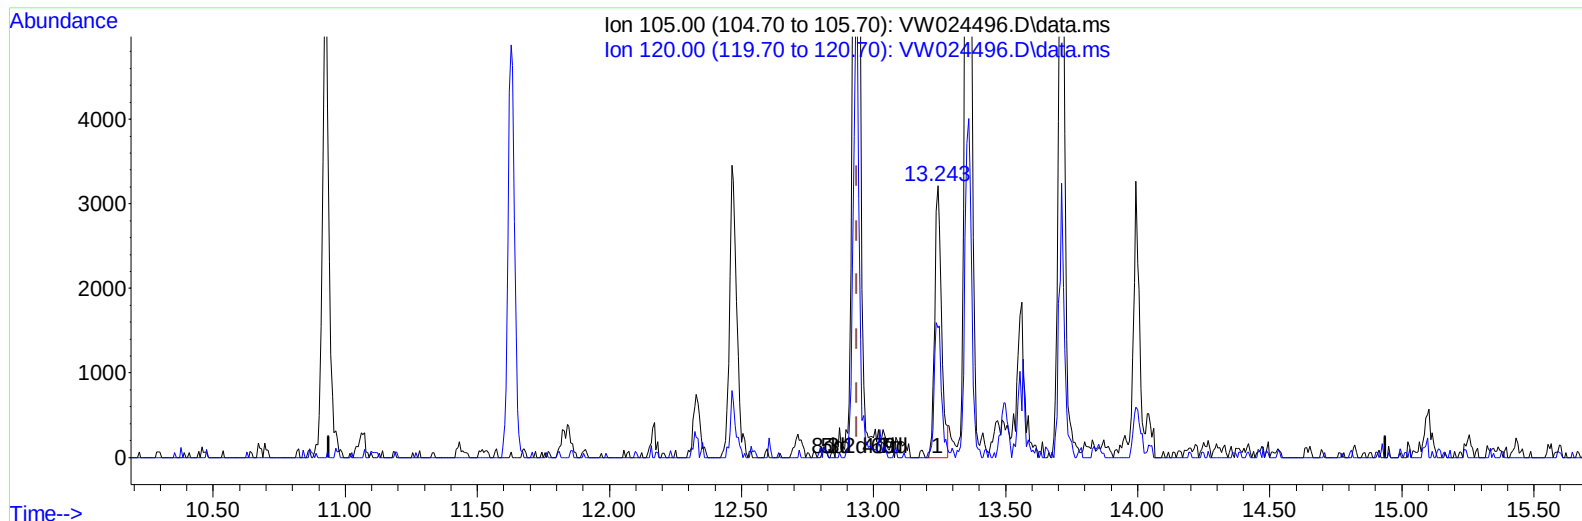

TIC: VW024496.D\data.ms

(62) 1,3,5-Trimethylbenzene

13.243min (+ 0.305) 0.31 ug/L

response 5804

Ion	Exp%	Act%
105.00	100.00	100.00
120.00	48.00	53.05
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024496.D
 Acq On : 30 Aug 2022 17:35
 Operator : SY/VA
 Sample : N4440-03
 Misc : 5.13g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0ZJ9

Manual IntegrationsAPPROVED

Quant Time: Aug 31 02:56:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 31 02:55:40 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/31/2022
 Supervised By :Mahesh Dadoda 08/31/2022

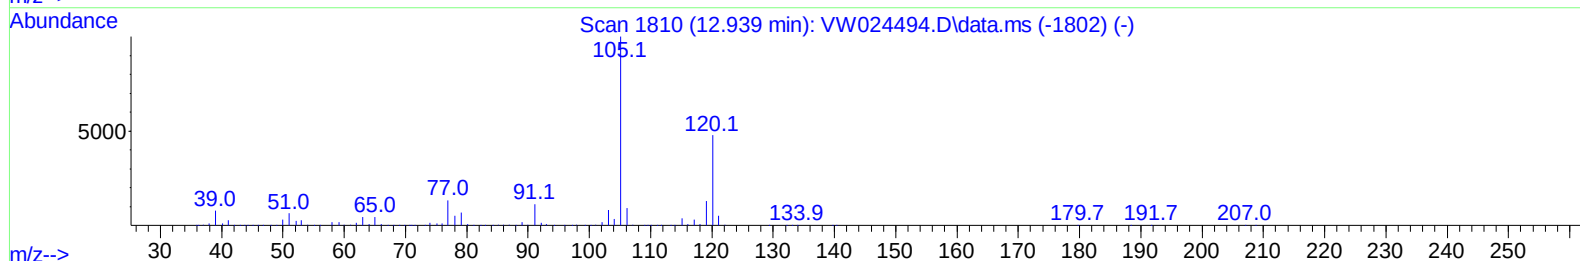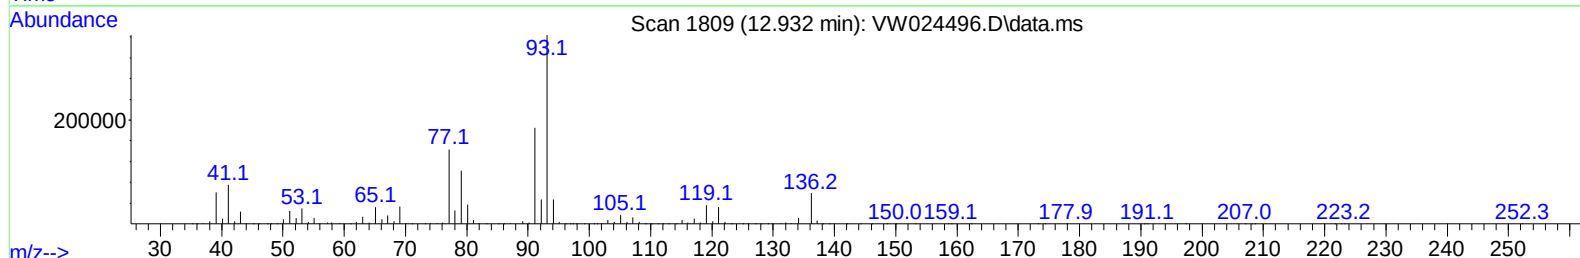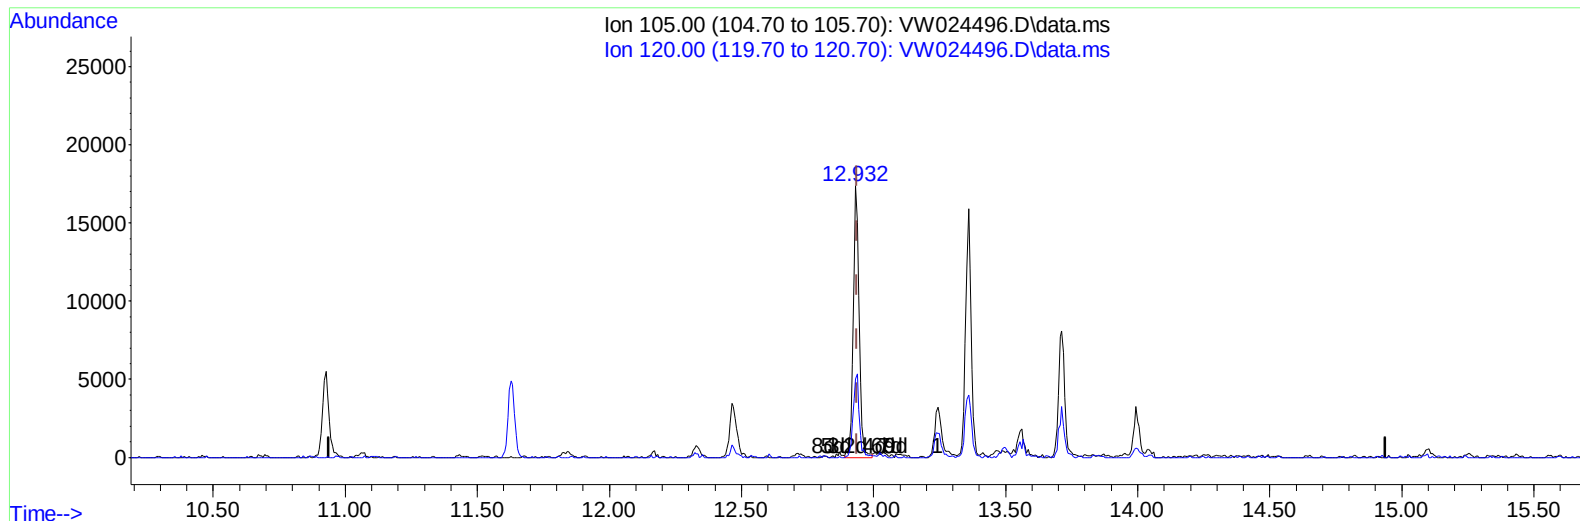

TIC: VW024496.D\data.ms

(62) 1,3,5-Trimethylbenzene

12.932min (-0.006) 1.42 ug/L m

response 26848

Ion	Exp%	Act%
105.00	100.00	100.00
120.00	48.00	11.47#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024496.D
 Acq On : 30 Aug 2022 17:35
 Operator : SY/VA
 Sample : N4440-03
 Misc : 5.13g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0ZJ9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/31/2022
 Supervised By :Mahesh Dadoda 08/31/2022

Quant Time: Aug 31 02:56:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 31 02:55:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	427912	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	384606	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	176841	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.337	65	203726	17.271	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	69.080%	
7) Chloroethane-d5	2.873	69	133145	15.065	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	60.280%	
11) 1,1-Dichloroethene-d2	3.995	63	139782	13.664	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110	Recovery	=	54.640%	
21) 2-Butanone-d5	7.080	46	52186	24.020	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	48.040%	
24) Chloroform-d	7.647	84	219527	15.957	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	63.840%	
26) 1,2-Dichloroethane-d4	8.299	65	122150	14.641	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	58.560%#	
32) Benzene-d6	8.268	84	422176	19.158	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	76.640%	
36) 1,2-Dichloropropane-d6	9.274	67	125343	18.290	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	73.160%	
41) Toluene-d8	10.323	98	379852	18.130	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	72.520%	
43) trans-1,3-Dichloroprop...	10.579	79	47725	14.881	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	59.520%	
47) 2-Hexanone-d5	10.927	63	43321	28.248	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	56.500%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	107630	13.872	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	55.480%	
66) 1,2-Dichlorobenzene-d4	13.847	152	111618	16.761	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	67.040%#	
Target Compounds						
13) Acetone	4.123	43	21886	16.880	ug/L	93
16) Methylene chloride	4.903	84	40397	5.629	ug/L	88
20) cis-1,2-Dichloroethene	7.171	96	7867	1.182	ug/L #	98
34) Trichloroethene	9.091	95	6295	0.997	ug/L	93
46) Tetrachloroethene	10.866	164	2296	0.468	ug/L	92
62) 1,3,5-Trimethylbenzene	12.932	105	26848m	1.418	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

