

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024498.D
 Acq On : 30 Aug 2022 18:24
 Operator : SY/VA
 Sample : N4440-04
 Misc : 4.60g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 C0ZK0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/31/2022
 Supervised By :Mahesh Dadoda 08/31/2022

08/31/2022
 Supervised By :Mahesh
 Dadoda
 08/31/2022

Quant Time: Aug 31 02:56:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 31 02:55:40 2022
 Response via : Initial Calibration

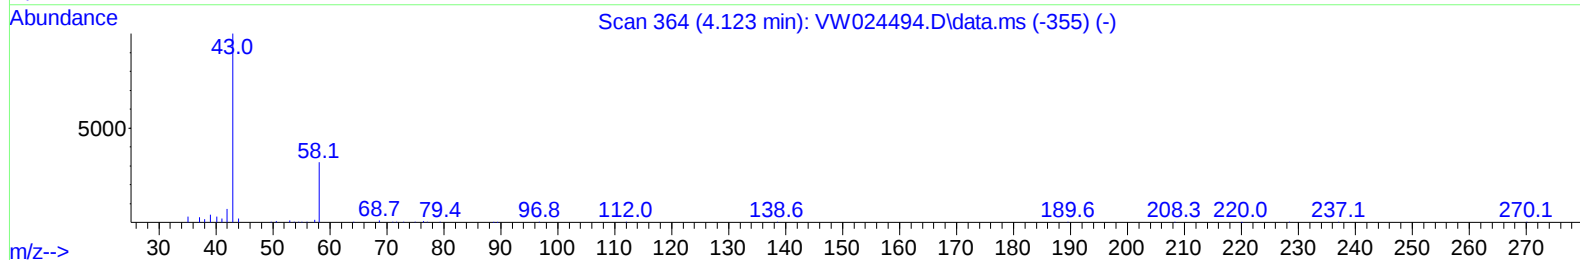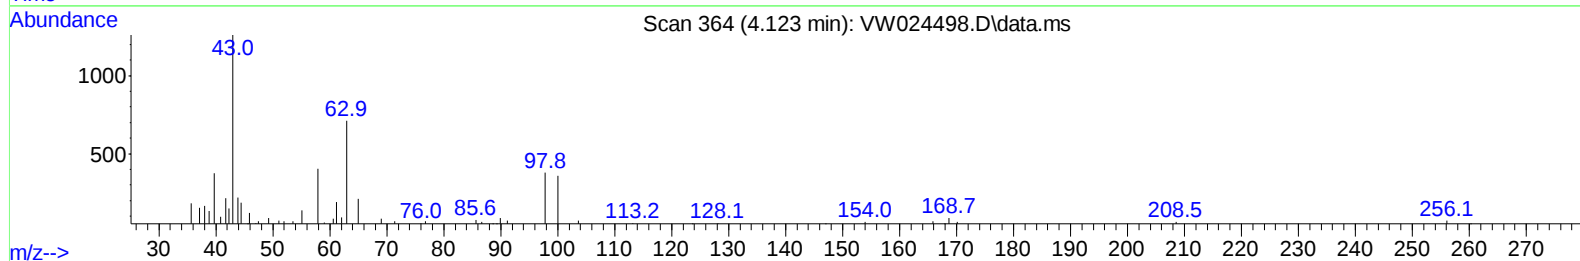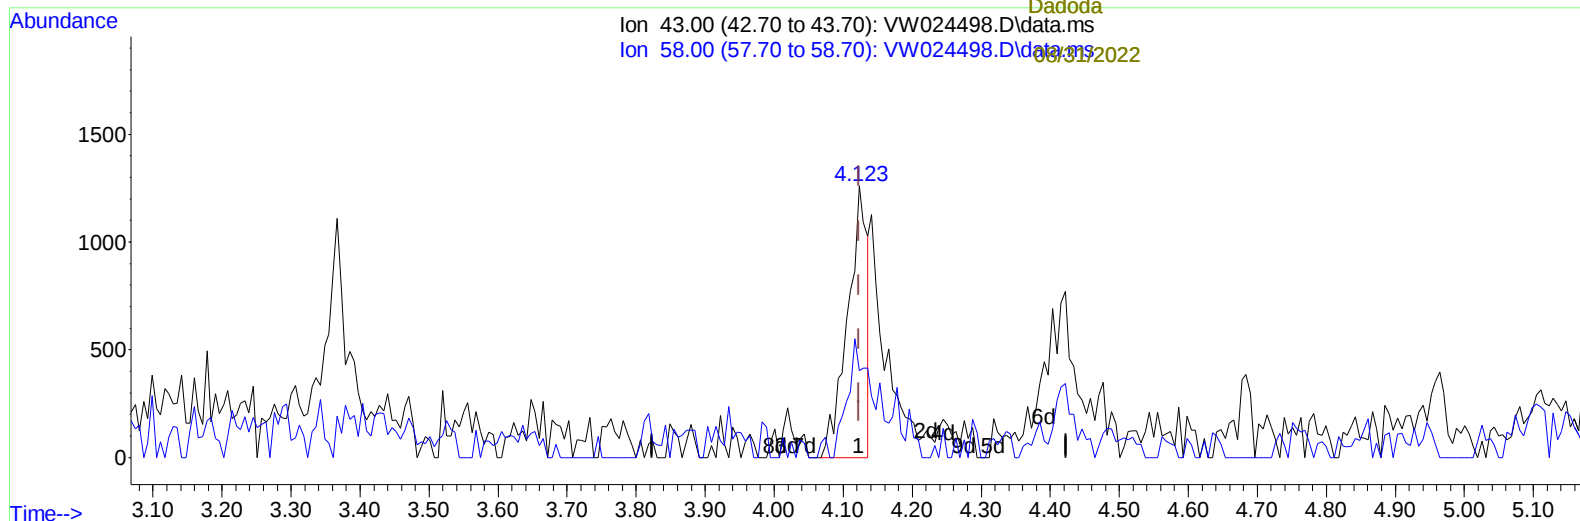

TIC: VW024498.D\data.ms

(13) Acetone (T)

4.123min (-0.000) 4.19 ug/L

response 2480

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	29.20	27.34
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024498.D
 Acq On : 30 Aug 2022 18:24
 Operator : SY/VA
 Sample : N4440-04
 Misc : 4.60g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 C0ZK0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/31/2022
 Supervised By :Mahesh Dadoda 08/31/2022

Quant Time: Aug 31 02:56:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 31 02:55:40 2022
 Response via : Initial Calibration

08/31/2022
 Supervised By :Mahesh
 Dadoda
 08/31/2022

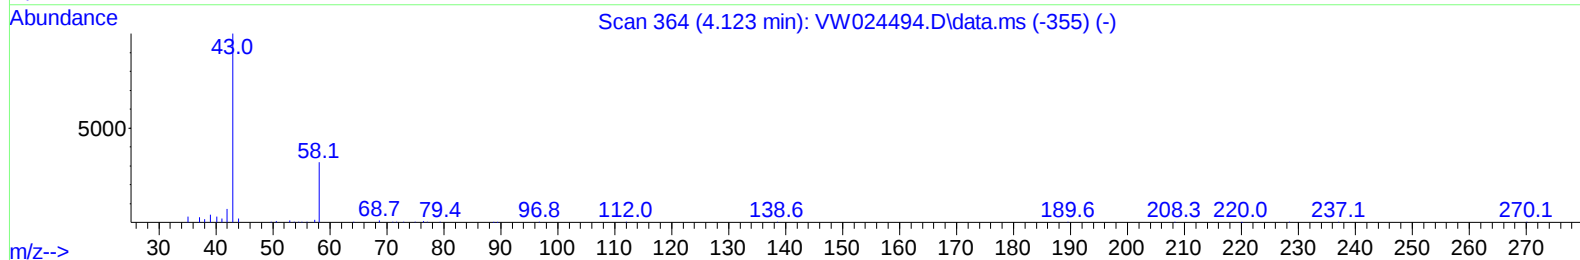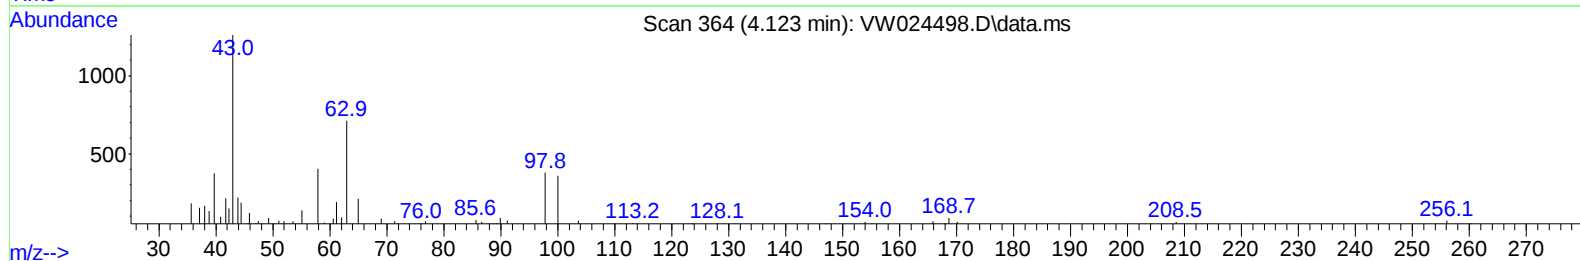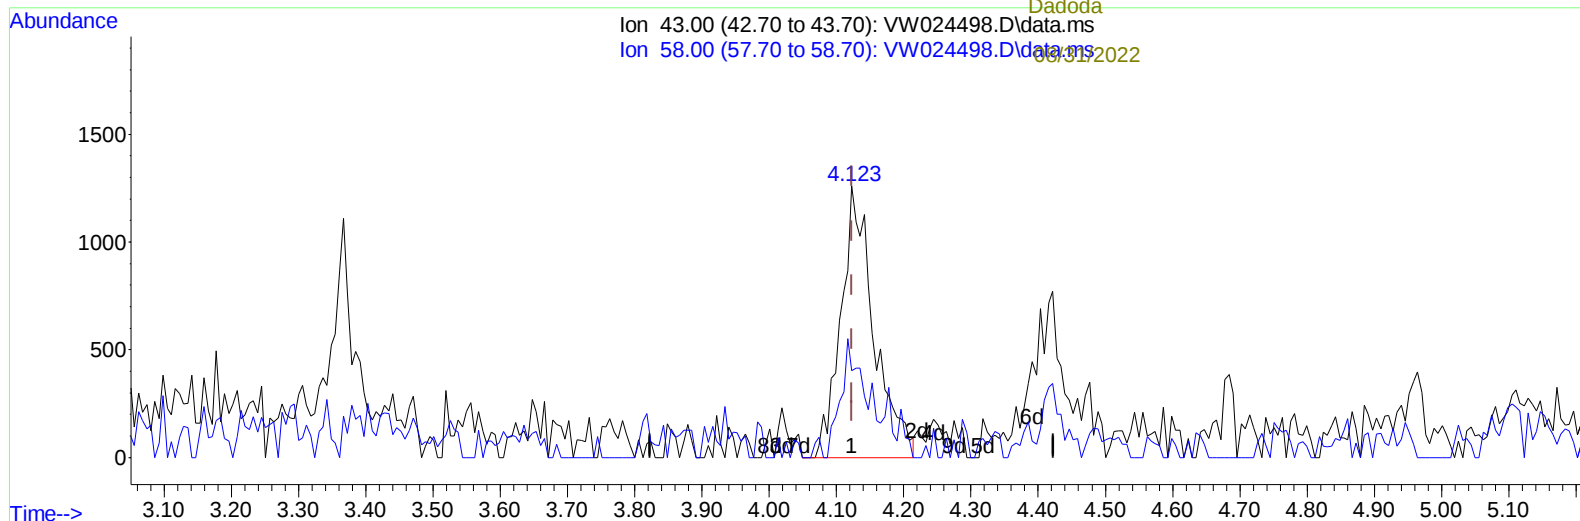

TIC: VW024498.D\data.ms

(13) Acetone (T)

4.123min (-0.000) 7.24 ug/L m

response 4287

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	29.20	15.82
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024498.D
 Acq On : 30 Aug 2022 18:24
 Operator : SY/VA
 Sample : N4440-04
 Misc : 4.60g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 C02K0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/31/2022
 Supervised By :Mahesh Dadoda 08/31/2022

08/31/2022
 Supervised By :Mahesh
 Dadoda

Quant Time: Aug 31 02:56:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 31 02:55:40 2022
 Response via : Initial Calibration

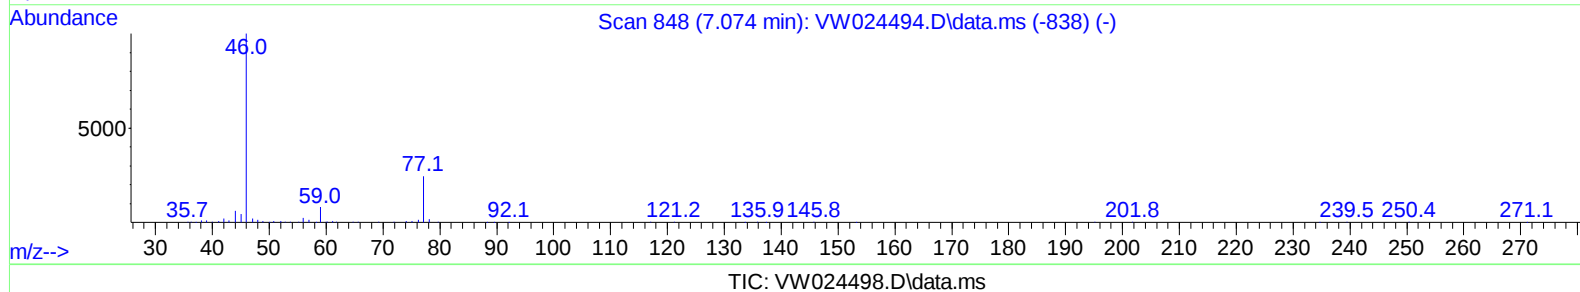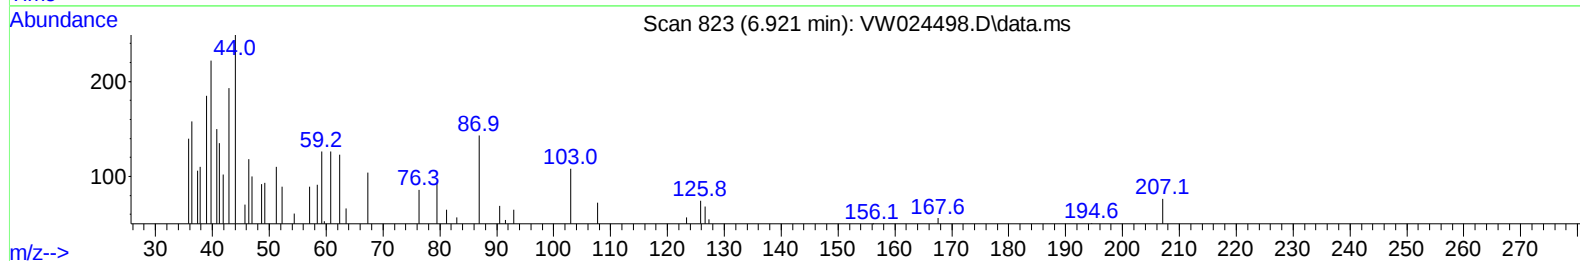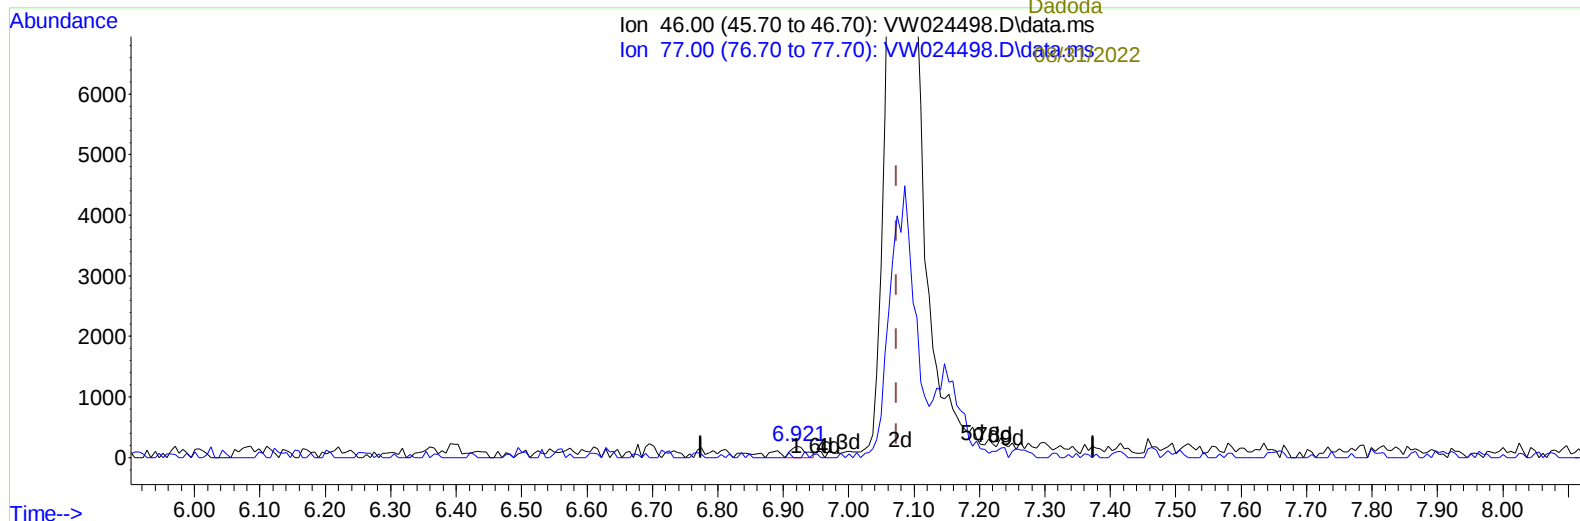

(21) 2-Butanone-d5 (S)

6.921min (-0.153) 0.31 ug/L

response 308

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	12.40	12.34
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024498.D
 Acq On : 30 Aug 2022 18:24
 Operator : SY/VA
 Sample : N4440-04
 Misc : 4.60g/10mL/MSVOA_W/SoIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 C0ZK0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/31/2022
 Supervised By :Mahesh Dadoda 08/31/2022

08/31/2022
 Supervised By :Mahesh
 Dadoda
 08/31/2022

Quant Time: Aug 31 02:56:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 31 02:55:40 2022
 Response via : Initial Calibration

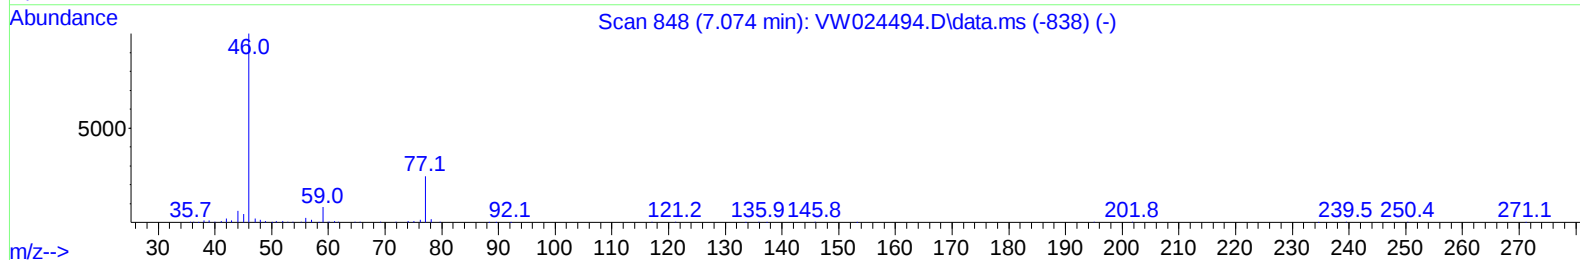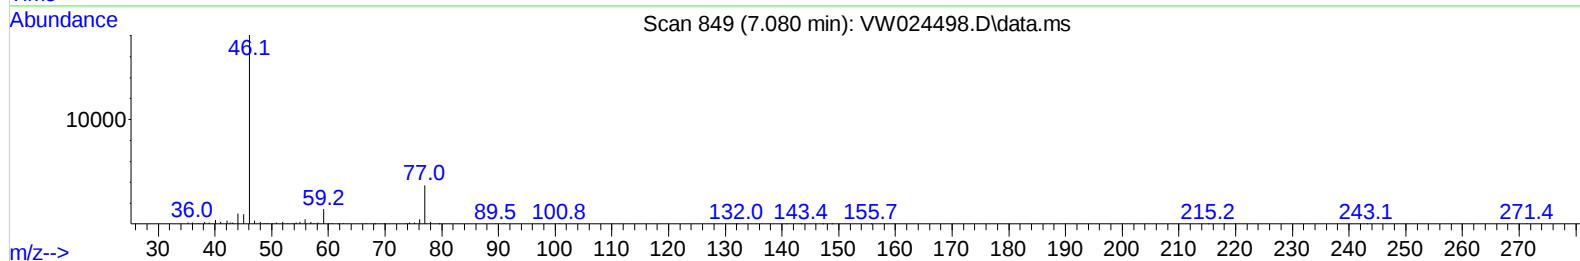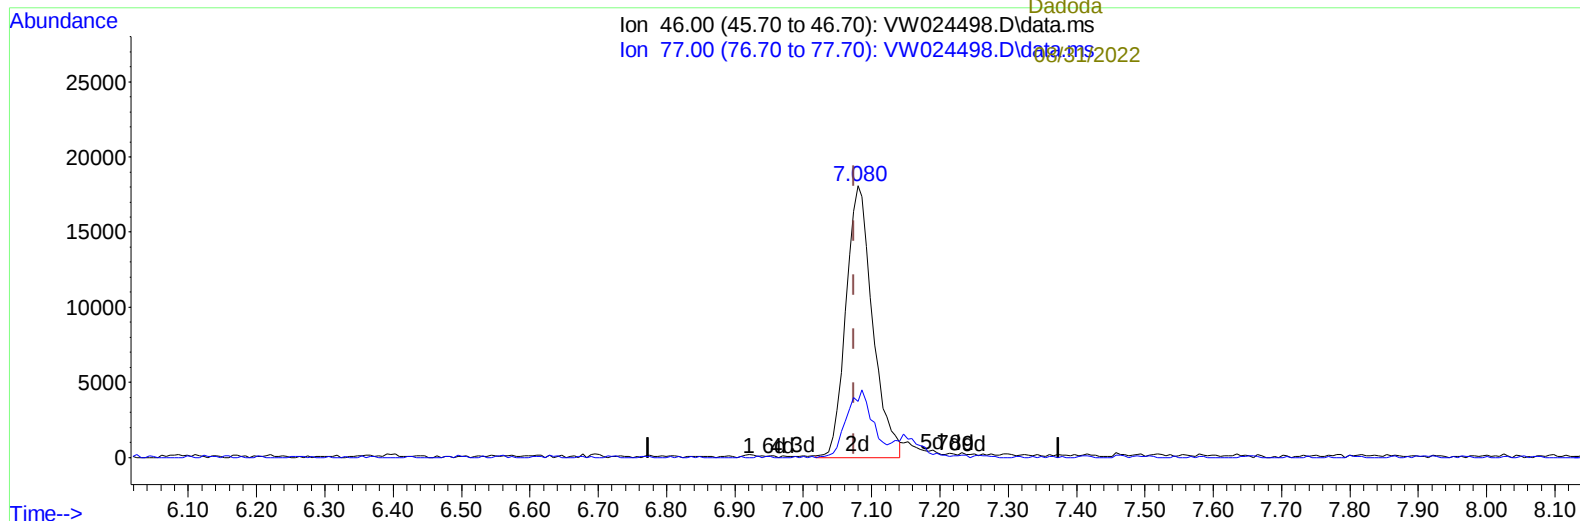

TIC: VW024498.D\data.ms

(21) 2-Butanone-d5 (S)

7.080min (+ 0.006) 49.48 ug/L m

response 49070

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	12.40	0.08#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024498.D
 Acq On : 30 Aug 2022 18:24
 Operator : SY/VA
 Sample : N4440-04
 Misc : 4.60g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 COZK0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/31/2022
 Supervised By :Mahesh Dadoda 08/31/2022

Quant Time: Aug 31 02:56:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 31 02:55:40 2022
 Response via : Initial Calibration

08/31/2022
 Supervised By :Mahesh
 Dadoda

08/31/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----08/31/2022						
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	195335	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	131813	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	26903	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.337	65	190384	35.357	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	141.440%	
7) Chloroethane-d5	2.873	69	134000	33.214	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	132.840%	
11) 1,1-Dichloroethene-d2	4.001	63	131568	28.174	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	112.680%#	
21) 2-Butanone-d5	7.080	46	49070m	49.477	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	98.960%	
24) Chloroform-d	7.647	84	220055	35.041	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	140.160%	
26) 1,2-Dichloroethane-d4	8.305	65	121409	31.880	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	127.520%	
32) Benzene-d6	8.269	84	373343	49.435	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	197.720%#	
36) 1,2-Dichloropropane-d6	9.268	67	124599	53.050	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	212.200%#	
41) Toluene-d8	10.323	98	290680	40.482	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	161.920%#	
43) trans-1,3-Dichloroprop...	10.573	79	36170	32.908	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	131.640%	
47) 2-Hexanone-d5	10.927	63	37837	71.989	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	143.980%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	91961	34.582	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	138.320%#	
66) 1,2-Dichlorobenzene-d4	13.853	152	34437	33.992	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	135.960%#	
Target Compounds						
					Qvalue	
13) Acetone	4.123	43	4287m	7.243	ug/L	
16) Methylene chloride	4.903	84	24596	7.508	ug/L	84
20) cis-1,2-Dichloroethene	7.171	96	7768	2.558	ug/L	90
34) Trichloroethene	9.092	95	42908	19.837	ug/L	92
46) Tetrachloroethene	10.860	164	19192	11.425	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
Data File : VW024498.D
Acq On : 30 Aug 2022 18:24
Operator : SY/VA
Sample : N4440-04
Misc : 4.60g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0ZK0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/31/2022
Supervised By :Mahesh Dadoda 08/31/2022

08/31/2022
Supervised By :Mahesh
Dadoda

08/31/2022

