

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024473.D
 Acq On : 30 Aug 2022 02:40
 Operator : SY/VA
 Sample : N4365-06
 Misc : 5.67g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBVY4

Quant Time: Aug 30 06:29:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 30 00:24:06 2022
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
 Supervised By :Mahesh Dadoda 08/31/2022

Supervised By :Mahesh
 Dadoda
 08/31/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	406256	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	387436	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	168132	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	193197	17.252	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	69.000%		
7) Chloroethane-d5	2.873	69	133592	15.921	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	63.680%		
11) 1,1-Dichloroethene-d2	4.007	63	148173	15.256	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	61.040%		
21) 2-Butanone-d5	7.080	46	55939m	27.119	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	54.240%		
24) Chloroform-d	7.647	84	233856	17.905	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	71.640%		
26) 1,2-Dichloroethane-d4	8.305	65	128816	16.264	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	65.040%#		
32) Benzene-d6	8.275	84	457462	20.608	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	82.440%		
36) 1,2-Dichloropropane-d6	9.275	67	133516	19.340	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	77.360%		
41) Toluene-d8	10.323	98	427312	20.246	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	81.000%		
43) trans-1,3-Dichloroprop...	10.573	79	48635	15.054	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	60.200%		
47) 2-Hexanone-d5	10.921	63	45402	29.389	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	58.780%		
56) 1,1,2,2-Tetrachloroeth...	12.689	84	110810	14.177	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	56.720%		
66) 1,2-Dichlorobenzene-d4	13.853	152	133336	21.059	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	84.240%		
Target Compounds						Qvalue
46) Tetrachloroethene	10.860	164	114073	23.103	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
Data File : VW024473.D
Acq On : 30 Aug 2022 02:40
Operator : SY/VA
Sample : N4365-06
Misc : 5.67g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
DBVY4


Quant Time: Aug 30 06:29:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Aug 30 00:24:06 2022
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 08/30/2022
Supervised By : Mahesh Dadoda 08/31/2022


Supervised By : Mahesh
Dadoda
08/31/2022

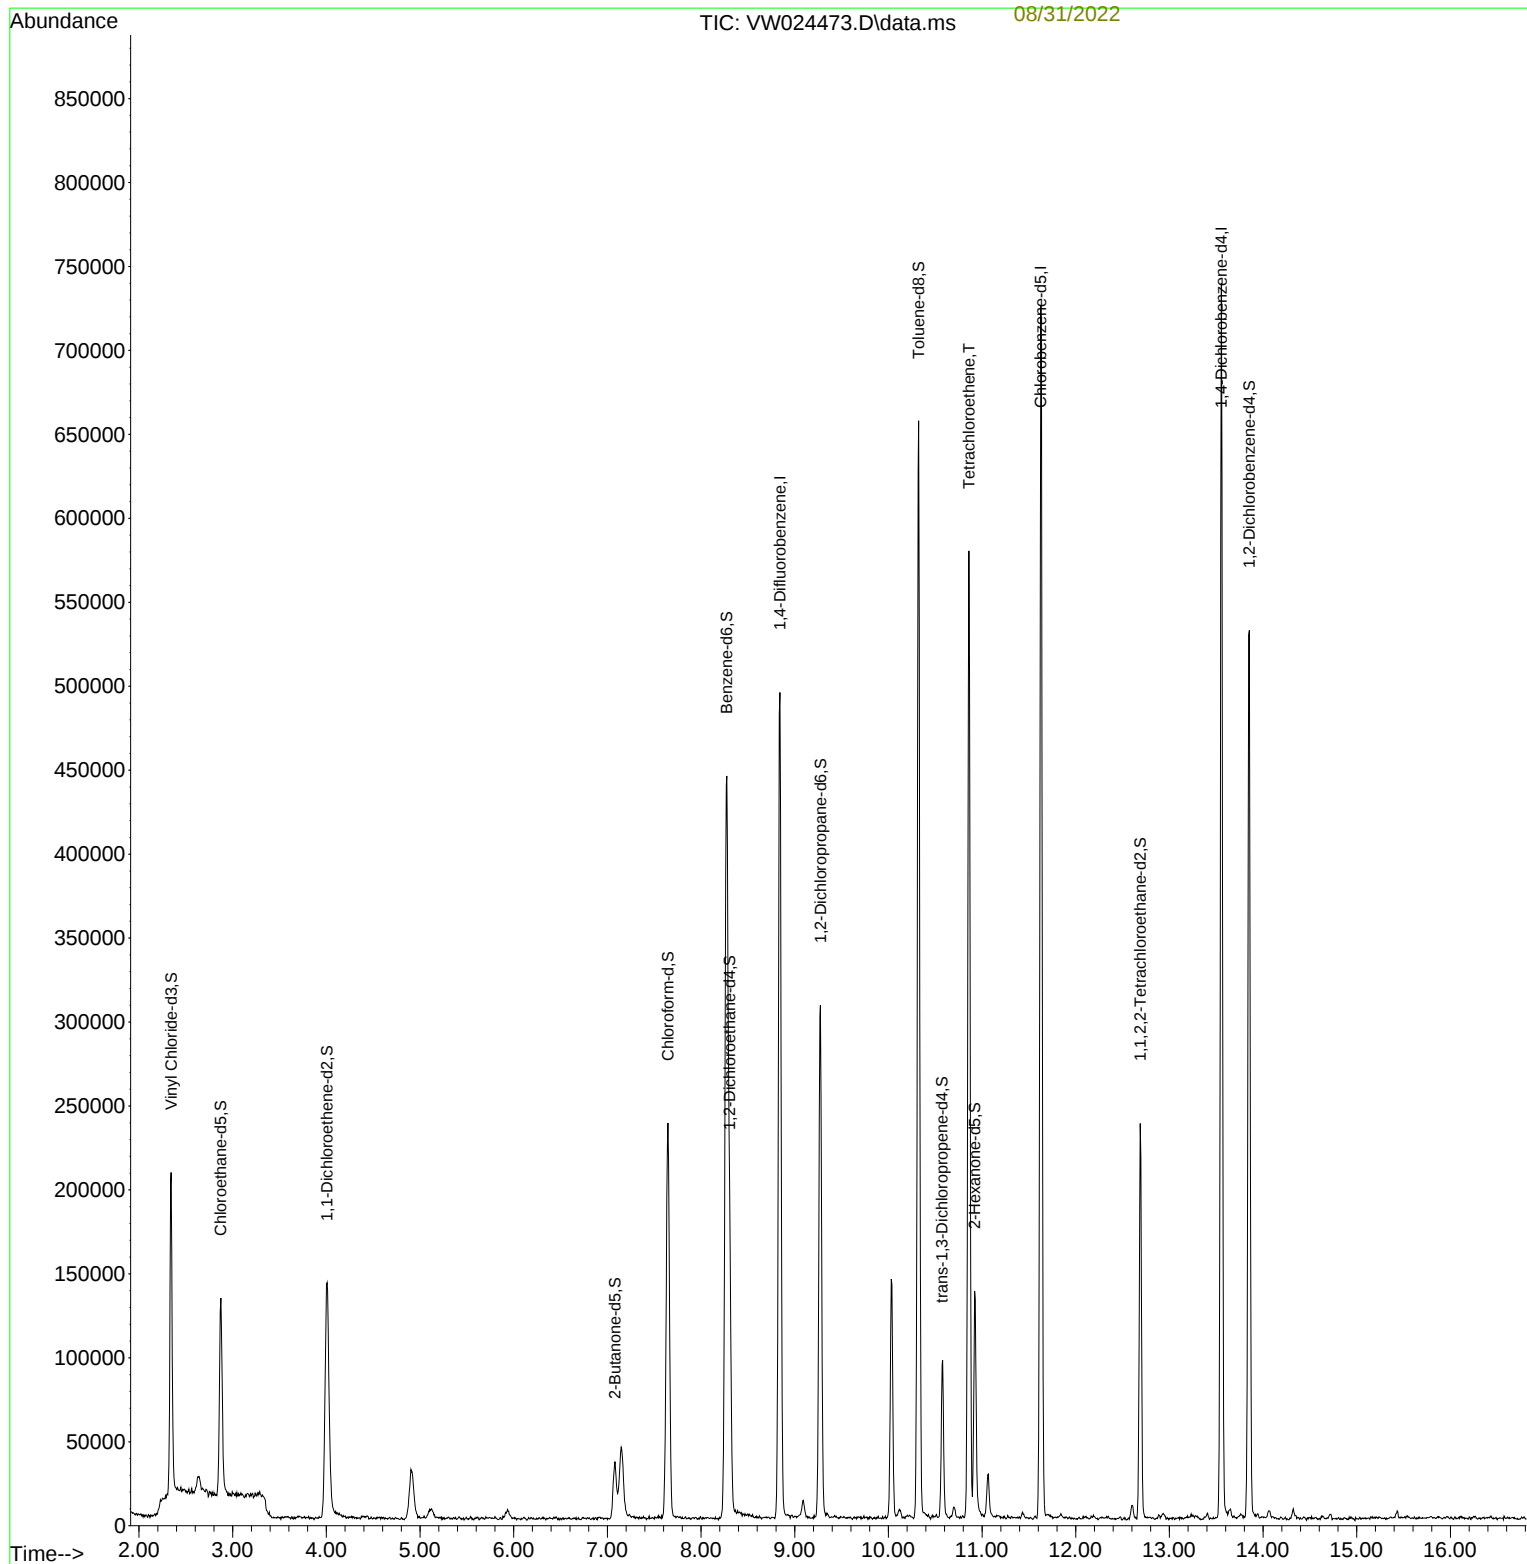

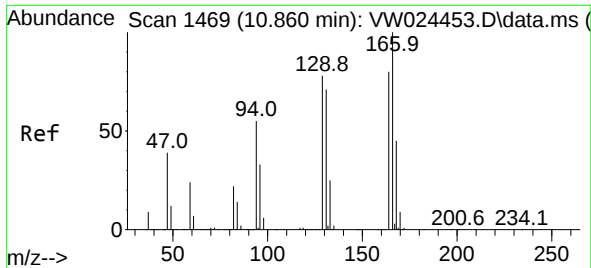

#46
Tetrachloroethene
Concen: 23.103 ug/L
RT: 10.860 min Scan# 1469
Delta R.T. 0.000 min
Lab File: VW024473.D
Acq: 30 Aug 2022 02:40



Instrument :
MSVOA_W
ClientSampleId :
DBVY4

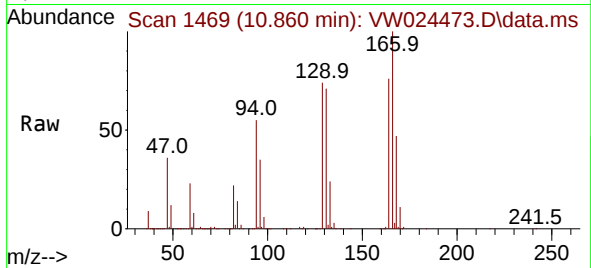

Tgt Ion:164 Resp: 114073
Ion Ratio Lower Upper
164 100
129 97.0 72.9 135.3
131 93.9 63.7 118.3
166 131.5 86.2 160.0

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 08/30/2022
Supervised By :Mahesh Dadoda 08/31/2022

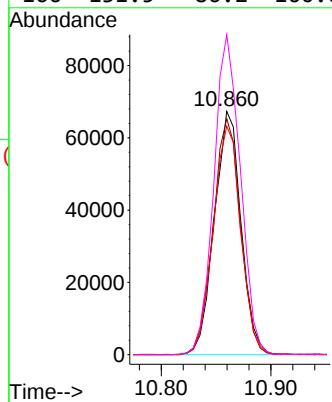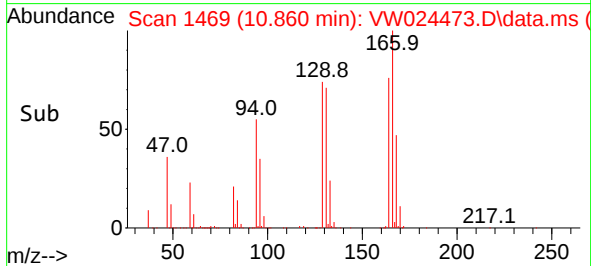

Supervised By :Mahesh
Dadoda
08/31/2022