

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
 Data File : VW024481.D
 Acq On : 30 Aug 2022 08:50
 Operator : SY/VA
 Sample : N4319-11
 Misc : 4.67g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0ZJ5

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 08/31/2022
 Supervised By :Mahesh Dadoda 08/31/2022

Quant Time: Aug 31 01:18:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Aug 30 07:05:43 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	331419	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	310085	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	123092	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	169408	18.543	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	74.160%		
7) Chloroethane-d5	2.873	69	101835	14.877	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	59.520%		
11) 1,1-Dichloroethene-d2	4.001	63	137206	17.317	ug/L	-0.01
Spiked Amount 25.000	Range 45 - 110		Recovery =	69.280%		
21) 2-Butanone-d5	7.080	46	37647	22.373	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	44.740%		
24) Chloroform-d	7.647	84	198493	18.629	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	74.520%		
26) 1,2-Dichloroethane-d4	8.299	65	104299m	16.142	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	64.560%#		
32) Benzene-d6	8.268	84	390252	21.966	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	87.880%		
36) 1,2-Dichloropropane-d6	9.268	67	111110	20.109	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	80.440%		
41) Toluene-d8	10.323	98	347923	20.597	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	82.400%		
43) trans-1,3-Dichloroprop...	10.573	79	41485	16.044	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	64.160%		
47) 2-Hexanone-d5	10.920	63	28915	23.386	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	46.780%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	78027	12.473	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	49.880%		
66) 1,2-Dichlorobenzene-d4	13.853	152	92677	19.994	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	79.960%		
Target Compounds					Qvalue	
13) Acetone	4.123	43	9500	9.460	ug/L	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082922\
Data File : VW024481.D
Acq On : 30 Aug 2022 08:50
Operator : SY/VA
Sample : N4319-11
Misc : 4.67g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
C0ZJ5

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 08/31/2022
Supervised By :Mahesh Dadoda 08/31/2022


Quant Time: Aug 31 01:18:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Aug 30 07:05:43 2022
Response via : Initial Calibration

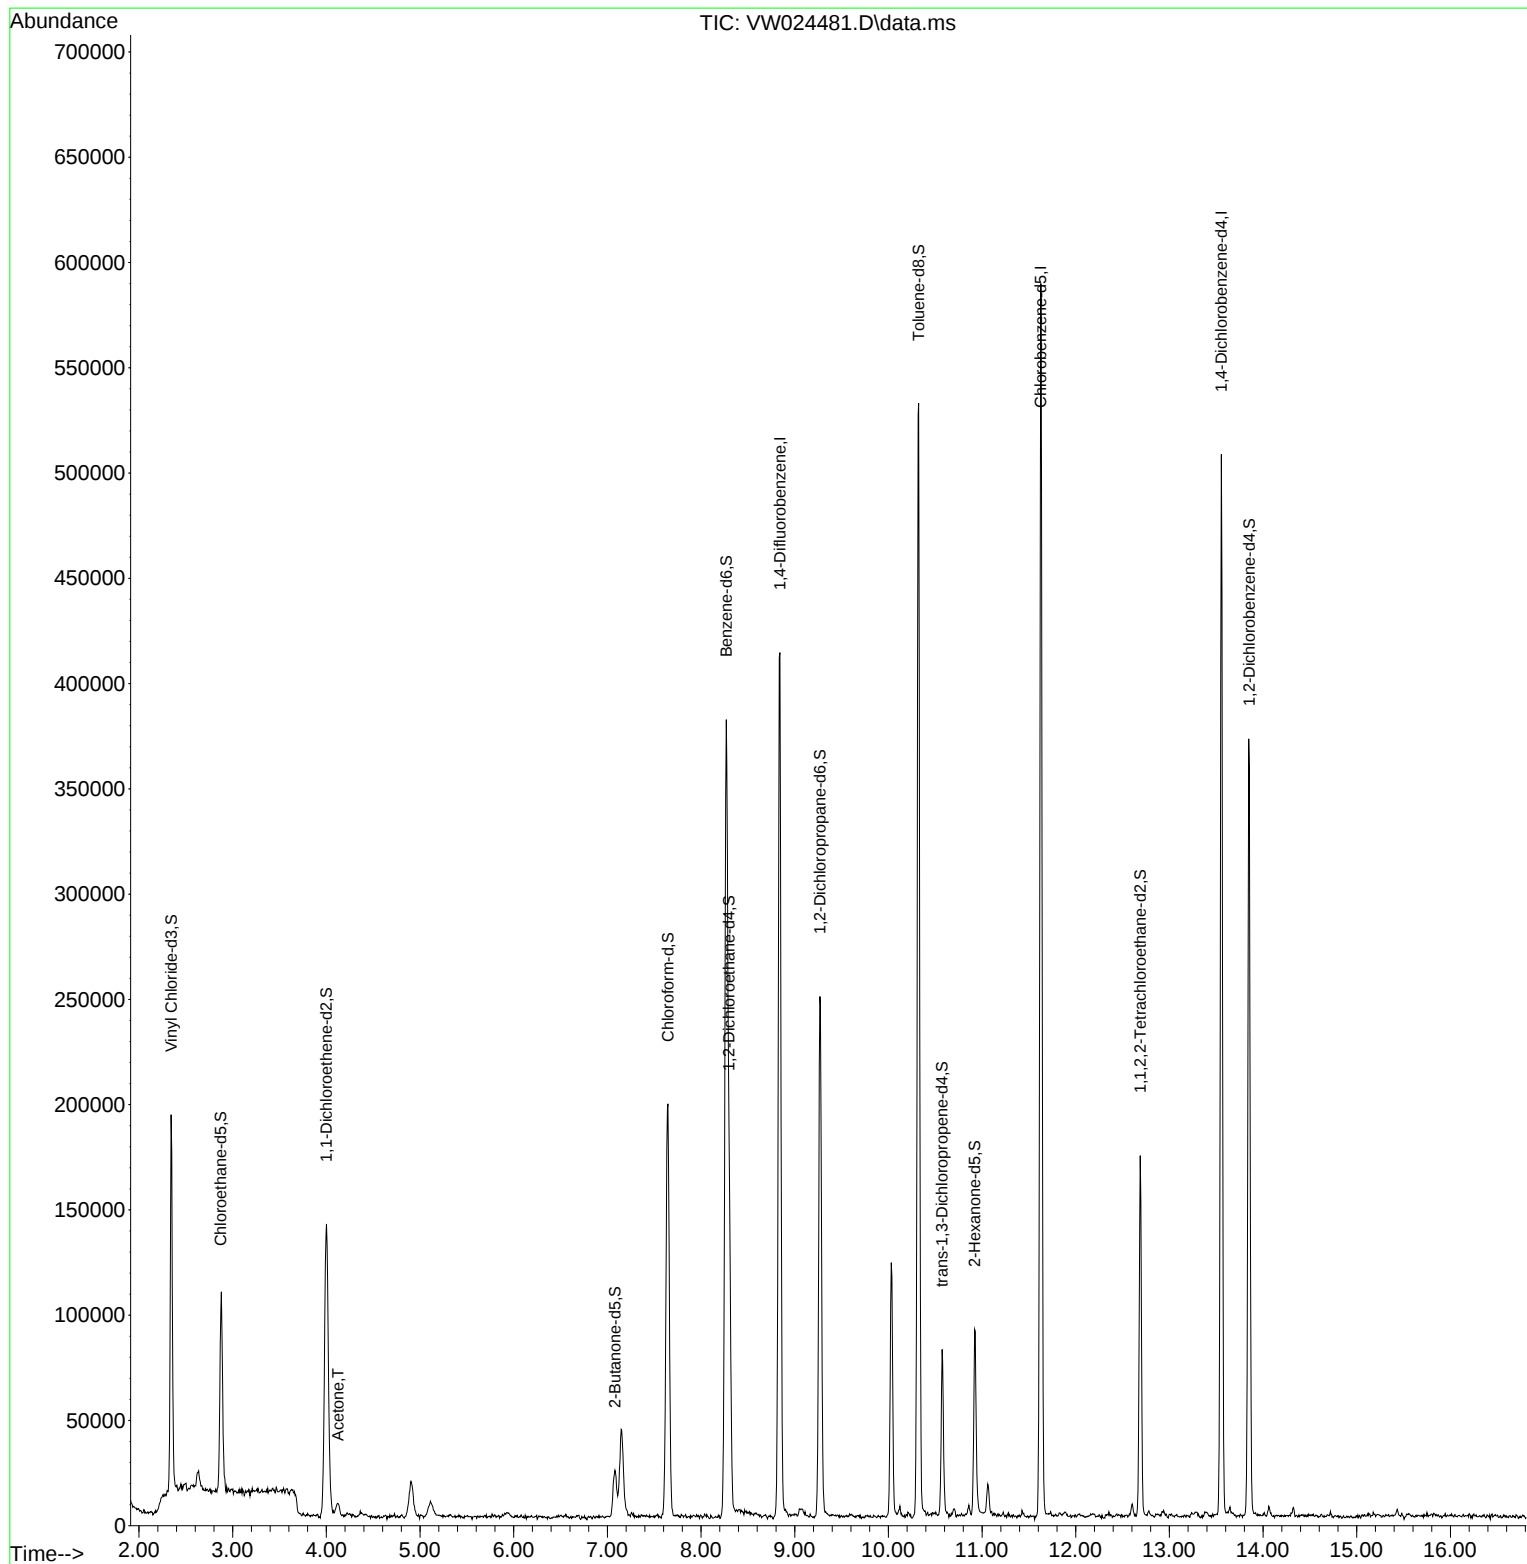

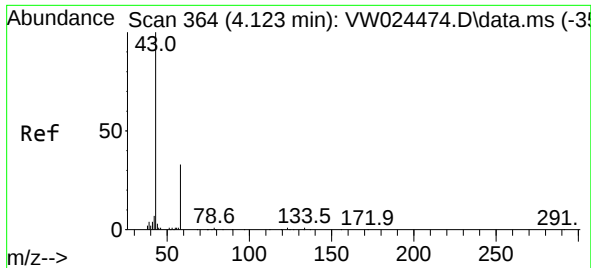

#13
 Acetone
 Concen: 9.460 ug/L
 RT: 4.123 min Scan# 30
 Delta R.T. 0.000 min
 Lab File: VW024481.D
 Acq: 30 Aug 2022 08:50

Instrument :
 MSVOA_W
 ClientSampleId :
 C0ZJ5

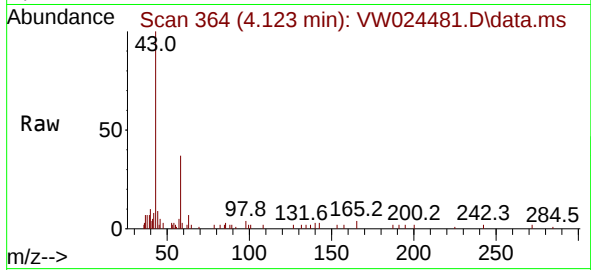

Tgt Ion: 43 Resp: 9500
 Ion Ratio Lower Upper
 43 100
 58 35.2 0.0 58.4

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 08/31/2022
 Supervised By :Mahesh Dadoda 08/31/2022

