

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082924\
 Data File : VW030095.D
 Acq On : 29 Aug 2024 13:21
 Operator : SY/MD
 Sample : P3722-04
 Misc : 5.00g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Quant Time: Aug 29 21:33:10 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Aug 29 21:32:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	176995	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	166519	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	69865	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	61871	23.490	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.960%
7) Chloroethane-d5	2.899	69	47057	25.173	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	100.680%
11) 1,1-Dichloroethene-d2	4.027	65	27730	24.642	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	98.560%
21) 2-Butanone-d5	7.075	46	30171	57.463	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	114.920%
24) Chloroform-d	7.648	84	126202	26.441	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	105.760%
26) 1,2-Dichloroethane-d4	8.307	65	70020	28.891	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	115.560%
32) Benzene-d6	8.276	84	250111	25.446	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	101.800%
36) 1,2-Dichloropropane-d6	9.270	67	79584	27.636	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	110.560%
41) Toluene-d8	10.325	98	227344	25.412	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	101.640%
43) trans-1,3-Dichloroprop...	10.575	79	29718	25.087	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	100.360%
47) 2-Hexanone-d5	10.922	63	23702	53.778	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	107.560%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	58952	27.804	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	111.200%
66) 1,2-Dichlorobenzene-d4	13.848	152	70210	27.783	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	111.120%
Target Compounds						Qvalue
16) Methylene chloride	4.917	84	6458	2.209	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082924\
Data File : VW030095.D
Acq On : 29 Aug 2024 13:21
Operator : SY/MD
Sample : P3722-04
Misc : 5.00g/10mL/MSVOA_W/SOIL/A
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001


Quant Time: Aug 29 21:33:10 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Aug 29 21:32:12 2024
Response via : Initial Calibration

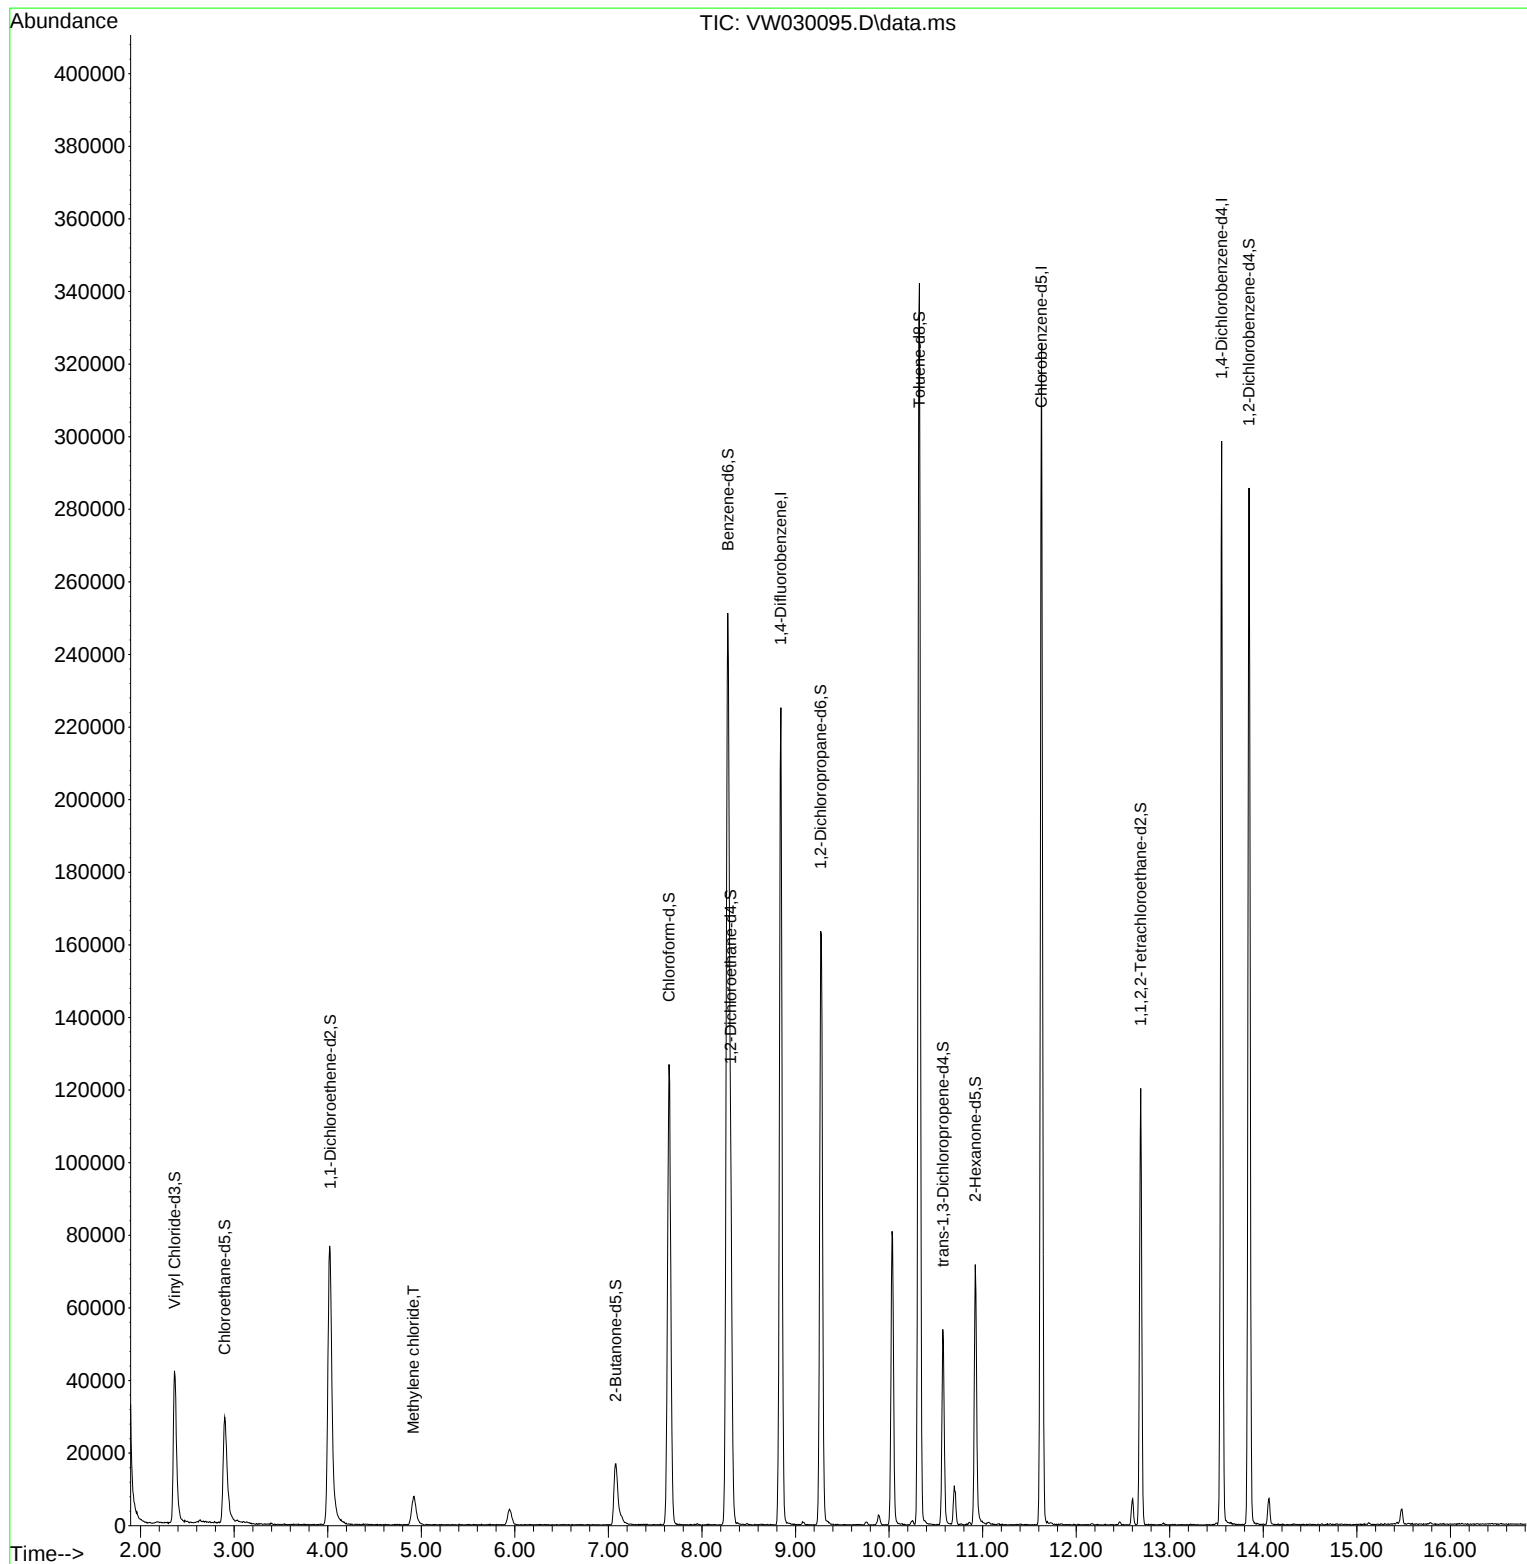

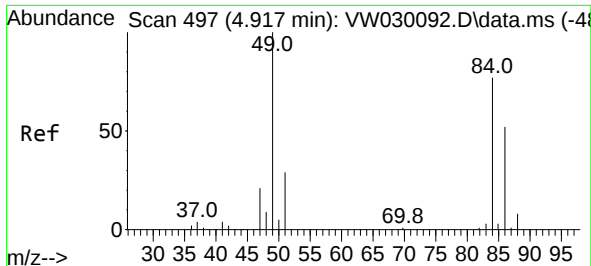

#16
Methylene chloride
Concen: 2.209 ug/L
RT: 4.917 min Scan# 49
Delta R.T. -0.000 min
Lab File: VW030095.D
Acq: 29 Aug 2024 13:21

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

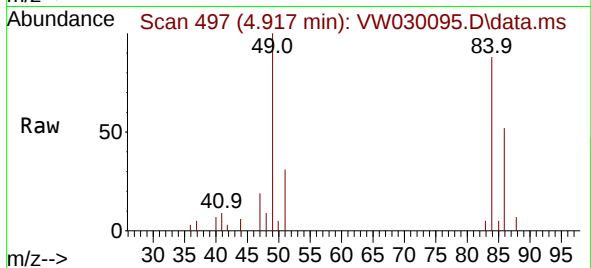

Tgt Ion: 84 Resp: 6458

Ion	Ratio	Lower	Upper
84	100		
86	59.6	44.2	82.2
49	113.5	79.9	148.3

