
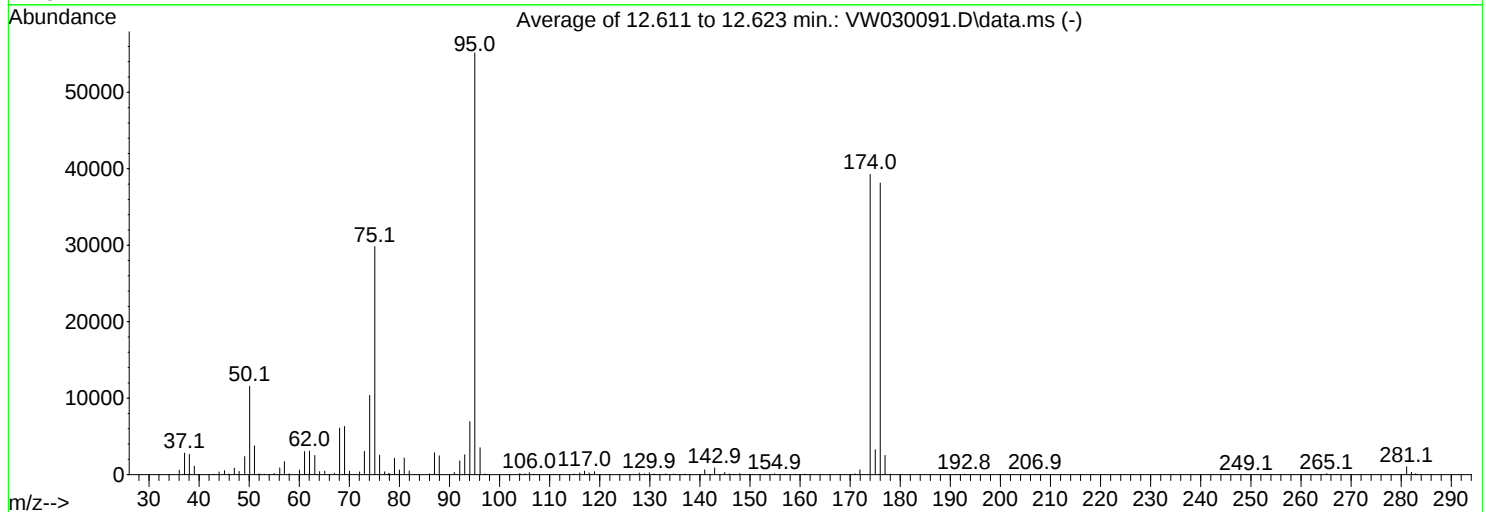


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW082924\
Data File : VW030091.D
Acq On : 29 Aug 2024 10:54
Operator : SY/MD
Sample : BFB554
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB554

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
Title : SFAM01.0
Last Update : Thu Aug 29 21:32:12 2024

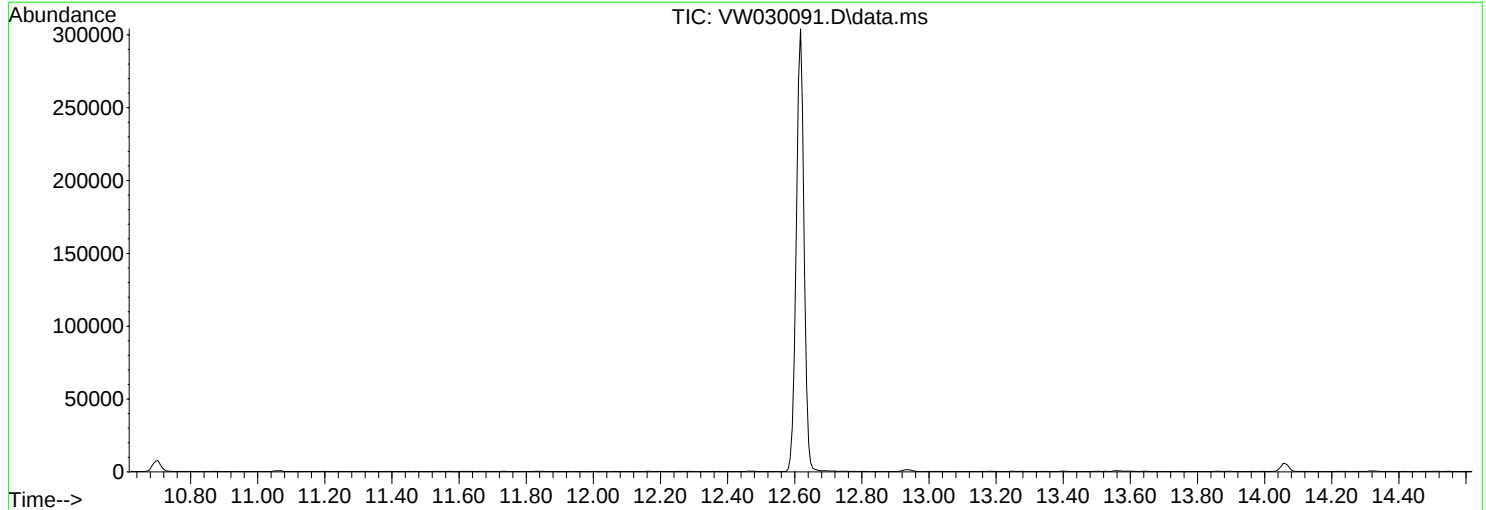

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1752

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	11564	PASS
75	95	30	80	54.1	29835	PASS
95	95	100	100	100.0	55160	PASS
96	95	5	9	6.4	3507	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	71.2	39283	PASS
175	174	5	9	8.3	3269	PASS
176	174	95	101	97.1	38147	PASS
177	176	5	9	6.6	2511	PASS

m/z	Abundance
40.00	153.0
44.00	117.0

Instrument :
MSVOA_W
ClientSampleId :
BFB554

m/z	Abundance
36.10	710.0
37.10	3199.0
38.10	2605.0
39.10	1139.0
39.90	193.0
42.90	60.0
44.10	513.0
45.10	594.0
46.00	82.0
47.10	886.0
48.00	483.0
49.10	2429.0
50.10	11935.0
51.00	3887.0
52.00	183.0
53.00	76.0
53.90	67.0
54.90	168.0
56.10	1034.0
57.00	1826.0
57.90	129.0
60.10	592.0
61.00	3333.0
62.00	3025.0
63.10	2742.0
64.10	460.0
65.10	620.0
67.00	211.0
68.10	6349.0
69.10	6262.0
70.00	432.0
72.10	362.0
73.00	3063.0
74.00	10407.0
75.10	29632.0
76.10	2733.0
77.00	427.0
78.10	296.0
79.00	2276.0
80.00	574.0
81.00	2065.0
82.00	553.0
86.10	64.0
87.00	2886.0
88.00	2573.0
91.00	292.0
92.00	1803.0
93.10	2367.0
94.10	6590.0
95.00	53208.0
96.10	3322.0
97.10	84.0
103.90	229.0
105.00	94.0
105.90	252.0
110.80	62.0
114.90	83.0
116.00	208.0
117.00	505.0
117.90	237.0
119.10	412.0
127.90	139.0
129.10	111.0
129.90	199.0
130.80	98.0
132.80	123.0
133.30	136.0
135.10	125.0
136.90	97.0
140.90	502.0
142.00	113.0
143.00	876.0
144.90	352.0
145.80	103.0
146.70	65.0
147.90	90.0
149.90	78.0
152.80	66.0
154.80	120.0
156.80	81.0
160.80	74.0
171.00	146.0
172.00	550.0
174.00	36816.0
175.00	2793.0
176.00	34488.0
177.00	2357.0
178.00	88.0
191.00	120.0
192.80	176.0
207.00	96.0
208.00	53.0

Instrument :
MSVOA_W
ClientSampleId :
BFB554

249.10	123.0
265.20	235.0
265.90	52.0
267.00	60.0
281.10	1524.0
282.20	392.0
282.90	308.0
284.10	78.0

Instrument :
MSVOA_W
ClientSampleId :
BFB554

m/z	Abundance
36.00	522.0
37.10	3103.0
38.10	3157.0
39.00	1136.0
40.00	145.0
43.10	96.0
44.10	511.0
45.10	571.0
45.90	92.0
47.10	897.0
48.00	495.0
49.10	2572.0
50.10	13192.0
51.10	3990.0
52.20	175.0
53.00	66.0
53.90	57.0
55.00	204.0
56.10	943.0
57.10	1943.0
58.00	101.0
60.10	685.0
61.10	3234.0
62.10	3425.0
63.10	2915.0
64.00	437.0
65.10	484.0
67.00	201.0
68.00	6884.0
69.00	7100.0
70.00	616.0
72.00	420.0
73.00	3279.0
74.00	11650.0
75.10	34608.0
76.00	2744.0
77.10	440.0
77.80	236.0
79.00	2305.0
80.00	679.0
80.90	2505.0
81.90	514.0
83.00	54.0
86.00	147.0
87.00	3236.0
88.00	2780.0
91.00	296.0
92.00	1934.0
93.10	2776.0
94.00	8294.0
95.00	61760.0
96.10	4118.0
97.30	107.0
104.10	165.0
105.10	120.0
106.00	296.0
106.80	96.0
110.80	88.0
114.80	93.0
115.90	232.0
117.00	483.0
117.90	273.0
118.90	345.0
128.00	244.0
128.90	70.0
129.90	311.0
130.80	115.0
133.10	118.0
134.80	145.0
136.90	122.0
141.00	779.0
142.90	1002.0
144.00	64.0
145.00	269.0
145.90	154.0
147.00	65.0
148.00	176.0
148.80	70.0
149.90	83.0
154.90	132.0
157.00	83.0
159.00	101.0
161.10	102.0
170.20	66.0
171.00	177.0
172.00	752.0
174.00	43288.0
175.00	3727.0
176.00	40072.0
177.00	2742.0
178.00	120.0
193.10	84.0

Instrument :
MSVOA_W
ClientSampleId :
BFB554

265.10	135.0
281.10	1138.0
282.00	317.0
283.20	208.0

Instrument :
MSVOA_W
ClientSampleId :
BFB554

m/z	Abundance
36.00	503.0
37.10	2196.0
38.00	2182.0
39.10	1046.0
39.90	180.0
43.90	416.0
45.10	383.0
45.80	75.0
47.00	797.0
48.10	307.0
49.10	2103.0
50.10	9566.0
51.00	3451.0
51.90	143.0
53.00	65.0
55.10	163.0
56.10	672.0
57.10	1353.0
57.90	73.0
60.00	471.0
61.00	2507.0
62.00	2770.0
63.00	1870.0
64.00	297.0
65.10	301.0
67.00	176.0
68.00	5044.0
69.10	5507.0
70.10	361.0
72.00	315.0
73.00	2792.0
74.10	9026.0
75.10	25264.0
76.10	2165.0
77.00	266.0
77.90	290.0
79.00	1909.0
80.00	570.0
81.00	1938.0
82.00	400.0
86.00	145.0
87.00	2495.0
87.90	2059.0
90.90	274.0
92.10	1633.0
93.00	2667.0
94.10	5975.0
95.10	50512.0
96.10	3082.0
97.00	152.0
104.00	235.0
105.10	90.0
105.90	246.0
106.80	79.0
114.80	97.0
116.10	235.0
116.90	368.0
117.90	211.0
118.90	406.0
127.80	261.0
128.90	114.0
129.90	255.0
130.90	83.0
133.20	60.0
134.70	135.0
137.10	105.0
141.00	598.0
143.00	765.0
145.00	233.0
145.80	80.0
148.00	112.0
149.90	53.0
155.00	125.0
156.80	74.0
159.00	75.0
160.90	95.0
170.20	57.0
170.80	72.0
171.90	578.0
174.00	37744.0
175.00	3288.0
176.00	39880.0
176.90	2433.0
177.90	59.0
206.90	73.0
265.00	59.0
281.10	410.0
281.90	120.0
282.10	122.0
283.00	68.0

Instrument :
MSVOA_W
ClientSampleId :
BFB554