




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW083024\
Data File : VW030114.D
Acq On : 30 Aug 2024 13:04
Operator : SY/MD
Sample : P3733-20 RE
Misc : 3.76g/10mL/MSVOA_W/SOIL/B
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A44B5RE

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 09/03/2024
Supervised By :Mahesh Dadoda 09/04/2024

Quant Time: Aug 30 23:55:23 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 30 23:54:36 2024
Response via : Initial Calibration

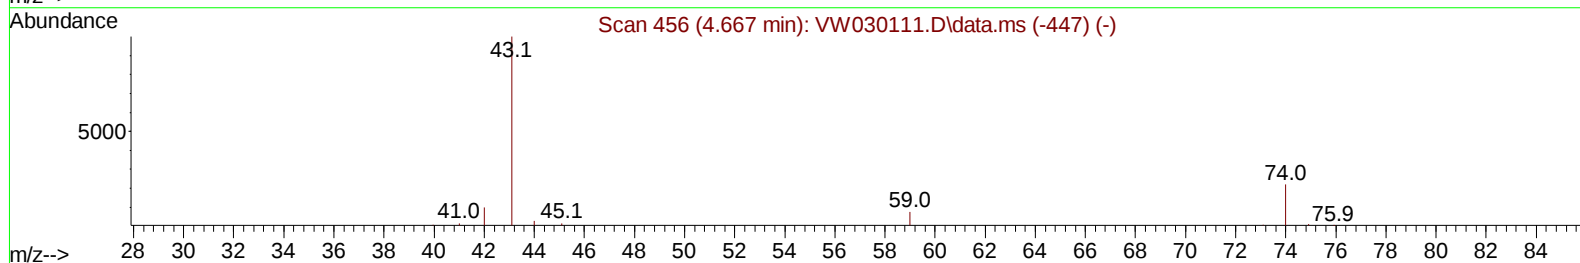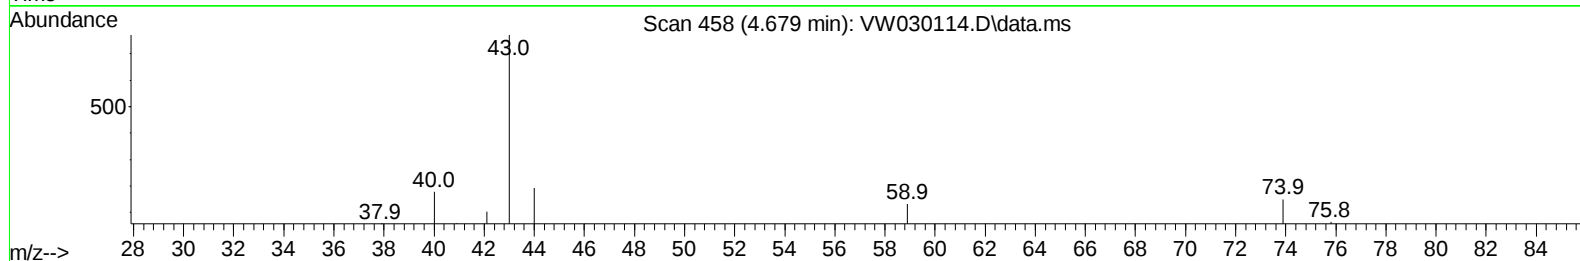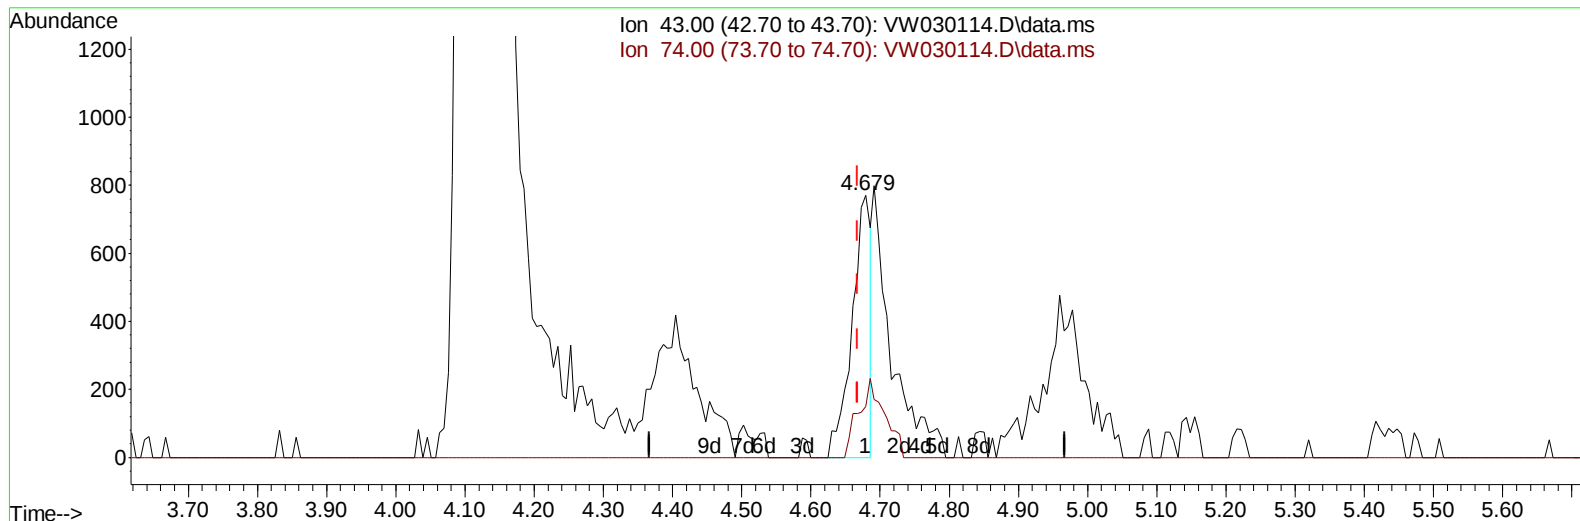

TIC: VW030114.D\data.ms

(15) Methyl Acetate (T)

4.679min (+ 0.012) 1.36 ug/L

response 1427

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	24.90	12.89#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW083024\
Data File : VW030114.D
Acq On : 30 Aug 2024 13:04
Operator : SY/MD
Sample : P3733-20 RE
Misc : 3.76g/10mL/MSVOA_W/SOIL/B
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A44B5RE

Manual IntegrationsAPPROVED

Quant Time: Aug 30 23:55:23 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 30 23:54:36 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 09/03/2024
Supervised By :Mahesh Dadoda 09/04/2024

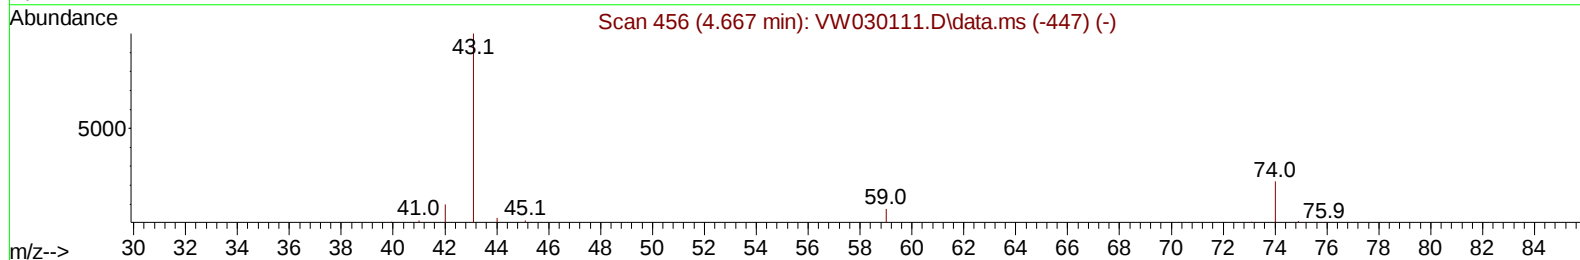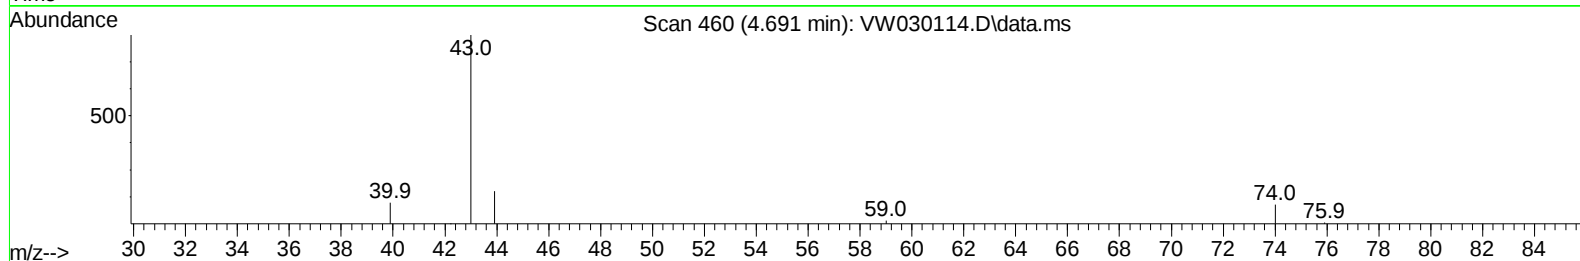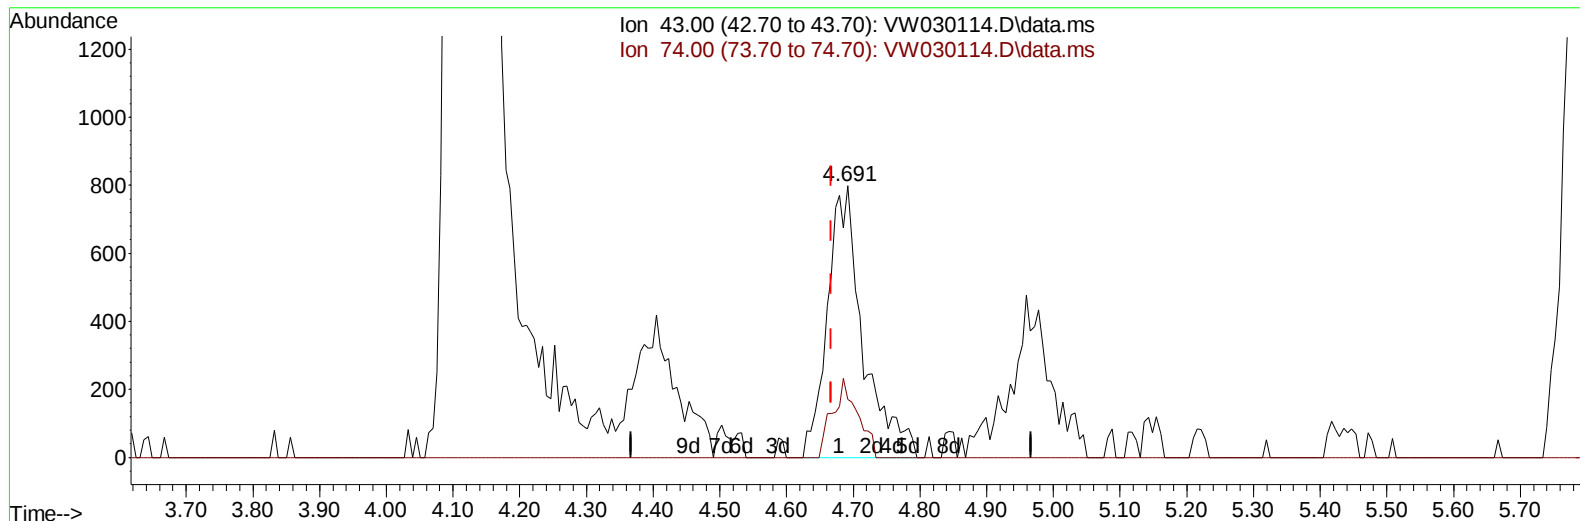

TIC: VW030114.D\data.ms

(15) Methyl Acetate (T)

4.691min (+ 0.024) 2.81 ug/L m

response 2948

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	24.90	6.24#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW083024\
 Data File : VW030114.D
 Acq On : 30 Aug 2024 13:04
 Operator : SY/MD
 Sample : P3733-20RE
 Misc : 3.76g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A44B5RE

Manual IntegrationsAPPROVED

Quant Time: Aug 30 23:55:23 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 30 23:54:36 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 09/03/2024
 Supervised By :Mahesh Dadoda 09/04/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	198660	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	107596	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	21821	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	70686	23.910	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	95.640%	
7) Chloroethane-d5	2.899	69	57591	27.448	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	109.800%	
11) 1,1-Dichloroethene-d2	4.027	65	31669	25.073	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	100.280%	
21) 2-Butanone-d5	7.075	46	40526	68.768	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	137.540%#	
24) Chloroform-d	7.648	84	127833	23.861	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	95.440%	
26) 1,2-Dichloroethane-d4	8.307	65	69496	25.547	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	102.200%	
32) Benzene-d6	8.276	84	233289	36.732	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	146.920%#	
36) 1,2-Dichloropropane-d6	9.276	67	77253	41.517	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	166.080%#	
41) Toluene-d8	10.325	98	158868	27.483	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	109.920%	
43) trans-1,3-Dichloroprop...	10.575	79	20523	26.813	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	107.240%	
47) 2-Hexanone-d5	10.922	63	25486	89.492	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	178.980%#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	30805	22.485	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	89.960%	
66) 1,2-Dichlorobenzene-d4	13.848	152	13103	16.601	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	66.400%#	
Target Compounds						
						Qvalue
13) Acetone	4.118	43	54468	101.050	ug/L	99
14) Carbon disulfide	4.387	76	87494	11.076	ug/L	98
15) Methyl Acetate	4.691	43	2948m	2.805	ug/L	
22) 2-Butanone	7.179	43	13171	17.076	ug/L	94
33) Benzene	8.325	78	13896	2.016	ug/L	100
42) Toluene	10.386	91	14817	2.018	ug/L	95
46) Tetrachloroethene	10.861	164	1144	0.812	ug/L	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW083024\
Data File : VW030114.D
Acq On : 30 Aug 2024 13:04
Operator : SY/MD
Sample : P3733-20 RE
Misc : 3.76g/10mL/MSVOA_W/SOIL/B
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A44B5RE

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 09/03/2024
Supervised By :Mahesh Dadoda 09/04/2024

Quant Time: Aug 30 23:55:23 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 30 23:54:36 2024
Response via : Initial Calibration

