
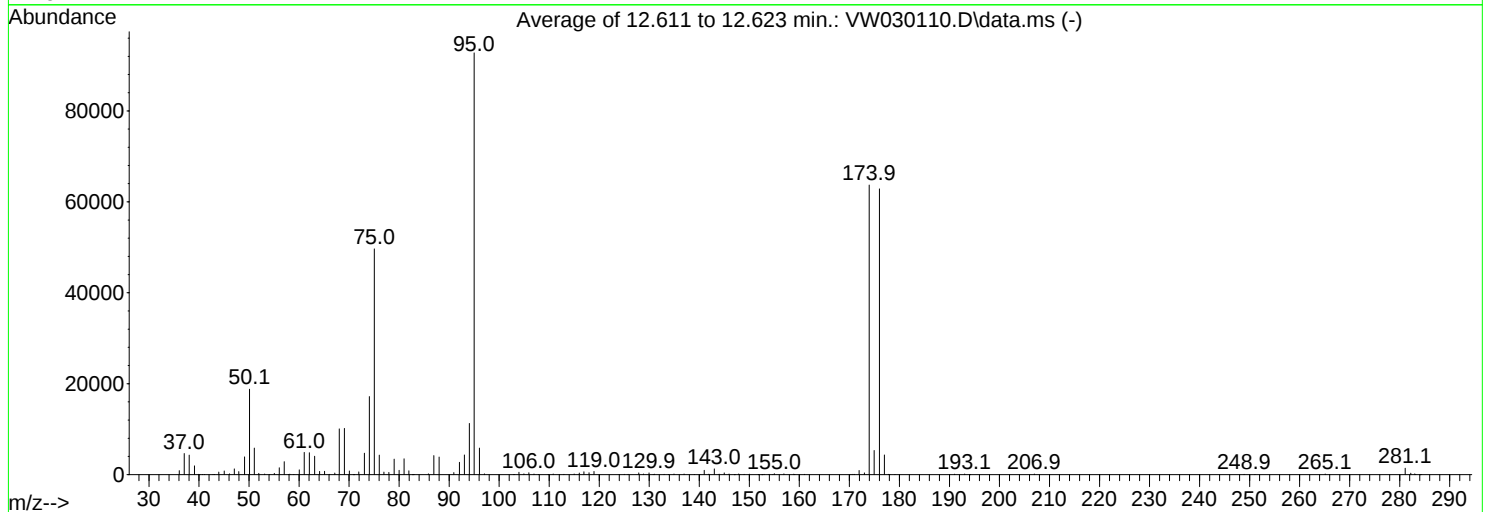


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW083024\
Data File : VW030110.D
Acq On : 30 Aug 2024 10:34
Operator : SY/MD
Sample : BFB555
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB555

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
Title : SFAM01.0
Last Update : Fri Aug 30 23:54:36 2024

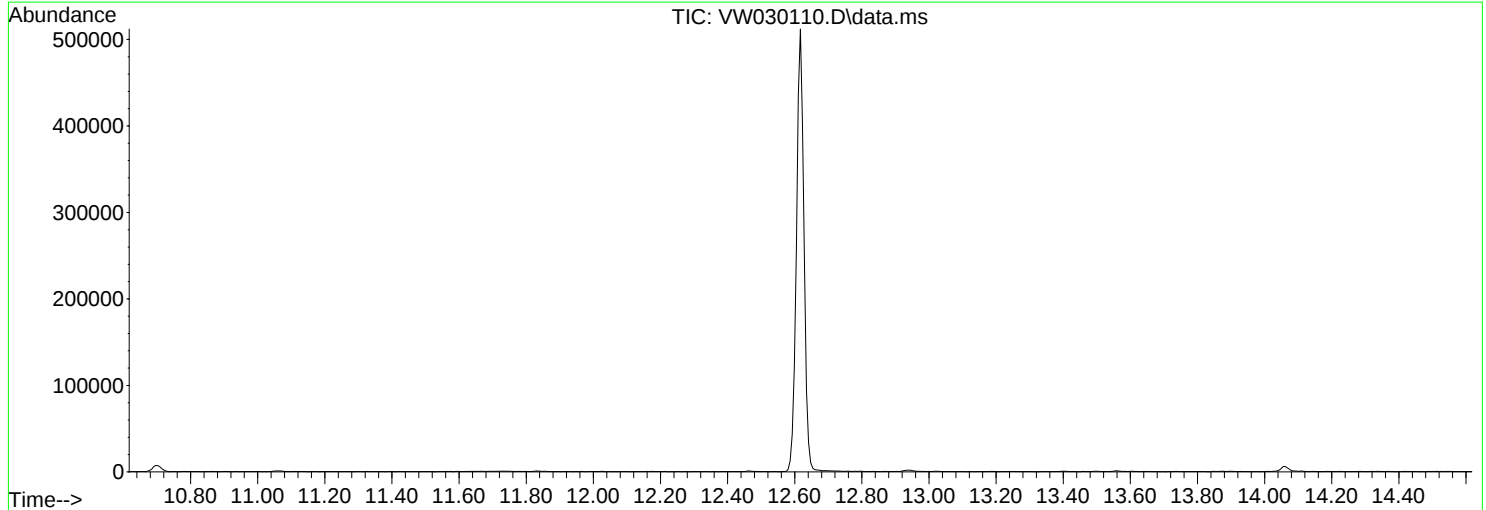

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.3	18792	PASS
75	95	30	80	53.5	49661	PASS
95	95	100	100	100.0	92768	PASS
96	95	5	9	6.3	5853	PASS
173	174	0.00	2	0.6	385	PASS
174	95	50	120	68.7	63709	PASS
175	174	5	9	8.4	5321	PASS
176	174	95	101	98.6	62840	PASS
177	176	5	9	6.9	4338	PASS

m/z	Abundance
40.00	133.0
42.20	50.0
43.90	122.0
56.90	53.0

Instrument :
MSVOA_W
ClientSampleId :
BFB555

m/z	Abundance
36.10	955.0
37.00	4995.0
38.00	4518.0
39.10	2173.0
39.90	193.0
41.10	97.0
42.80	76.0
44.00	681.0
45.10	826.0
46.00	183.0
47.10	1367.0
48.00	608.0
49.10	3731.0
50.10	18480.0
51.00	5921.0
52.00	234.0
53.10	214.0
54.10	57.0
55.10	302.0
56.00	1514.0
57.10	2704.0
57.90	112.0
58.20	100.0
58.90	53.0
60.00	1145.0
61.00	5141.0
62.10	5079.0
63.10	4159.0
64.10	812.0
65.20	820.0
66.00	73.0
67.10	364.0
68.00	9862.0
69.10	10924.0
70.10	807.0
70.90	58.0
71.90	587.0
73.00	4848.0
74.00	16792.0
75.10	49264.0
76.00	4137.0
77.00	498.0
77.90	530.0
79.00	3380.0
80.00	720.0
81.00	3501.0
82.00	835.0
82.70	51.0
85.80	223.0
86.90	3743.0
88.00	3732.0
91.00	486.0
92.00	2599.0
93.10	4656.0
94.00	10583.0
95.00	89272.0
96.00	5783.0
97.00	175.0
102.90	101.0
103.90	506.0
105.00	169.0
106.00	383.0
107.00	111.0
107.90	72.0
109.80	111.0
110.90	124.0
113.00	72.0
115.10	140.0
116.00	284.0
116.90	708.0
117.90	369.0
118.90	667.0
124.00	61.0
125.10	96.0
127.90	333.0
129.00	96.0
129.90	360.0
130.80	102.0
132.90	106.0
133.80	58.0
134.90	169.0
136.90	112.0
139.00	61.0
141.00	872.0
141.90	120.0
143.00	1247.0
144.00	68.0
145.00	541.0
145.90	154.0
147.00	55.0
147.90	309.0
148.90	64.0

Instrument :
MSVOA_W
ClientSampleId :
BFB555

150.00	60.0
152.50	52.0
153.00	85.0
153.90	68.0
154.70	143.0
155.10	149.0
156.90	109.0
158.90	106.0
160.90	80.0
171.00	178.0
171.90	1032.0
173.00	1155.0
173.90	56872.0
174.90	4549.0
176.00	57264.0
177.00	4193.0
177.90	141.0
179.10	90.0
191.00	208.0
193.10	229.0
194.00	52.0
207.10	181.0
248.90	137.0
251.00	87.0
265.10	283.0
266.00	76.0
281.10	2289.0
282.20	493.0
283.00	365.0
284.40	78.0

Instrument :
MSVOA_W
ClientSampleId :
BFB555

m/z	Abundance
36.00	897.0
37.00	5049.0
38.00	4694.0
39.10	1927.0
40.10	220.0
43.10	74.0
44.00	803.0
45.00	980.0
46.10	175.0
47.10	1233.0
47.90	800.0
49.10	4641.0
50.10	21392.0
51.10	6649.0
51.90	286.0
53.20	103.0
54.10	69.0
55.00	353.0
56.10	1855.0
57.10	3211.0
58.10	154.0
59.00	51.0
60.00	1215.0
61.10	5728.0
62.00	5073.0
63.10	4560.0
64.10	752.0
65.00	818.0
66.10	111.0
67.10	365.0
68.10	11347.0
69.10	11074.0
70.10	941.0
72.00	602.0
73.10	5158.0
74.10	19664.0
75.00	55648.0
76.10	5094.0
76.90	690.0
78.00	534.0
79.00	3873.0
80.00	1278.0
81.00	3890.0
81.90	912.0
85.90	205.0
87.00	4859.0
88.00	4410.0
90.90	518.0
92.00	3115.0
93.00	4591.0
94.10	12860.0
95.00	105240.0
96.00	6694.0
97.10	220.0
103.10	71.0
103.90	605.0
104.90	235.0
106.00	444.0
106.90	175.0
110.00	108.0
110.80	167.0
112.10	50.0
112.90	105.0
114.90	183.0
116.00	386.0
117.00	620.0
117.90	536.0
119.00	750.0
124.00	58.0
124.90	76.0
125.70	71.0
127.90	484.0
128.80	173.0
130.00	367.0
131.00	147.0
133.00	76.0
133.90	56.0
134.90	182.0
137.00	153.0
139.00	59.0
140.10	103.0
141.00	1074.0
141.90	173.0
143.00	1358.0
143.90	137.0
145.00	351.0
146.00	157.0
147.70	146.0
149.00	88.0
150.10	120.0
153.00	84.0
154.00	74.0

Instrument :
MSVOA_W
ClientSampleId :
BFB555

154.90	222.0
156.90	250.0
158.90	171.0
161.00	65.0
170.70	175.0
171.90	988.0
174.00	75880.0
175.00	5940.0
176.00	73136.0
177.00	4645.0
177.80	116.0
191.10	97.0
193.00	163.0
206.90	147.0
248.90	113.0
251.10	53.0
265.20	94.0
281.10	1419.0
282.20	365.0
283.00	196.0

Instrument :
MSVOA_W
ClientSampleId :
BFB555

m/z	Abundance
36.00	748.0
37.10	3900.0
38.10	3675.0
39.10	1686.0
40.00	180.0
40.70	78.0
43.10	76.0
44.00	568.0
45.00	607.0
46.20	159.0
47.00	1235.0
48.00	637.0
49.10	3351.0
50.10	16504.0
51.10	5005.0
52.00	285.0
53.20	99.0
55.10	226.0
56.00	1192.0
57.10	2788.0
58.10	107.0
60.10	793.0
61.00	3793.0
62.10	4273.0
63.10	3378.0
64.10	529.0
65.10	533.0
66.00	85.0
67.20	282.0
68.00	9040.0
69.00	8506.0
70.00	735.0
72.00	593.0
73.10	4104.0
74.10	15108.0
75.10	44072.0
76.10	3635.0
77.00	468.0
78.00	415.0
79.00	2979.0
80.00	863.0
81.00	3106.0
81.90	756.0
83.00	90.0
85.80	137.0
87.00	3929.0
88.00	3521.0
91.00	419.0
92.10	2438.0
93.10	3700.0
94.10	10306.0
95.00	83792.0
96.10	5081.0
97.00	146.0
103.10	61.0
104.00	443.0
104.90	170.0
105.90	402.0
106.90	125.0
109.90	51.0
110.70	97.0
112.00	52.0
115.10	92.0
116.00	362.0
117.00	604.0
118.00	344.0
119.00	650.0
125.80	104.0
127.90	335.0
128.90	162.0
129.90	452.0
131.00	129.0
135.00	120.0
137.00	206.0
140.10	62.0
141.00	874.0
142.00	89.0
143.00	1195.0
144.00	123.0
145.00	289.0
145.90	163.0
148.10	235.0
149.00	61.0
149.90	97.0
151.80	53.0
152.90	100.0
153.90	78.0
155.00	311.0
156.90	152.0
159.10	89.0
161.10	67.0
170.30	63.0

Instrument :
MSVOA_W
ClientSampleId :
BFB555

172.00	783.0
174.00	58376.0
175.00	5473.0
176.00	58120.0
177.00	4177.0
178.10	143.0
192.90	59.0
206.80	86.0
265.10	59.0
281.00	500.0
282.20	111.0
283.20	166.0
284.00	58.0

Instrument :
MSVOA_W
ClientSampleId :
BFB555