

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW083122\
 Data File : VW024511.D
 Acq On : 31 Aug 2022 14:01
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK548

Quant Time: Sep 01 03:00:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 31 02:55:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	311612	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	295519	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	129052	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	187490	21.827	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.320%
7) Chloroethane-d5	2.873	69	119405	18.553	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	74.200%
11) 1,1-Dichloroethene-d2	4.111	63	549	0.074	ug/L	0.10
Spiked Amount	25.000	Range	45 - 110	Recovery	=	0.280%#
21) 2-Butanone-d5	7.080	46	47444	29.987	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	59.980%
24) Chloroform-d	7.647	84	188178	18.784	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	75.120%
26) 1,2-Dichloroethane-d4	8.116	65	52	0.009	ug/L	-0.19
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.040%#
32) Benzene-d6	8.269	84	379858	22.434	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	89.720%
36) 1,2-Dichloropropane-d6	9.275	67	109900	20.871	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	83.480%
41) Toluene-d8	10.323	98	350163	21.751	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	87.000%
43) trans-1,3-Dichloroprop...	10.579	79	43630	17.706	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	70.840%
47) 2-Hexanone-d5	10.927	63	38525	32.694	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	65.380%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	92615	15.535	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	62.120%
66) 1,2-Dichlorobenzene-d4	13.847	152	106768	21.970	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	87.880%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.037	75	4185	0.631	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW083122\
Data File : VW024511.D
Acq On : 31 Aug 2022 14:01
Operator : SY/VA
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK548

Quant Time: Sep 01 03:00:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082622SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 31 02:55:40 2022
Response via : Initial Calibration

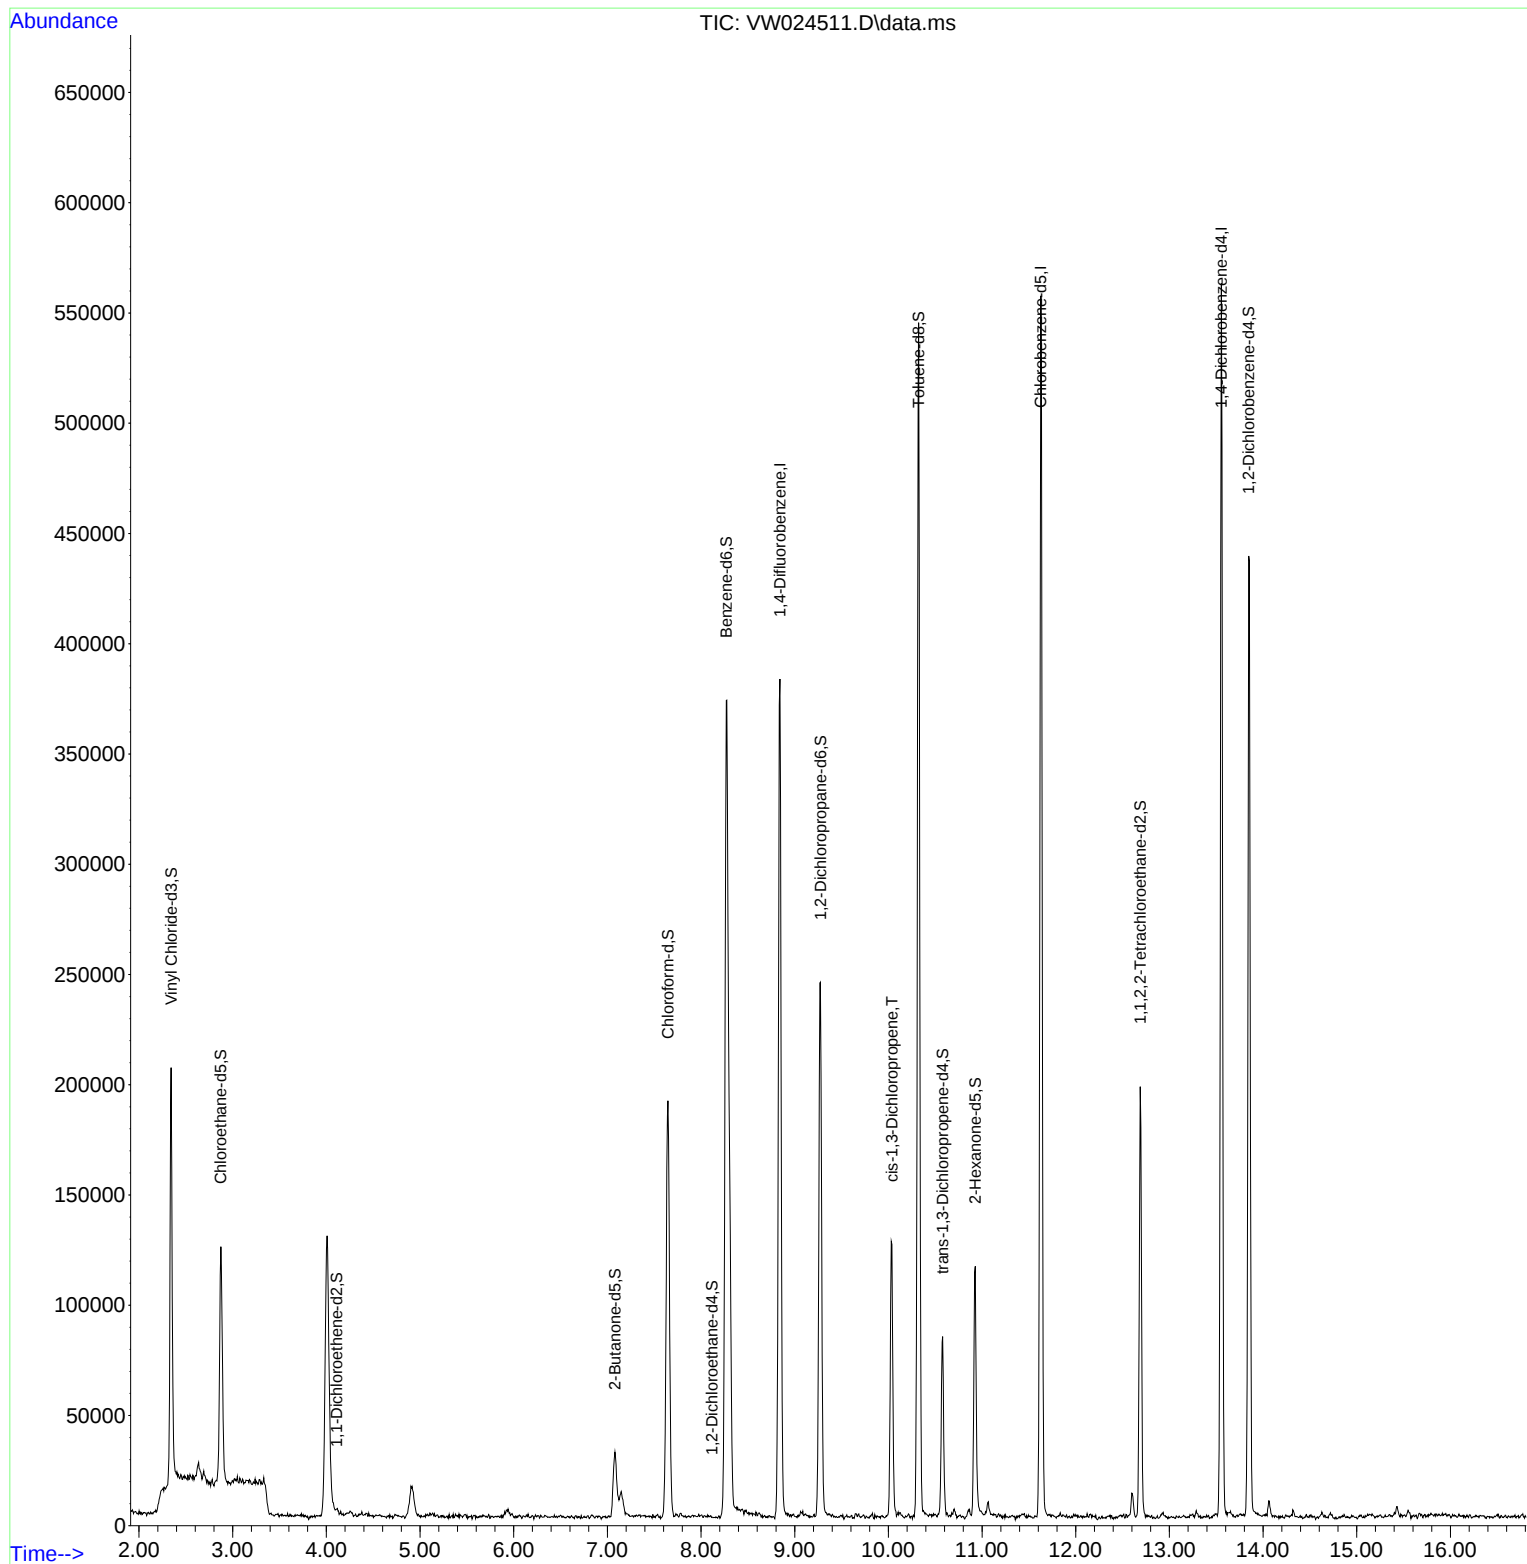

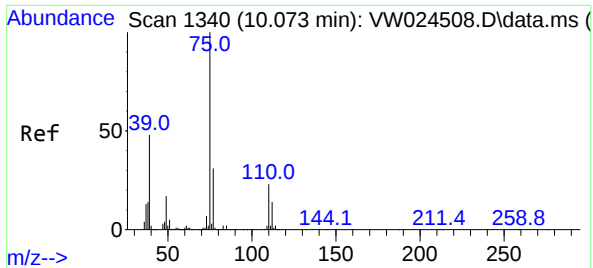

#39
 cis-1,3-Dichloropropene
 Concen: 0.631 ug/L
 RT: 10.037 min Scan# 11
 Delta R.T. -0.030 min
 Lab File: VW024511.D
 Acq: 31 Aug 2022 14:01

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK548

Tgt Ion: 75 Resp: 4185
 Ion Ratio Lower Upper
 75 100
 77 37.0 21.8 40.6

