

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090222\
 Data File : VW024529.D
 Acq On : 02 Sep 2022 13:25
 Operator : SY/VA
 Sample : VW0902SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK594

Quant Time: Sep 02 23:59:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 02 23:58:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.835	114	328235	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	313133	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	137396	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	181656	27.729	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	110.920%
7) Chloroethane-d5	2.873	69	129645	26.580	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	106.320%
11) 1,1-Dichloroethene-d2	4.007	63	142080	18.419	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	73.680%
21) 2-Butanone-d5	7.074	46	48728	47.168	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.340%
24) Chloroform-d	7.647	84	209730	23.996	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.000%
26) 1,2-Dichloroethane-d4	8.305	65	118546	25.115	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	100.440%
32) Benzene-d6	8.275	84	424124	25.965	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	103.880%
36) 1,2-Dichloropropane-d6	9.274	67	120546	25.221	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	100.880%
41) Toluene-d8	10.323	98	401673	25.822	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	103.280%
43) trans-1,3-Dichloroprop...	10.579	79	51152	24.533	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	98.120%
47) 2-Hexanone-d5	10.920	63	37707	46.058	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.120%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	97844	22.518	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	90.080%
66) 1,2-Dichlorobenzene-d4	13.853	152	115685	25.738	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	102.960%
Target Compounds						
39) cis-1,3-Dichloropropene	10.030	75	4604	0.682	ug/L	Qvalue 87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090222\
Data File : VW024529.D
Acq On : 02 Sep 2022 13:25
Operator : SY/VA
Sample : VW0902SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK594

Quant Time: Sep 02 23:59:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 02 23:58:31 2022
Response via : Initial Calibration

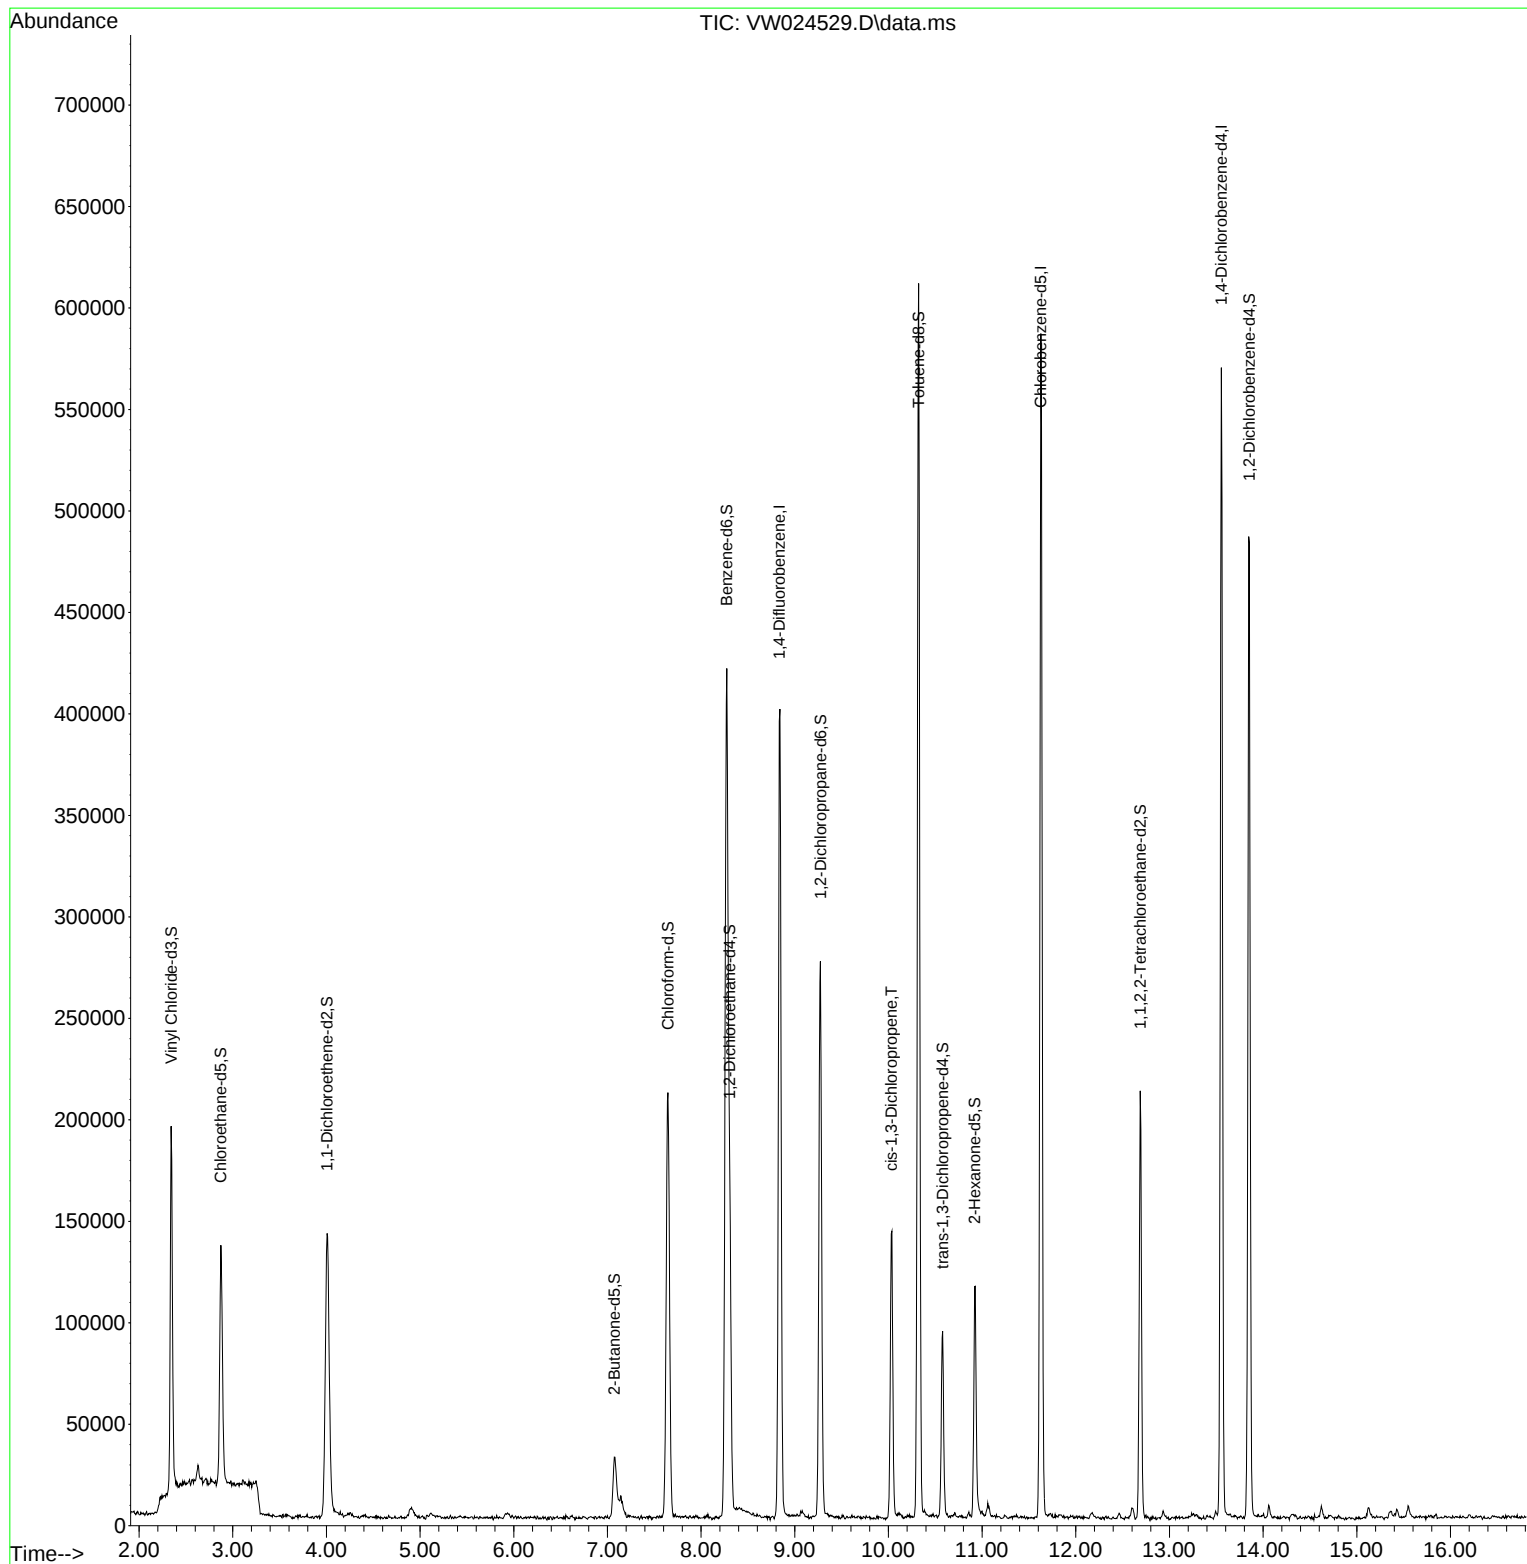

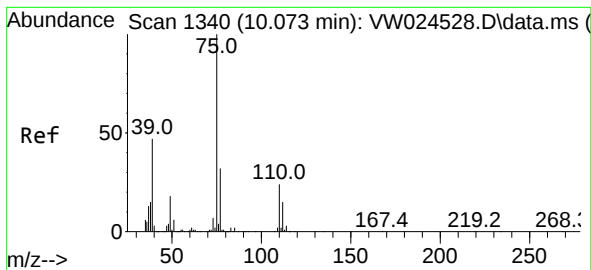

#39
 cis-1,3-Dichloropropene
 Concen: 0.682 ug/L
 RT: 10.030 min Scan# 11
 Delta R.T. -0.043 min
 Lab File: VW024529.D
 Acq: 02 Sep 2022 13:25

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK594

Tgt Ion: 75 Resp: 4604
 Ion Ratio Lower Upper
 75 100
 77 38.6 22.0 40.8

