

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090222\
 Data File : VW024533.D
 Acq On : 02 Sep 2022 15:05
 Operator : SY/VA
 Sample : N4483-01
 Misc : 6.45g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW351

Quant Time: Sep 03 00:04:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 02 23:58:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	278596	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	240679	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	89275	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	88283	15.877	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	63.520%
7) Chloroethane-d5	2.873	69	78342	18.924	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.680%
11) 1,1-Dichloroethene-d2	4.001	63	63129	9.642	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	38.560%#
21) 2-Butanone-d5	7.074	46	66564	75.913	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	151.820%#
24) Chloroform-d	7.647	84	178148	24.014	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.040%
26) 1,2-Dichloroethane-d4	8.202	65	115	0.029	ug/L	-0.10
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.120%#
32) Benzene-d6	8.269	84	261825	20.854	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	83.400%
36) 1,2-Dichloropropane-d6	9.275	67	100200	27.276	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	109.120%
41) Toluene-d8	10.323	98	196306	16.418	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	65.680%
43) trans-1,3-Dichloroprop...	10.573	79	40370	25.191	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	100.760%
47) 2-Hexanone-d5	10.921	63	50696	80.565	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	161.120%#
56) 1,1,2,2-Tetrachloroeth...	12.689	84	117995	35.331	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	141.320%#
66) 1,2-Dichlorobenzene-d4	13.853	152	73893	25.302	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	101.200%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.031	75	3578	0.689	ug/L	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090222\
Data File : VW024533.D
Acq On : 02 Sep 2022 15:05
Operator : SY/VA
Sample : N4483-01
Misc : 6.45g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW351

Quant Time: Sep 03 00:04:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 02 23:58:31 2022
Response via : Initial Calibration

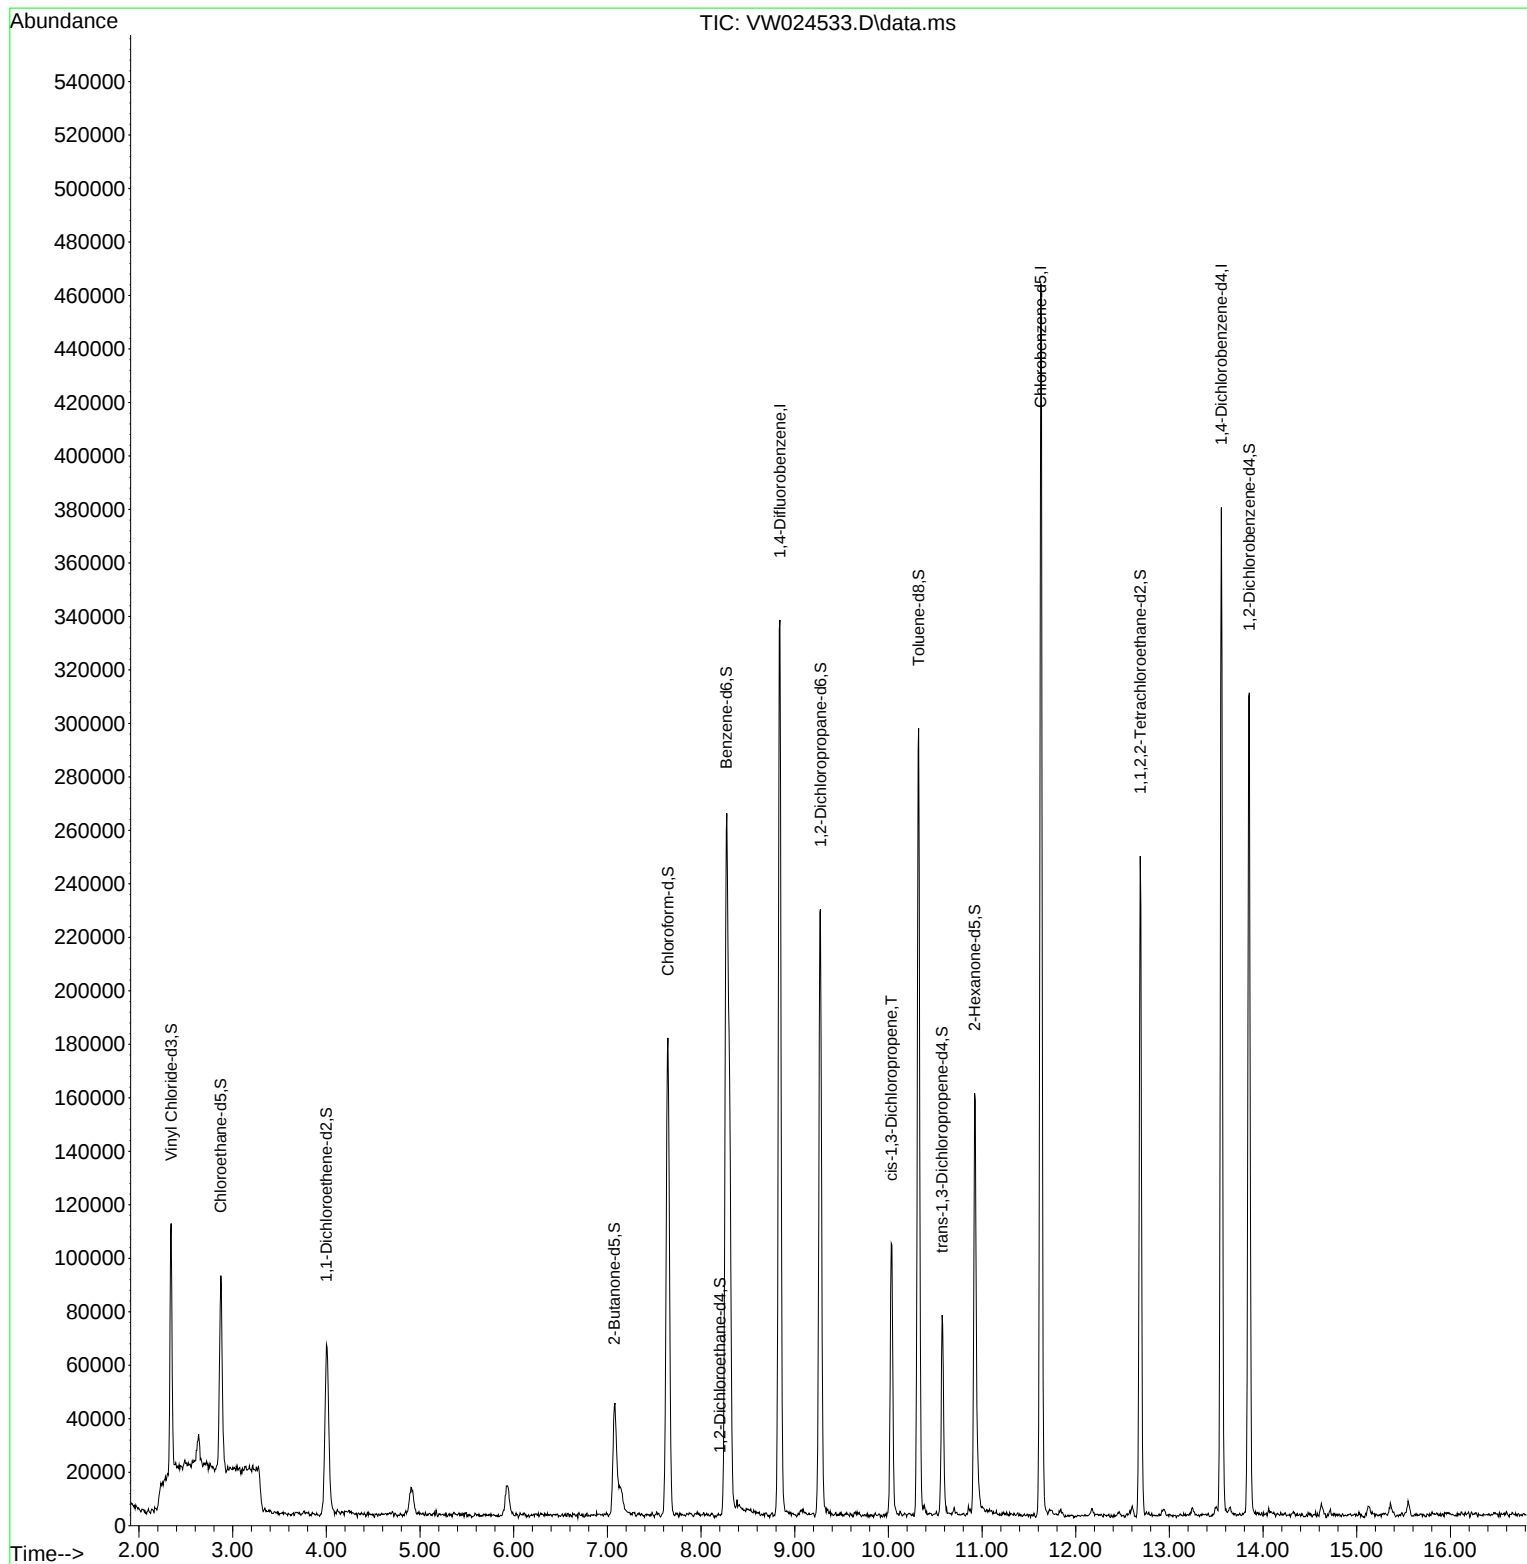

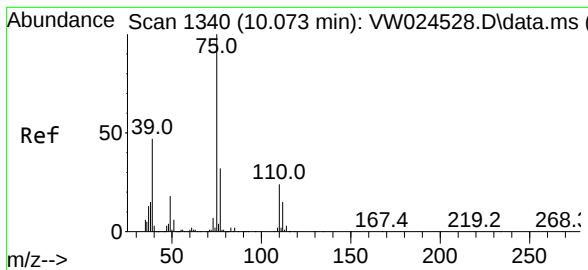

#39
 cis-1,3-Dichloropropene
 Concen: 0.689 ug/L
 RT: 10.031 min Scan# 11
 Delta R.T. -0.043 min
 Lab File: VW024533.D
 Acq: 02 Sep 2022 15:05

Instrument :
 MSVOA_W
 ClientSampleId :
 EW351

Tgt Ion: 75 Resp: 3578
 Ion Ratio Lower Upper
 75 100
 77 40.7 22.0 40.8

