

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090222\
 Data File : VW024535.D
 Acq On : 02 Sep 2022 15:54
 Operator : SY/VA
 Sample : N4483-06
 Misc : 9.76g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW354

Quant Time: Sep 03 00:04:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 02 23:58:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	276761	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	259250	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	96471	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	94023	17.022	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	68.080%
7) Chloroethane-d5	2.873	69	87107	21.180	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.720%
11) 1,1-Dichloroethene-d2	4.007	63	62405	9.595	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	38.360%#
21) 2-Butanone-d5	7.080	46	75384	86.542	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	173.080%#
24) Chloroform-d	7.647	84	181983	24.694	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	98.760%
26) 1,2-Dichloroethane-d4	8.427	65	190	0.048	ug/L	0.12
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.200%#
32) Benzene-d6	8.269	84	271195	20.053	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	80.200%
36) 1,2-Dichloropropane-d6	9.275	67	105380	26.631	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	106.520%
41) Toluene-d8	10.317	98	202819	15.748	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	63.000%
43) trans-1,3-Dichloroprop...	10.579	79	39041	22.616	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	90.480%
47) 2-Hexanone-d5	10.921	63	60511	89.274	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	178.540%#
56) 1,1,2,2-Tetrachloroeth...	12.689	84	131526	36.561	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	146.240%#
66) 1,2-Dichlorobenzene-d4	13.853	152	86109	27.285	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	109.160%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.031	75	3091	0.553	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090222\
Data File : VW024535.D
Acq On : 02 Sep 2022 15:54
Operator : SY/VA
Sample : N4483-06
Misc : 9.76g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW354

Quant Time: Sep 03 00:04:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 02 23:58:31 2022
Response via : Initial Calibration

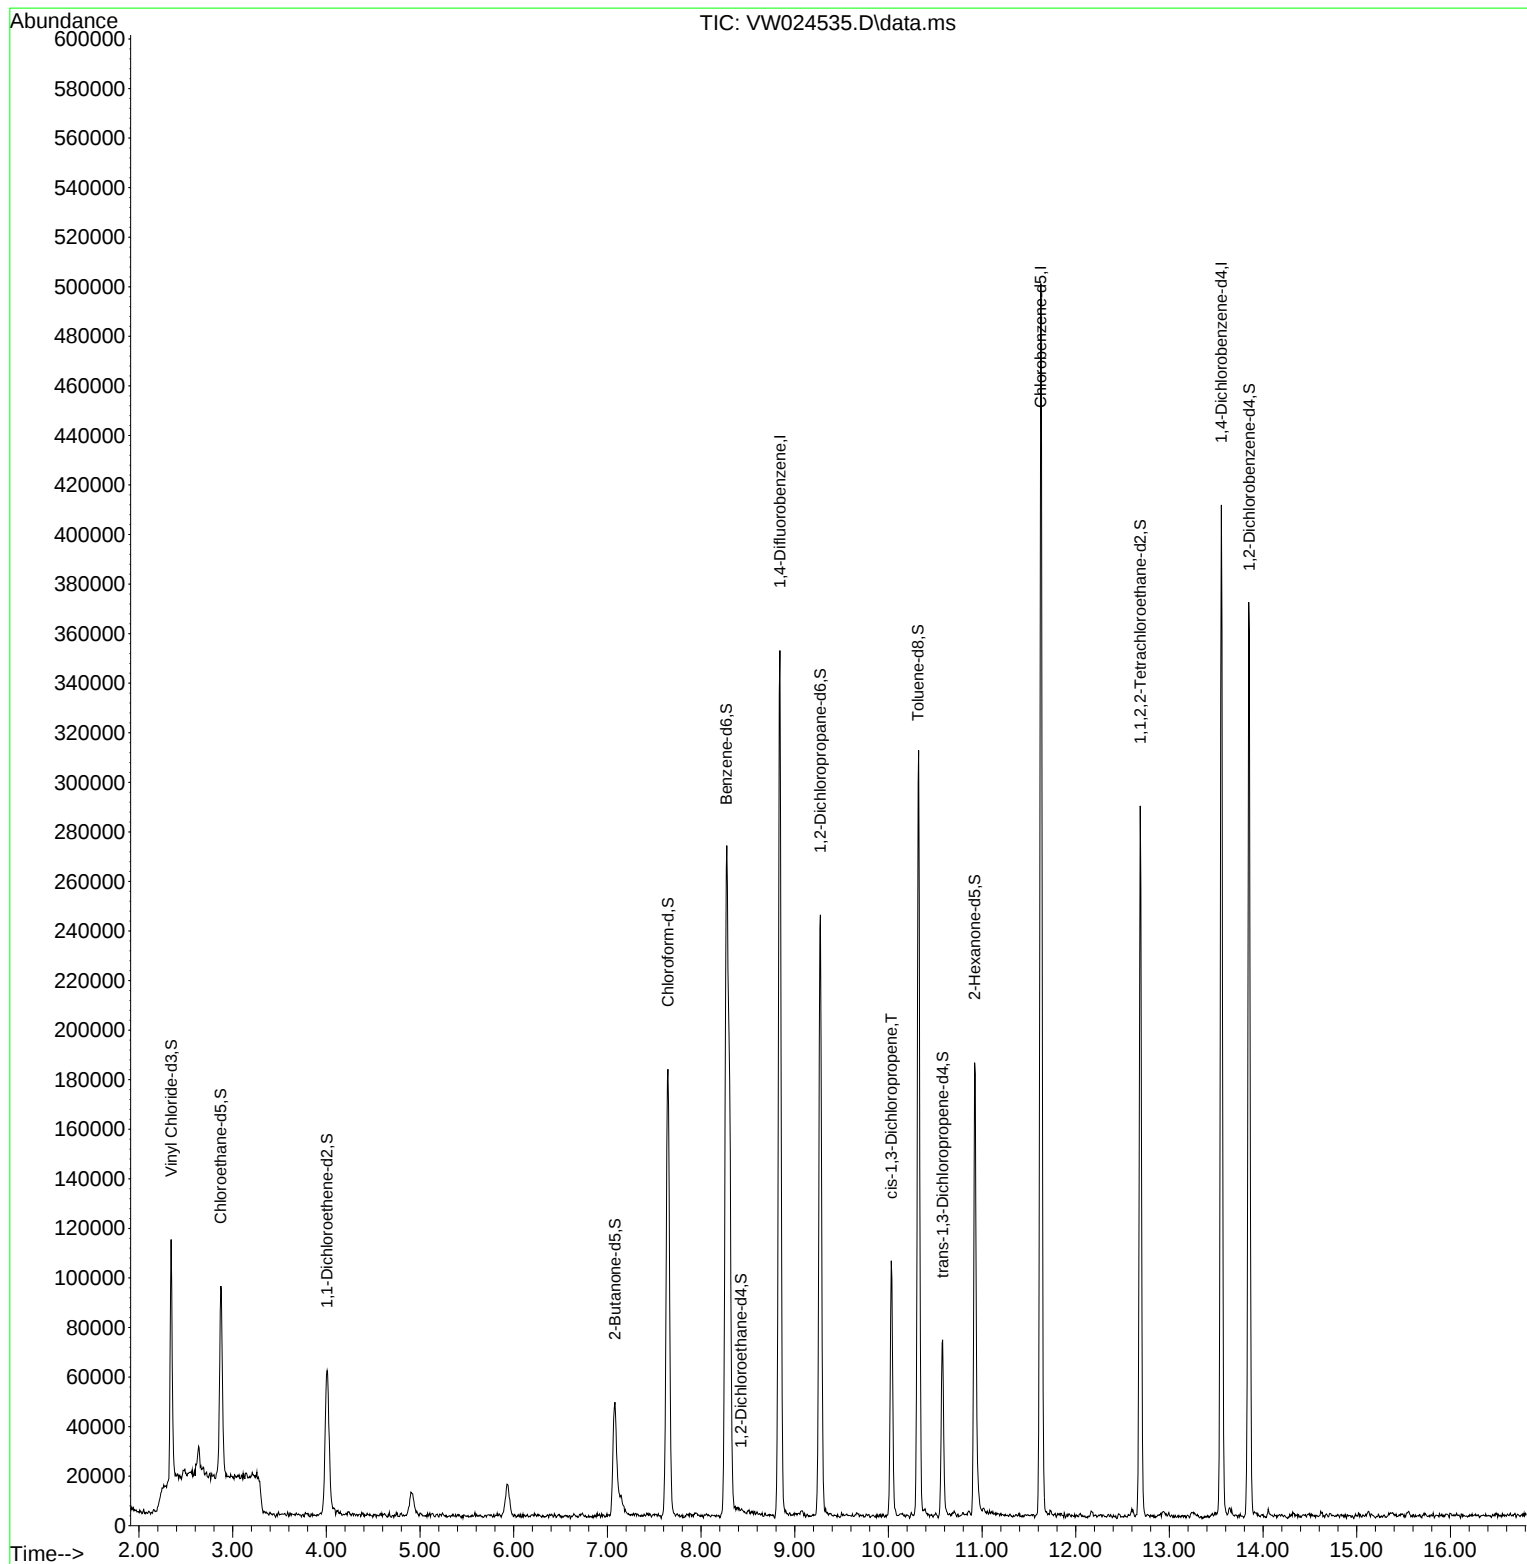

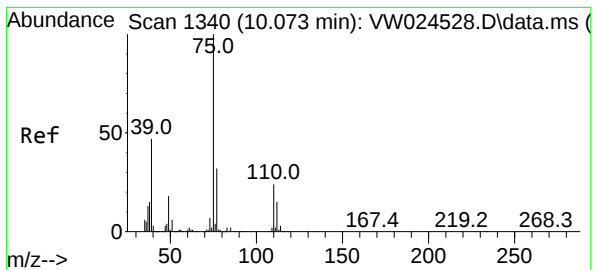

#39
 cis-1,3-Dichloropropene
 Concen: 0.553 ug/L
 RT: 10.031 min Scan# 11
 Delta R.T. -0.043 min
 Lab File: VW024535.D
 Acq: 02 Sep 2022 15:54

Instrument :
 MSVOA_W
 ClientSampleId :
 EW354

Tgt Ion: 75 Resp: 3091
 Ion Ratio Lower Upper
 75 100
 77 29.8 22.0 40.8

