

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090222\
 Data File : VW024541.D
 Acq On : 02 Sep 2022 18:21
 Operator : SY/VA
 Sample : N4483-12
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW360

Quant Time: Sep 03 00:06:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 02 23:58:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	292306	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	250301	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	73202	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.337	65	113145	19.394	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	77.560%
7) Chloroethane-d5	2.873	69	102243	23.538	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	94.160%
11) 1,1-Dichloroethene-d2	4.001	63	65382	9.518	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	38.080%#
21) 2-Butanone-d5	7.080	46	67684	73.570	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	147.140%#
24) Chloroform-d	7.647	84	202423	26.007	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	104.040%
26) 1,2-Dichloroethane-d4	8.299	65	136351	32.438	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	129.760%
32) Benzene-d6	8.269	84	289888	22.202	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	88.800%
36) 1,2-Dichloropropane-d6	9.268	67	115603	30.259	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	121.040%#
41) Toluene-d8	10.317	98	208901	16.800	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	67.200%
43) trans-1,3-Dichloroprop...	10.579	79	37362	22.417	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.680%
47) 2-Hexanone-d5	10.927	63	45957	70.226	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	140.460%#
56) 1,1,2,2-Tetrachloroeth...	12.689	84	131925	37.983	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	151.920%#
66) 1,2-Dichlorobenzene-d4	13.847	152	71321	29.783	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	119.120%
Target Compounds					Qvalue	
48) 2-Hexanone	10.951	43	4210	2.837	ug/L #	44


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090222\
Data File : VW024541.D
Acq On : 02 Sep 2022 18:21
Operator : SY/VA
Sample : N4483-12
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW360

Quant Time: Sep 03 00:06:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 02 23:58:31 2022
Response via : Initial Calibration

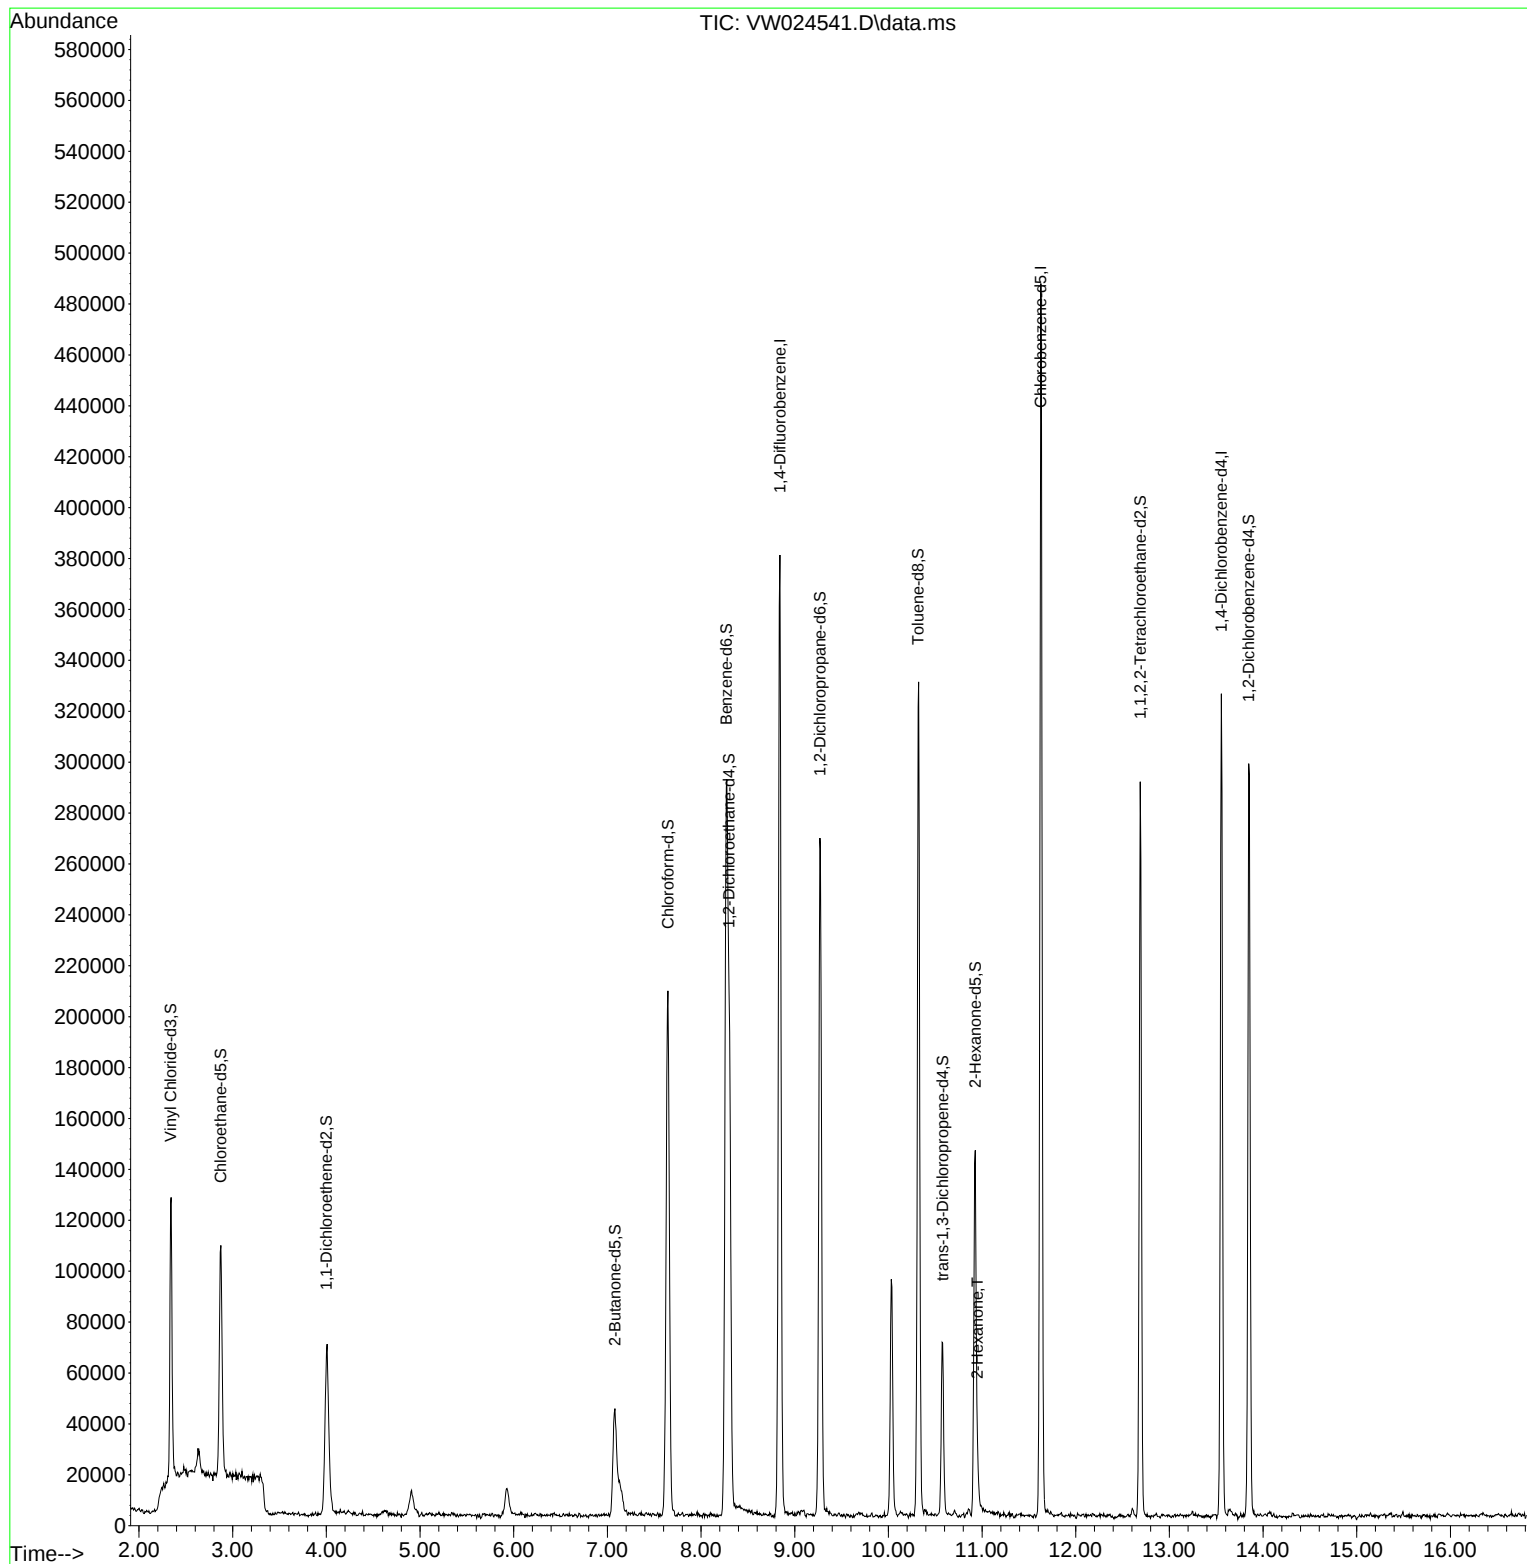

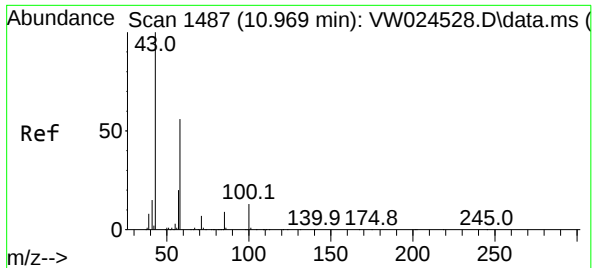

#48
 2-Hexanone
 Concen: 2.837 ug/L
 RT: 10.951 min Scan# 14
 Delta R.T. -0.018 min
 Lab File: VW024541.D
 Acq: 02 Sep 2022 18:21

Instrument :
 MSVOA_W
 ClientSampleId :
 EW360

Tgt Ion: 43	Resp: 4210
Ion Ratio	Lower Upper
43	100
58	4.3 44.2 66.2#
57	4.7 15.5 23.3#
100	0.6 11.4 17.2#

