




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090222\
 Data File : VW024522.D
 Acq On : 02 Sep 2022 09:35
 Operator : SY/VA
 Sample : VSTD2.525
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VSTD2.5425

Manual IntegrationsAPPROVED

Quant Time: Sep 02 23:32:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 02 23:31:46 2022
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

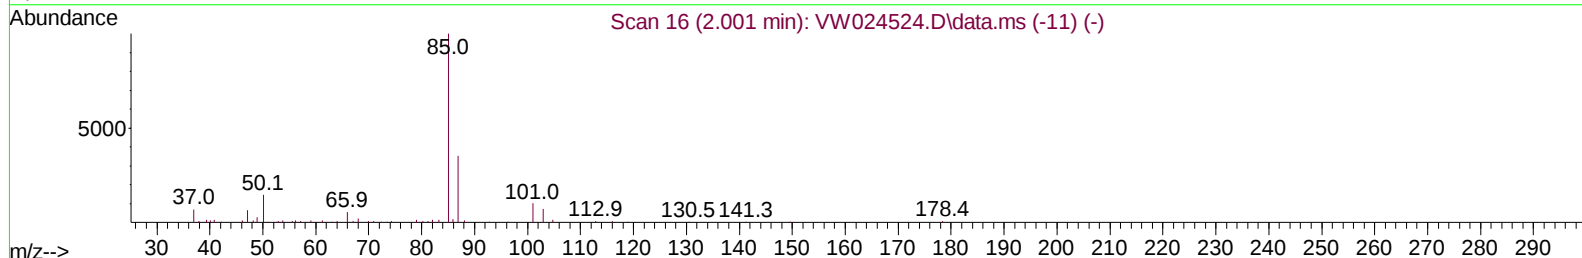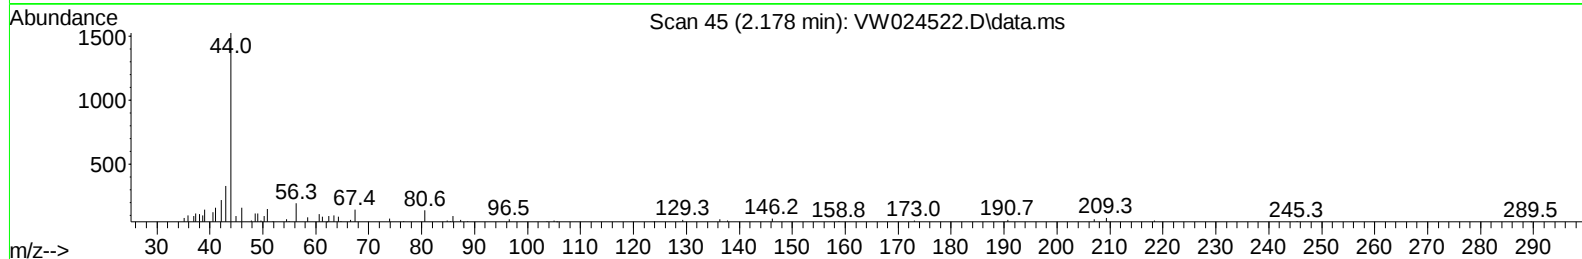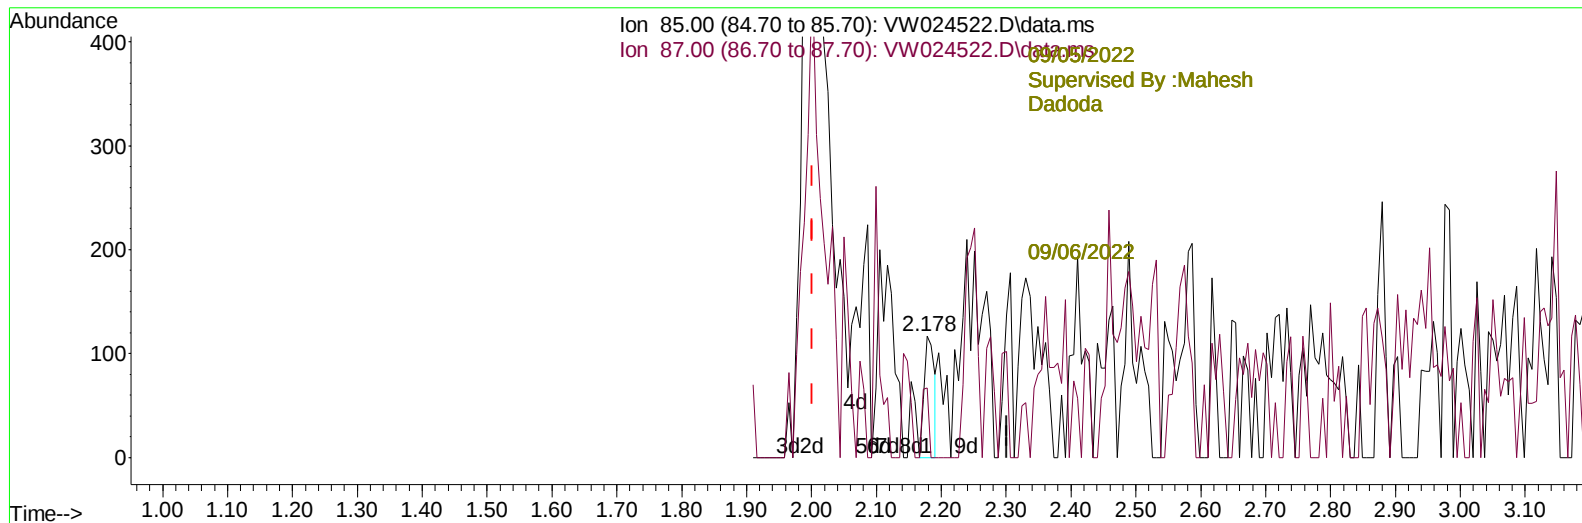

TIC: VW024522.D\data.ms

(2) Dichlorodifluoromethane (T)

2.178min (+ 0.177) 0.15 ug/L

response 132

Ion	Exp%	Act%
85.00	100.00	100.00
87.00	31.30	37.12
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090222\
 Data File : VW024522.D
 Acq On : 02 Sep 2022 09:35
 Operator : SY/VA
 Sample : VSTD2.525
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VSTD2.5425

Manual IntegrationsAPPROVED

Quant Time: Sep 02 23:32:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 02 23:31:46 2022
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

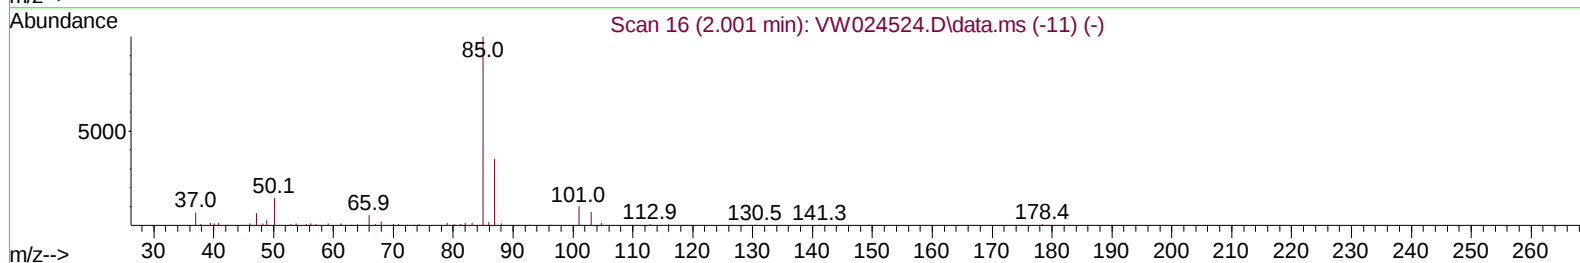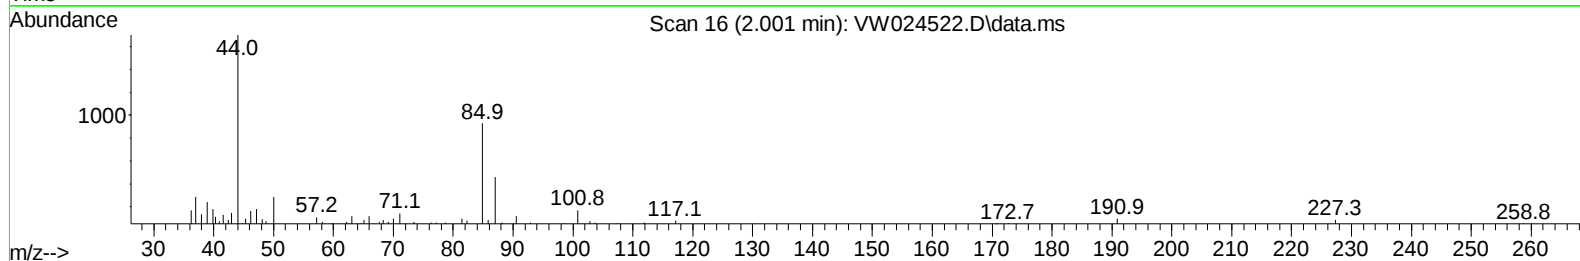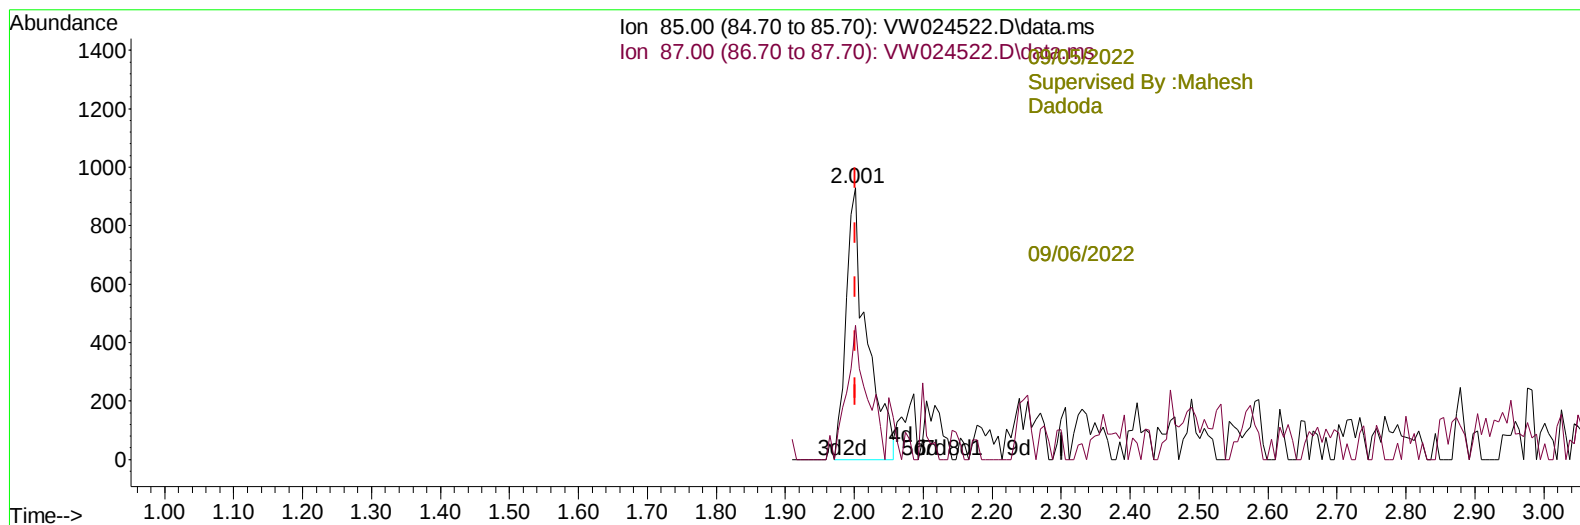

TIC: VW024522.D\data.ms

(2) Dichlorodifluoromethane (T)

2.001min (+ 0.000) 2.13 ug/L m

response 1915

Ion	Exp%	Act%
85.00	100.00	100.00
87.00	31.30	2.56#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090222\
 Data File : VW024522.D
 Acq On : 02 Sep 2022 09:35
 Operator : SY/VA
 Sample : VSTD2.525
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VSTD2.5425

Manual IntegrationsAPPROVED

Quant Time: Sep 02 23:32:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 02 23:31:46 2022
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

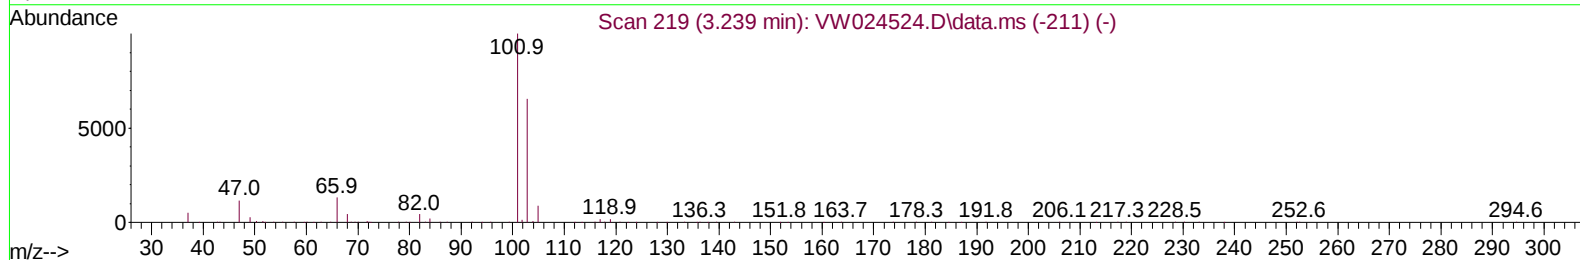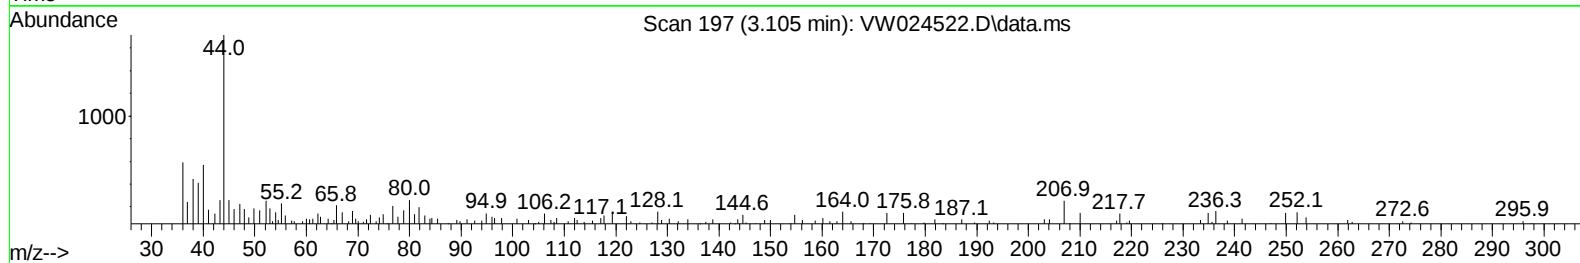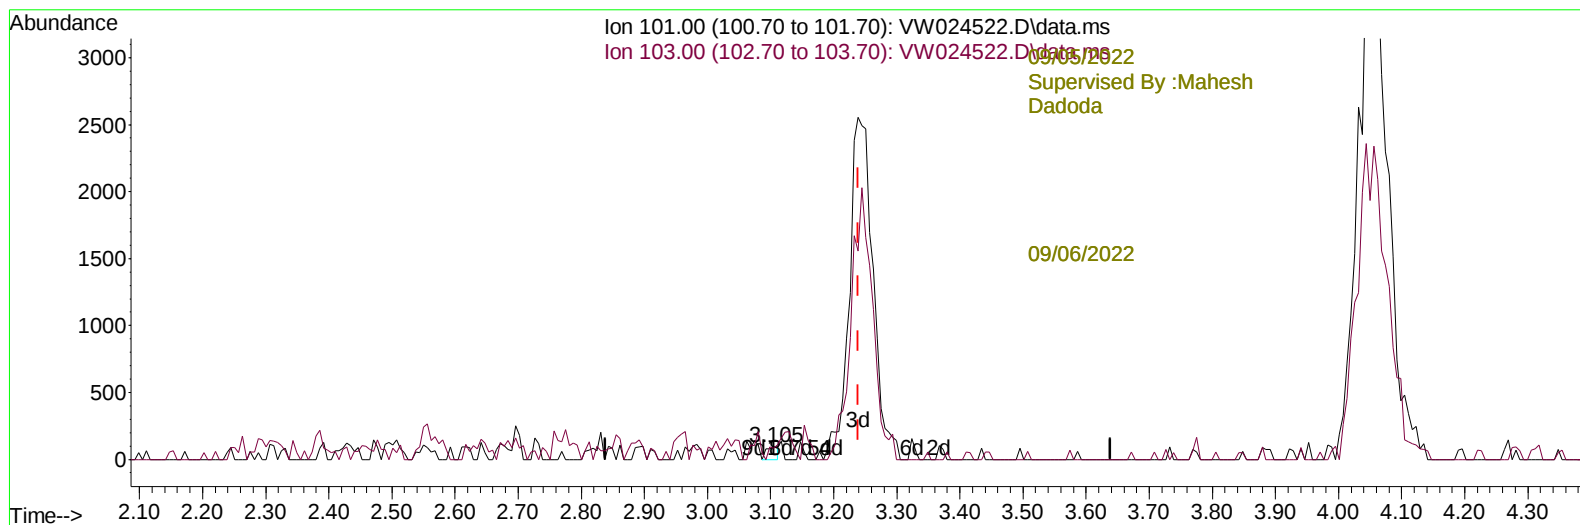

TIC: VW024522.D\data.ms

(9) Trichlorofluoromethane (T)

3.105min (-0.134) 0.04 ug/L

response 122

Ion	Exp%	Act%
101.00	100.00	100.00
103.00	64.70	53.28
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090222\
 Data File : VW024522.D
 Acq On : 02 Sep 2022 09:35
 Operator : SY/VA
 Sample : VSTD2.525
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VSTD2.5425

Manual IntegrationsAPPROVED

Quant Time: Sep 02 23:32:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 02 23:31:46 2022
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

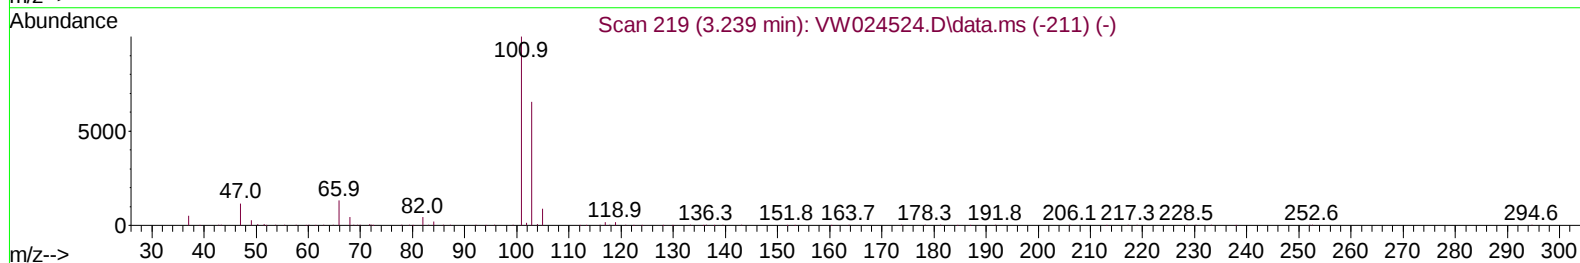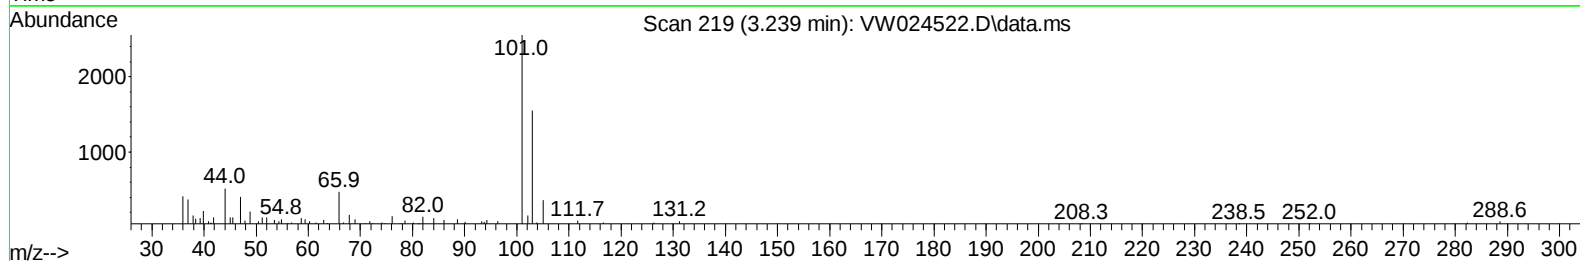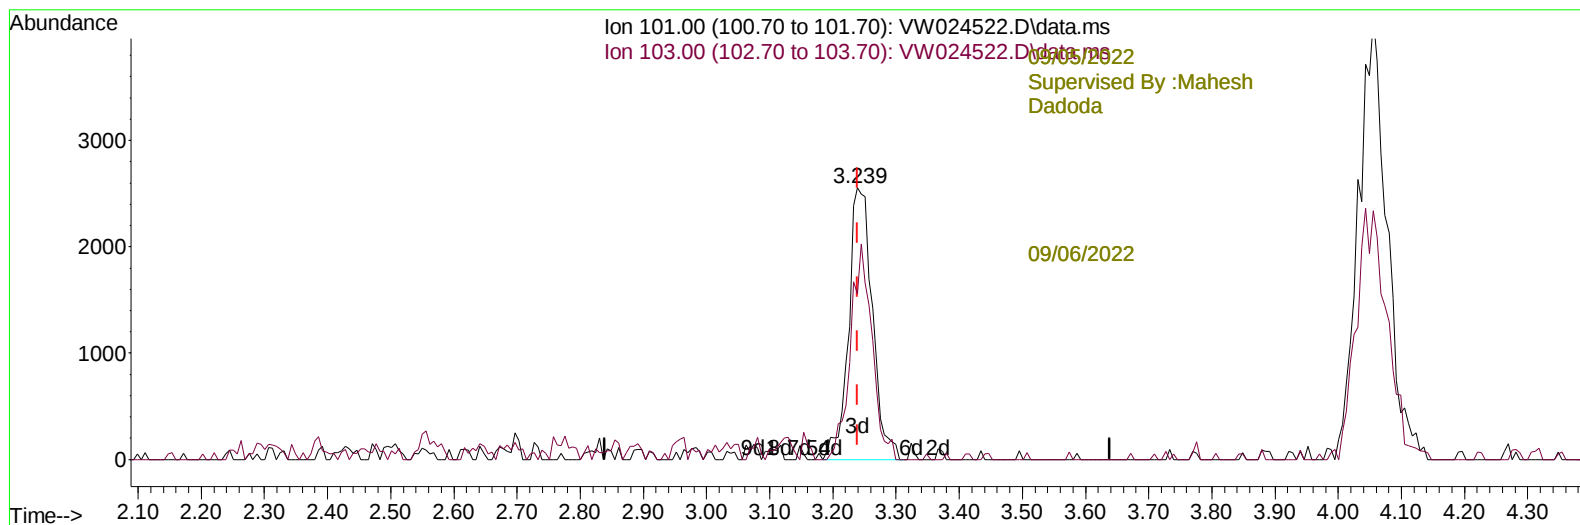

TIC: VW024522.D\data.ms

(9) Trichlorofluoromethane (T)

3.239min (+ 0.000) 2.19 ug/L m

response 6711

Ion	Exp%	Act%
101.00	100.00	100.00
103.00	64.70	0.97#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090222\
 Data File : VW024522.D
 Acq On : 02 Sep 2022 09:35
 Operator : SY/VA
 Sample : VSTD2.525
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VSTD2.5425

Manual IntegrationsAPPROVED

Quant Time: Sep 02 23:32:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 02 23:31:46 2022
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

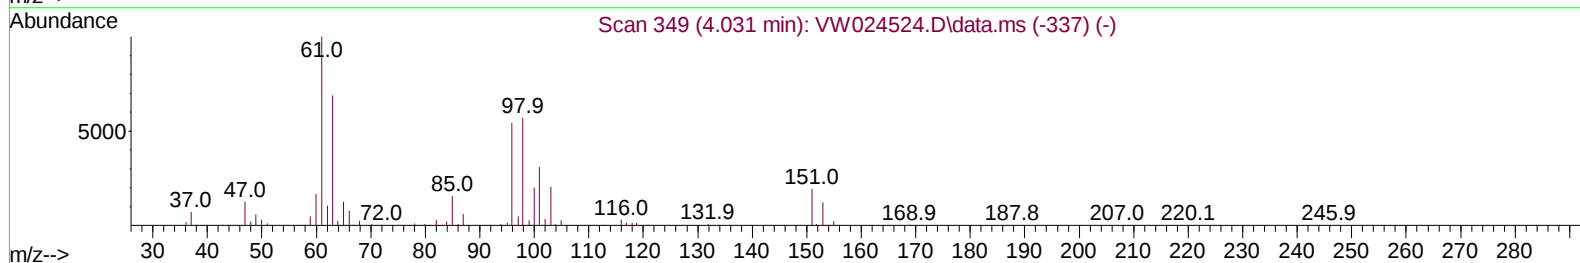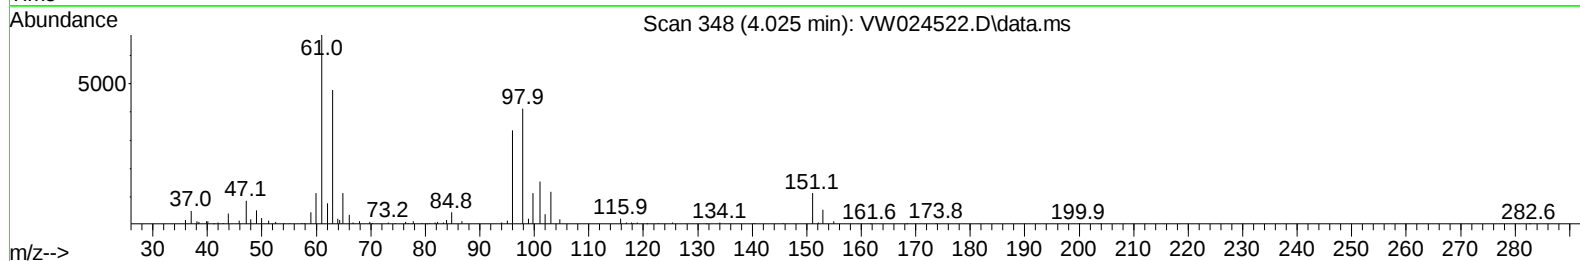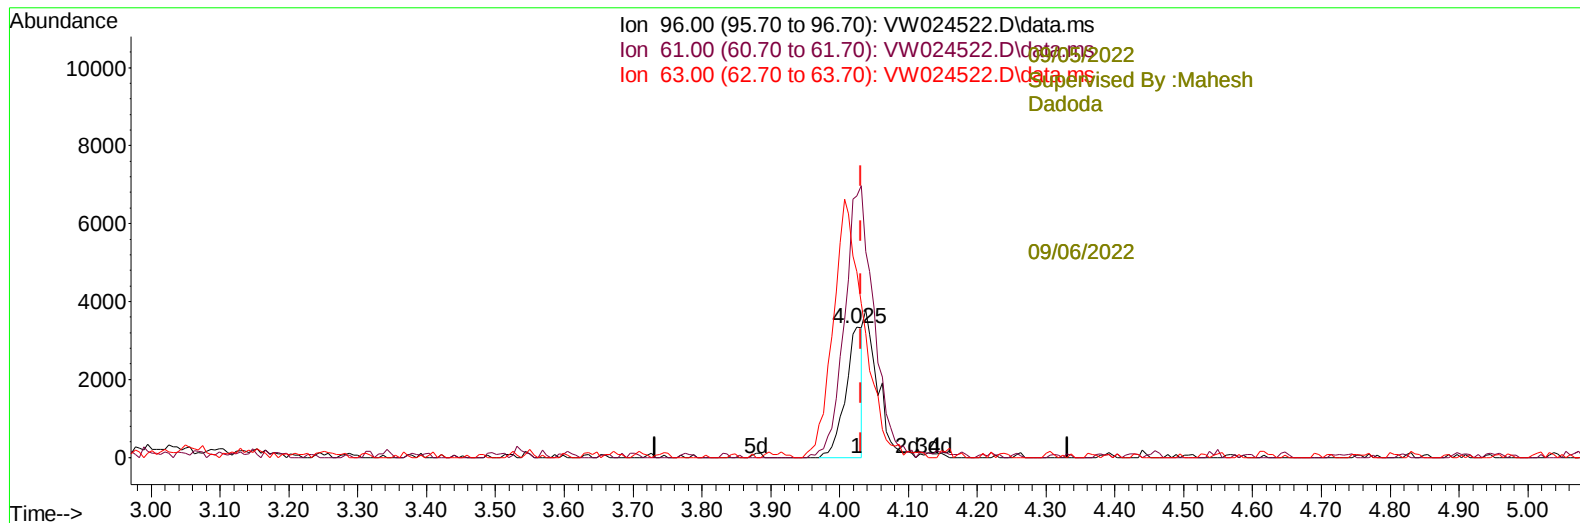

TIC: VW024522.D\data.ms

(12) 1,1-Dichloroethene (T)

4.025min (-0.006) 1.40 ug/L

response 5658

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	184.50	200.99
63.00	128.80	142.61
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090222\
 Data File : VW024522.D
 Acq On : 02 Sep 2022 09:35
 Operator : SY/VA
 Sample : VSTD2.525
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VSTD2.5425

Manual IntegrationsAPPROVED

Quant Time: Sep 02 23:32:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 02 23:31:46 2022
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

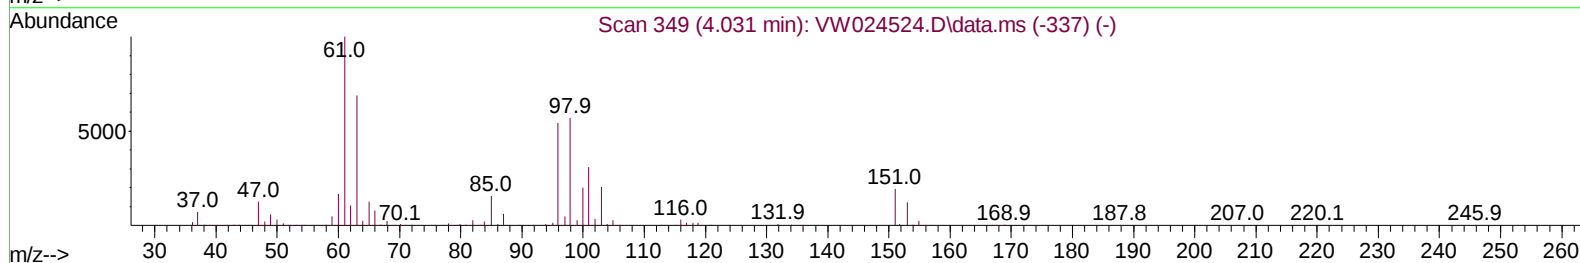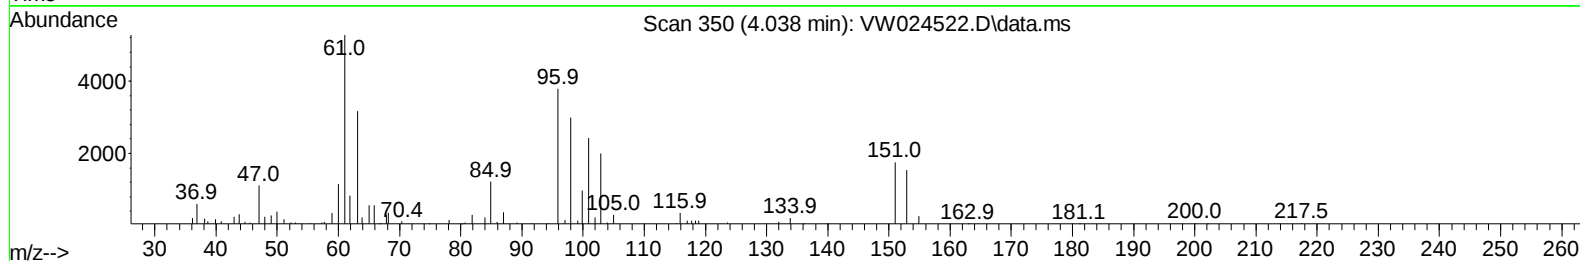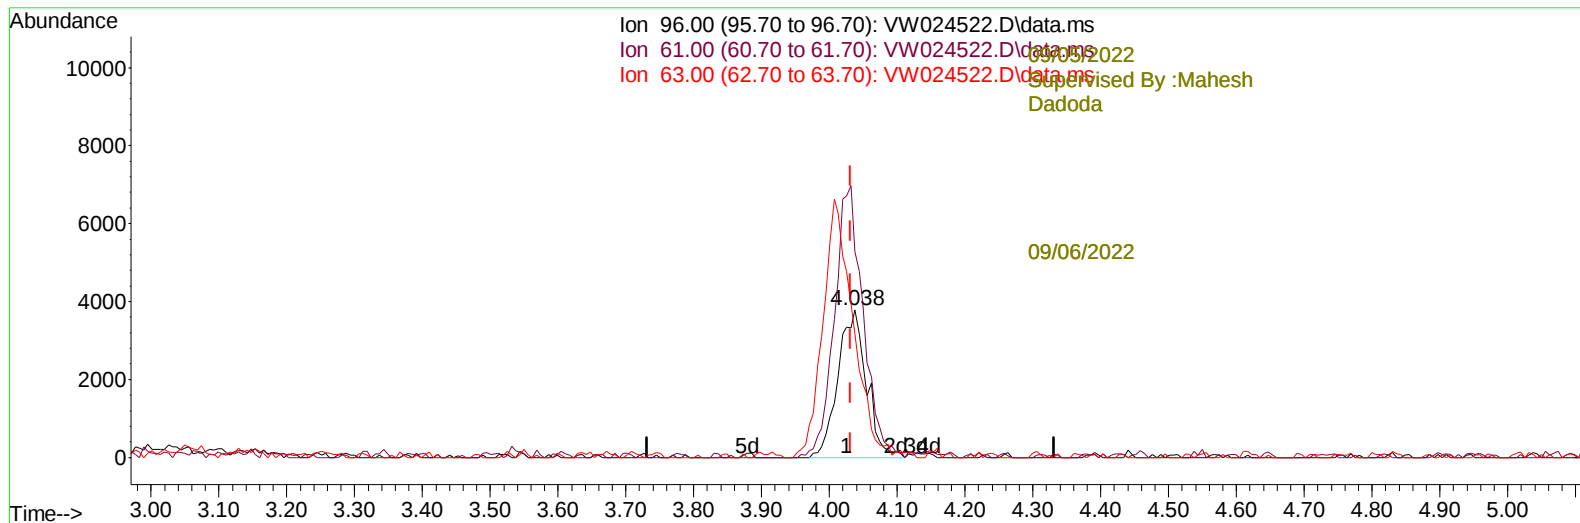

TIC: VW024522.D\data.ms

(12) 1,1-Dichloroethene (T)

4.038min (+ 0.006) 2.72 ug/L m

response 11043

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	184.50	139.16
63.00	128.80	83.78#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090222\
 Data File : VW024522.D
 Acq On : 02 Sep 2022 09:35
 Operator : SY/VA
 Sample : VSTD2.525
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VSTD2.5425

Manual IntegrationsAPPROVED

Quant Time: Sep 02 23:32:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 02 23:31:46 2022
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

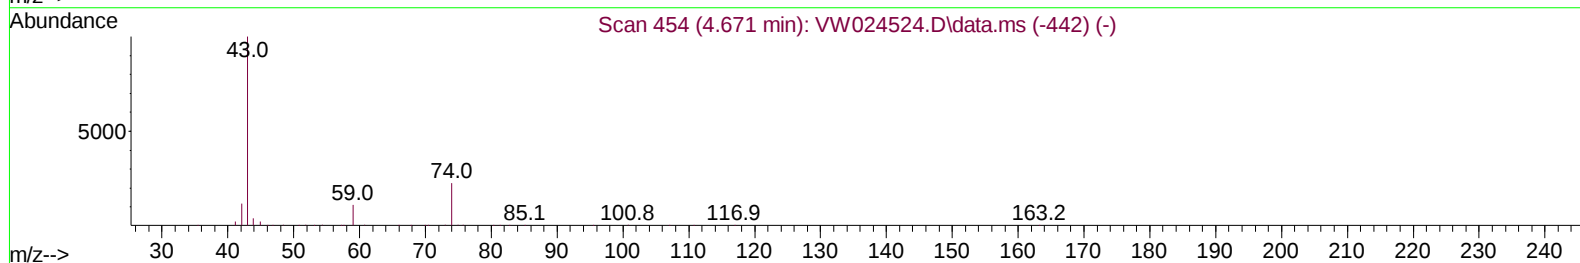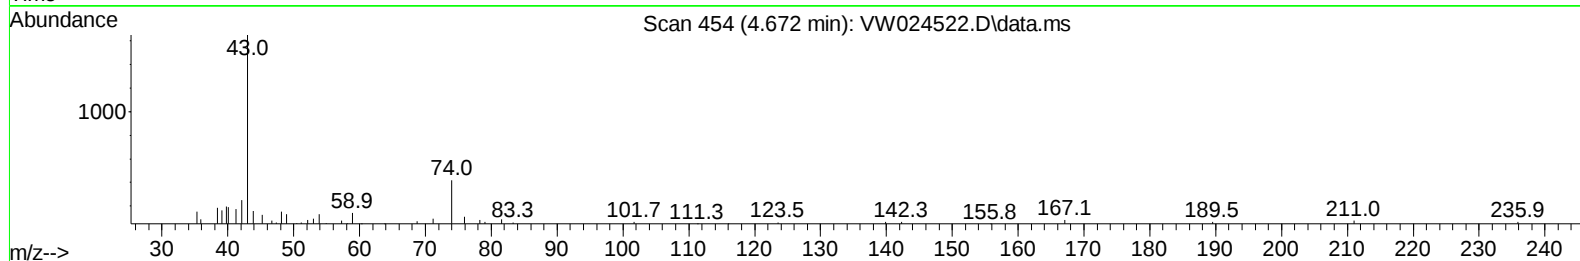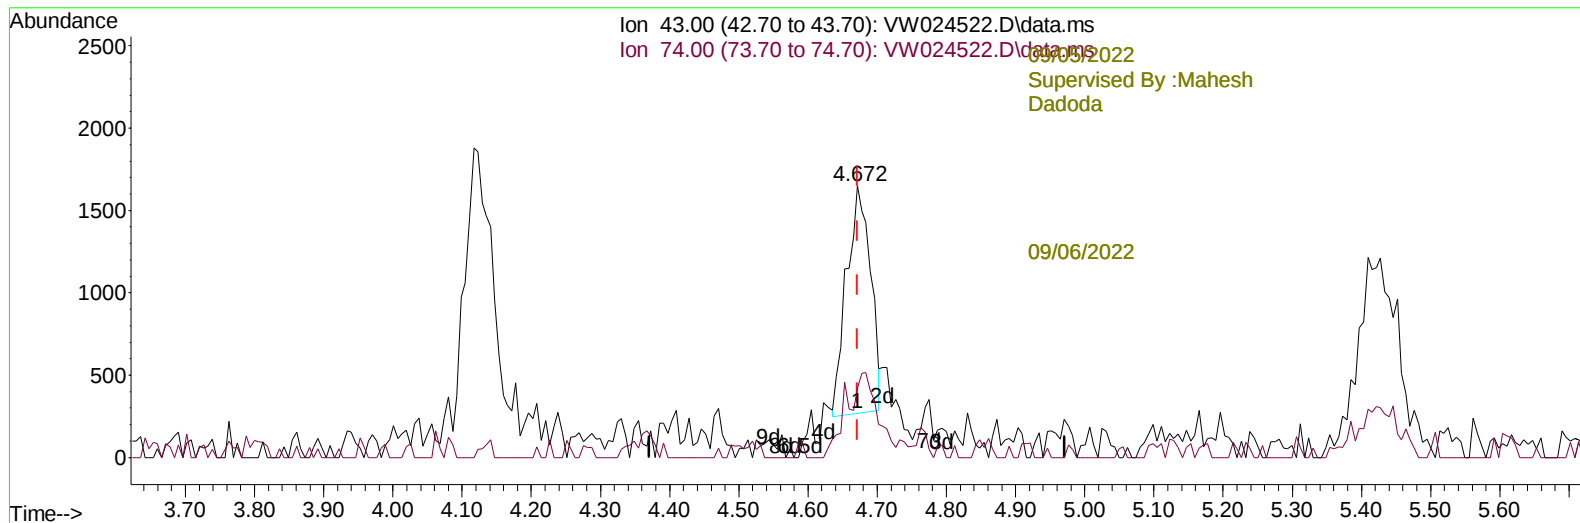

TIC: VW024522.D\data.ms

(15) Methyl Acetate (T)

4.672min (+ 0.000) 1.81 ug/L

response 3317

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	24.40	20.89
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090222\
Data File : VW024522.D
Acq On : 02 Sep 2022 09:35
Operator : SY/VA
Sample : VSTD2.525
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VSTD2.5425

Manual IntegrationsAPPROVED

Quant Time: Sep 02 23:32:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 02 23:31:46 2022
Response via : Initial Calibration

Reviewed By :Semsettin
Yesilyurt

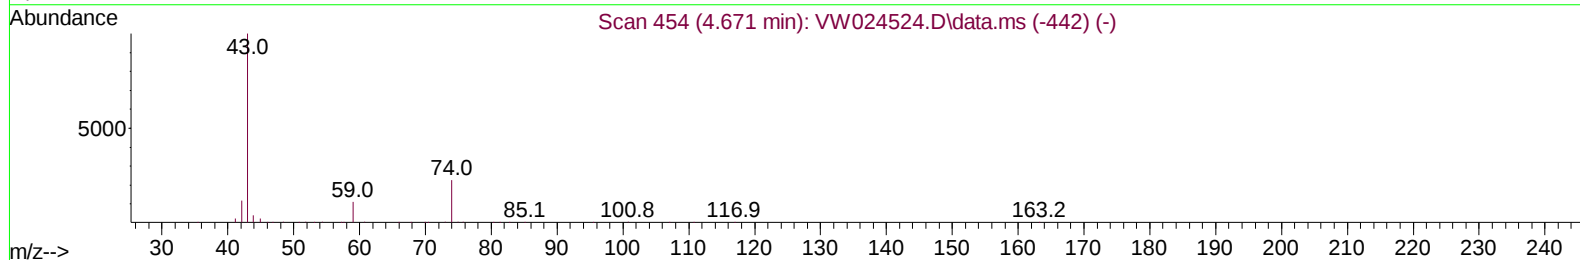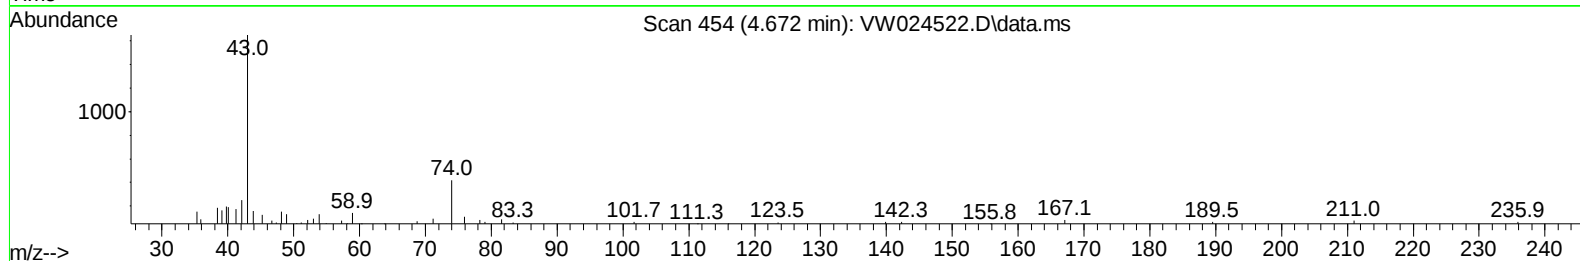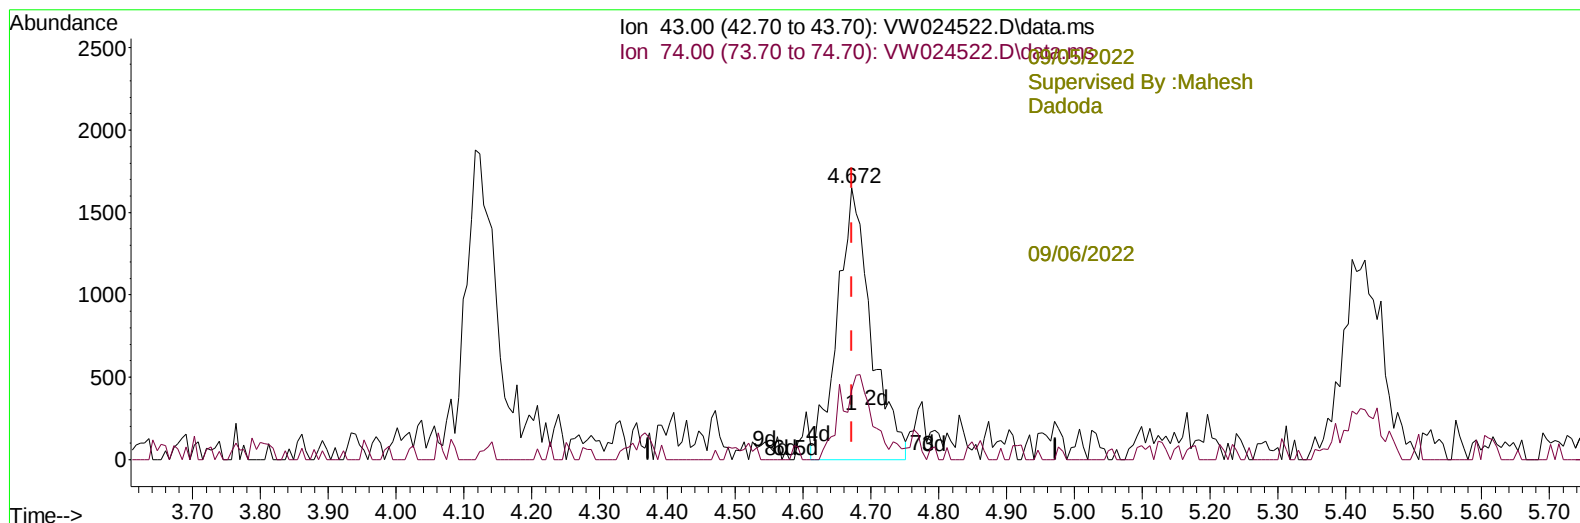

TIC: VW024522.D\data.ms

(15) Methyl Acetate (T)

4.672min (+ 0.000) 3.10 ug/L m

response 5674

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	24.40	12.21#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090222\
Data File : VW024522.D
Acq On : 02 Sep 2022 09:35
Operator : SY/VA
Sample : VSTD2.525
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VSTD2.5425

Manual IntegrationsAPPROVED

Quant Time: Sep 02 23:32:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 02 23:31:46 2022
Response via : Initial Calibration

Reviewed By :Semsettin
Yesilyurt

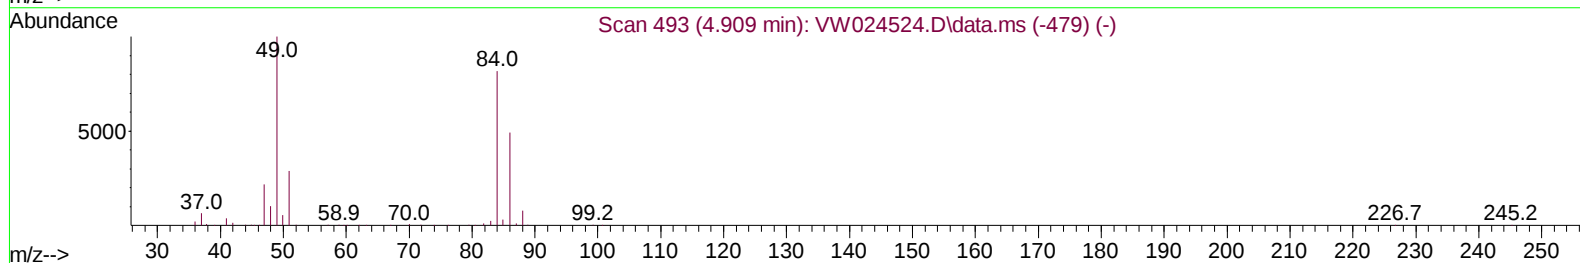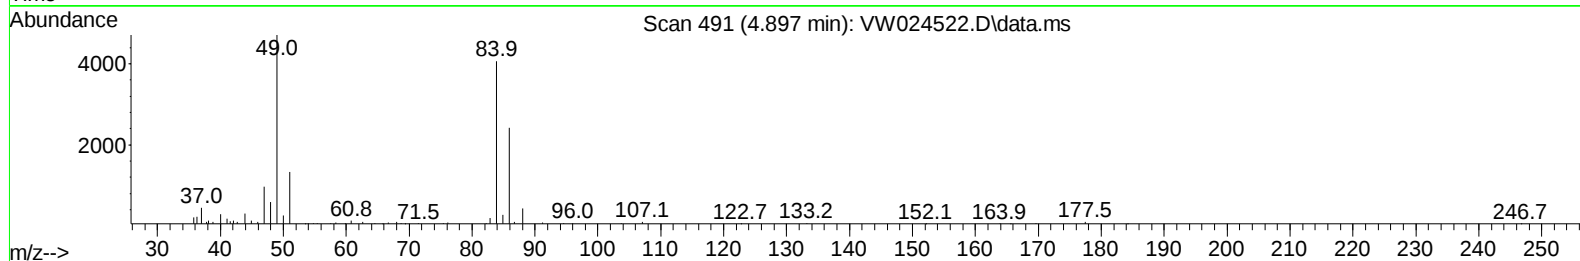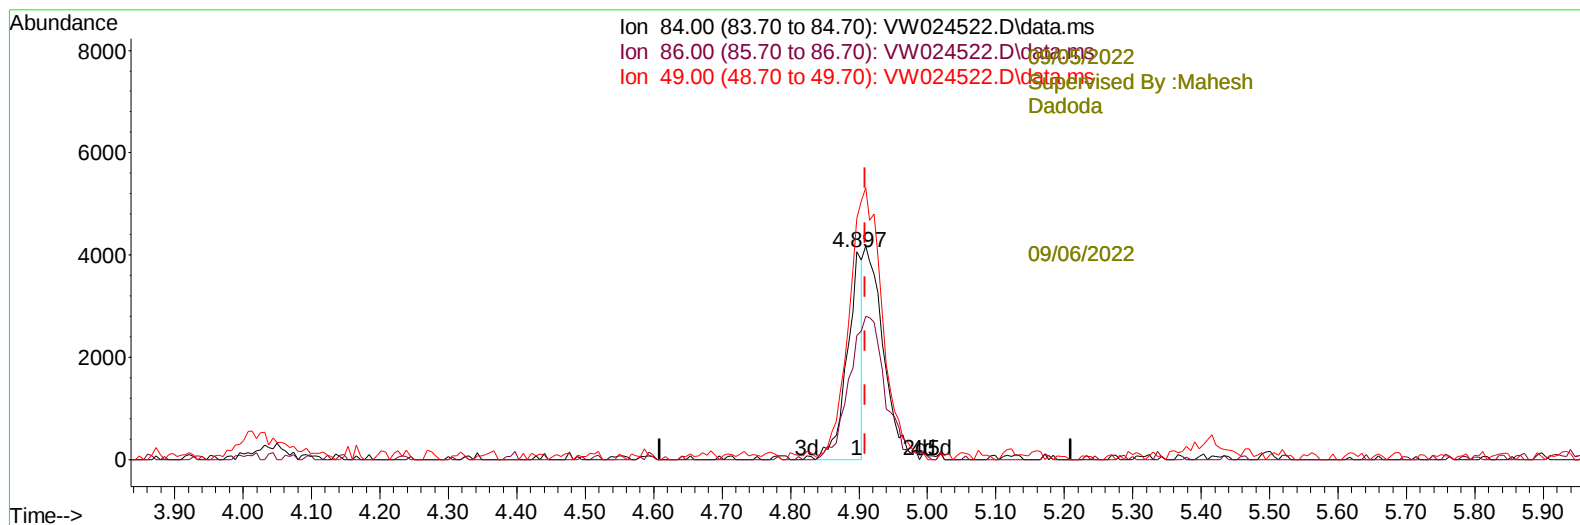

TIC: VW024522.D\data.ms

(16) Methylene chloride (T)

4.897min (-0.012) 1.34 ug/L

response 6239

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	60.10	61.99
49.00	122.20	115.89
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090222\
 Data File : VW024522.D
 Acq On : 02 Sep 2022 09:35
 Operator : SY/VA
 Sample : VSTD2.525
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VSTD2.5425

Manual IntegrationsAPPROVED

Quant Time: Sep 02 23:32:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 02 23:31:46 2022
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

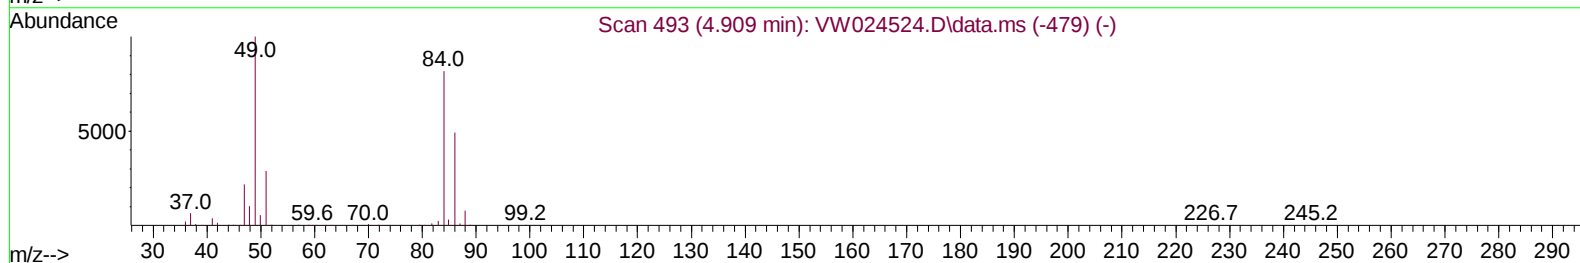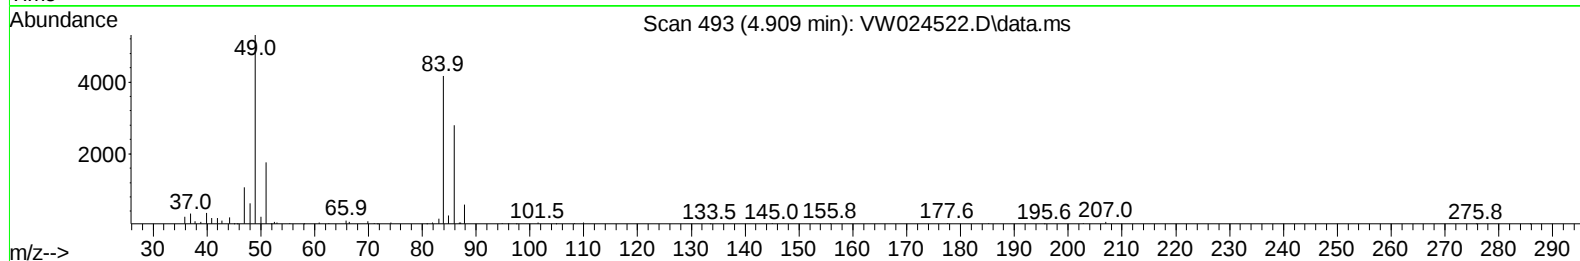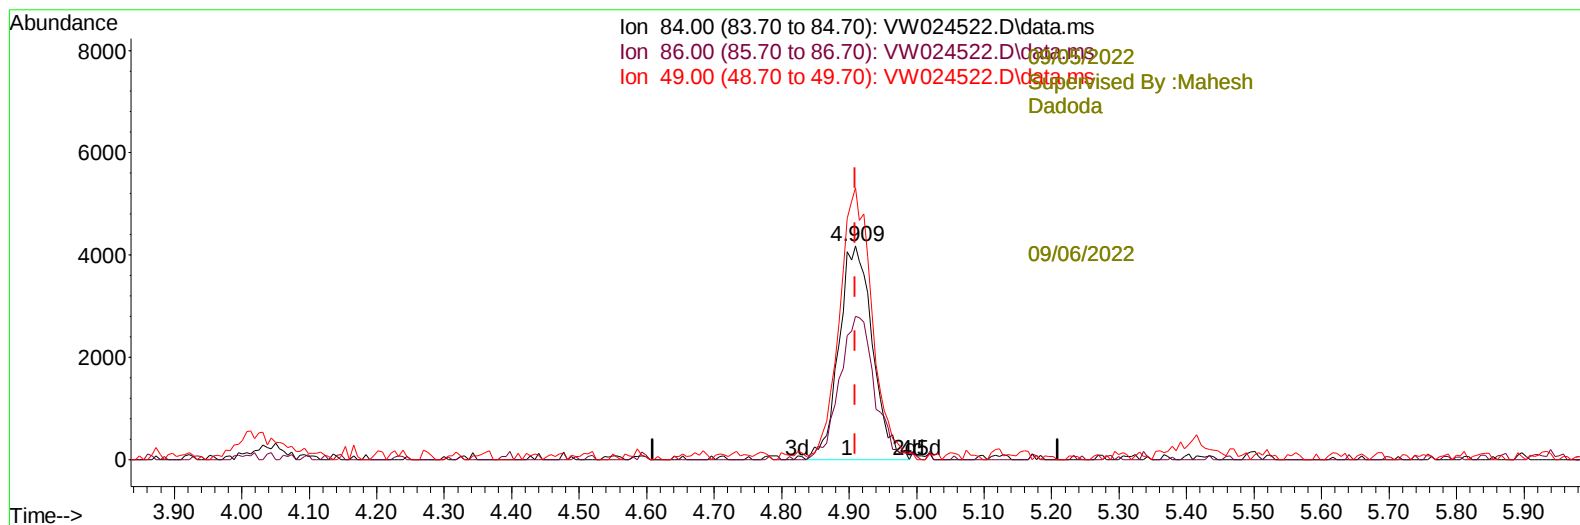

TIC: VW024522.D\data.ms

(16) Methylene chloride (T)

4.909min (+ 0.000) 3.09 ug/L m

response 14377

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	60.10	67.03
49.00	122.20	127.18
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090222\
 Data File : VW024522.D
 Acq On : 02 Sep 2022 09:35
 Operator : SY/VA
 Sample : VSTD2.525
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VSTD2.5425

Manual IntegrationsAPPROVED

Quant Time: Sep 02 23:32:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 02 23:31:46 2022
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

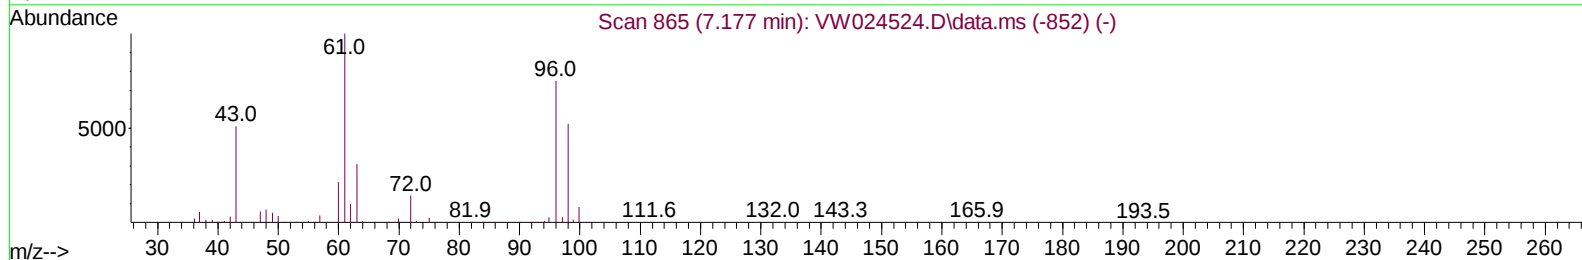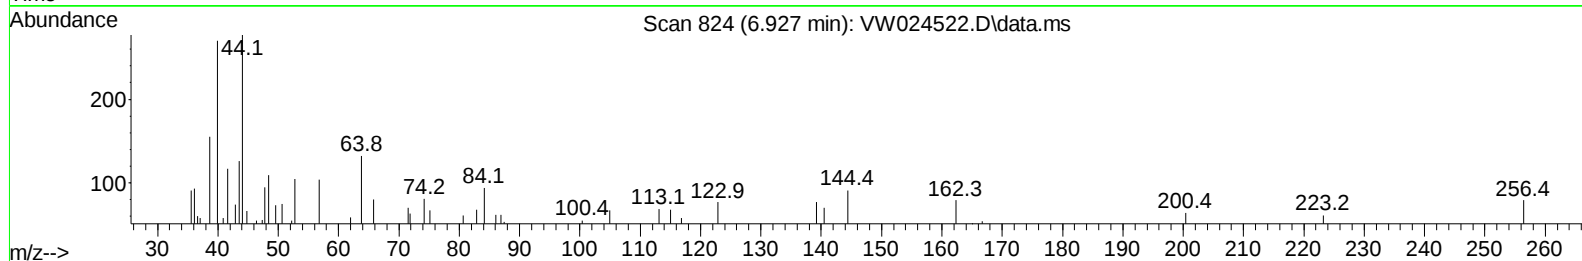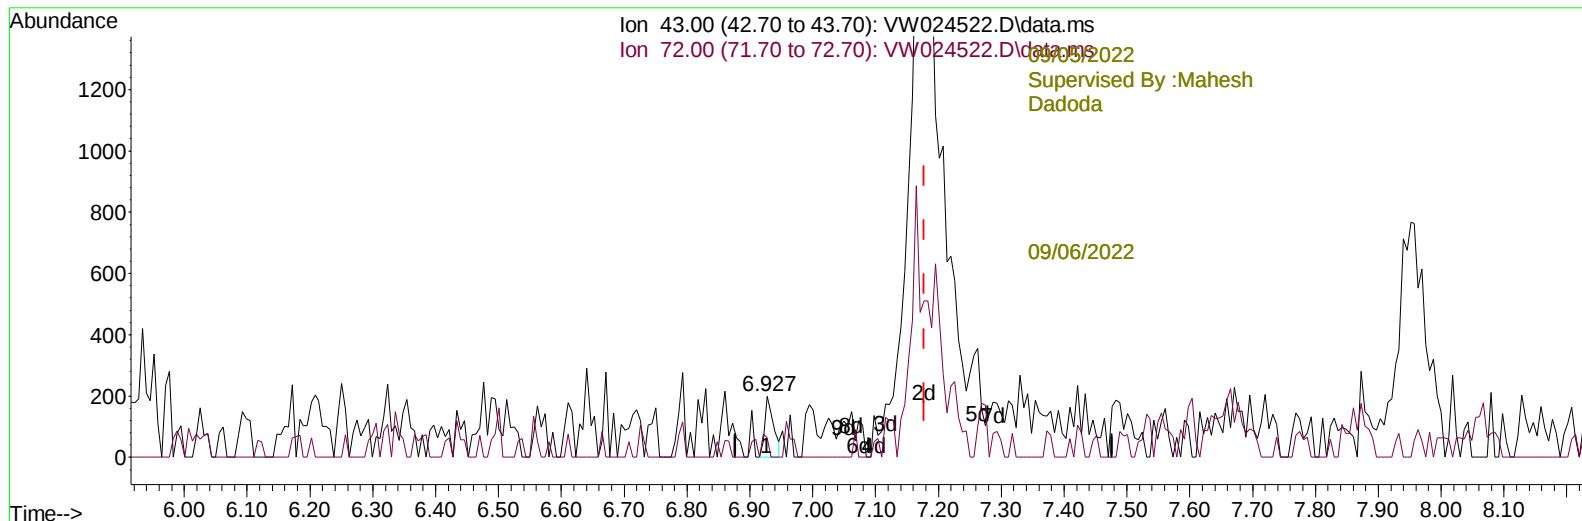

TIC: VW024522.D\data.ms

(22) 2-Butanone (T)

6.927min (-0.250) 0.15 ug/L

response 195

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	29.10	26.15
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090222\
 Data File : VW024522.D
 Acq On : 02 Sep 2022 09:35
 Operator : SY/VA
 Sample : VSTD2.525
 Misc : 5.00g/10mL/MSVOA_W/SoIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VSTD2.5425

Manual IntegrationsAPPROVED

Quant Time: Sep 02 23:32:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 02 23:31:46 2022
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

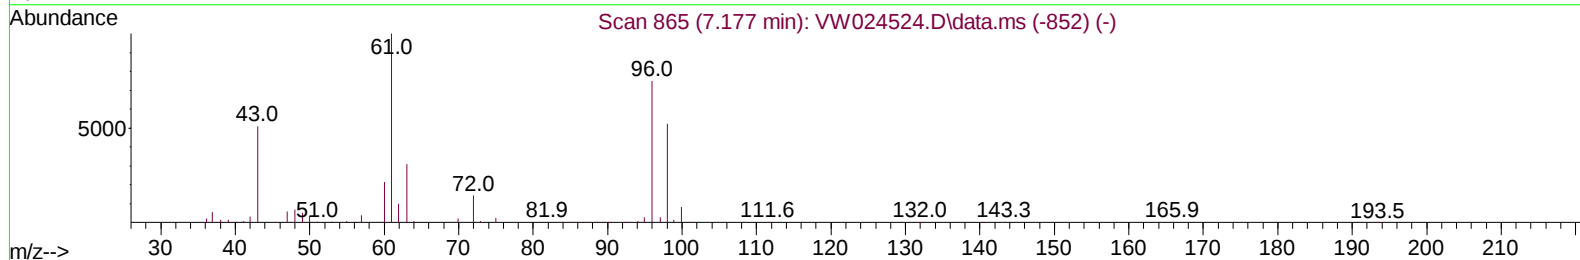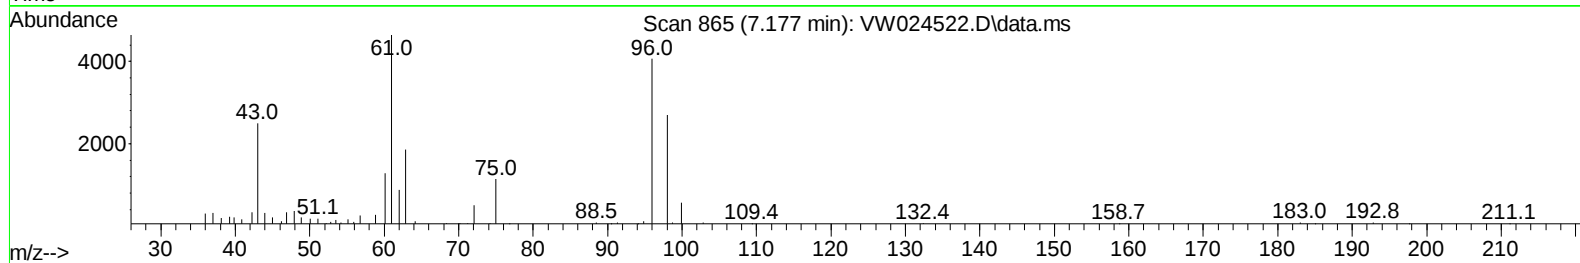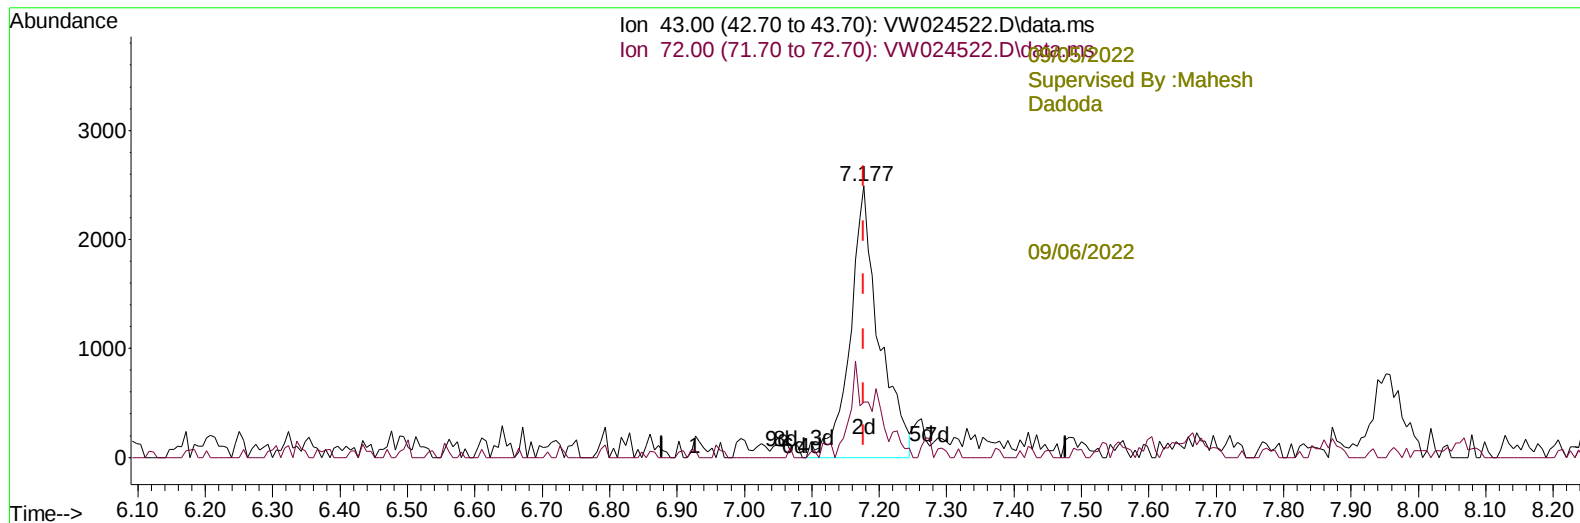

TIC: VW024522.D\data.ms

(22) 2-Butanone (T)

7.177min (+ 0.000) 5.65 ug/L m

response 7394

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	29.10	0.69#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090222\
 Data File : VW024522.D
 Acq On : 02 Sep 2022 09:35
 Operator : SY/VA
 Sample : VSTD2.525
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VSTD2.5425

Manual IntegrationsAPPROVED

Quant Time: Sep 02 23:32:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 02 23:31:46 2022
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

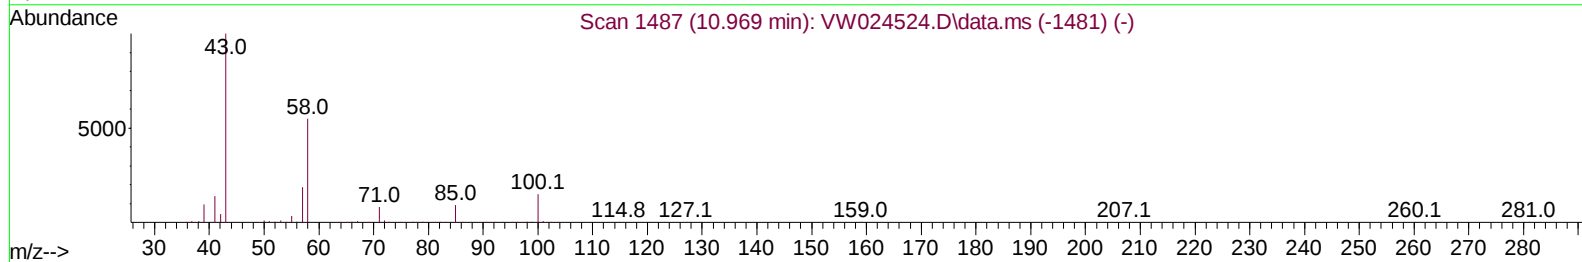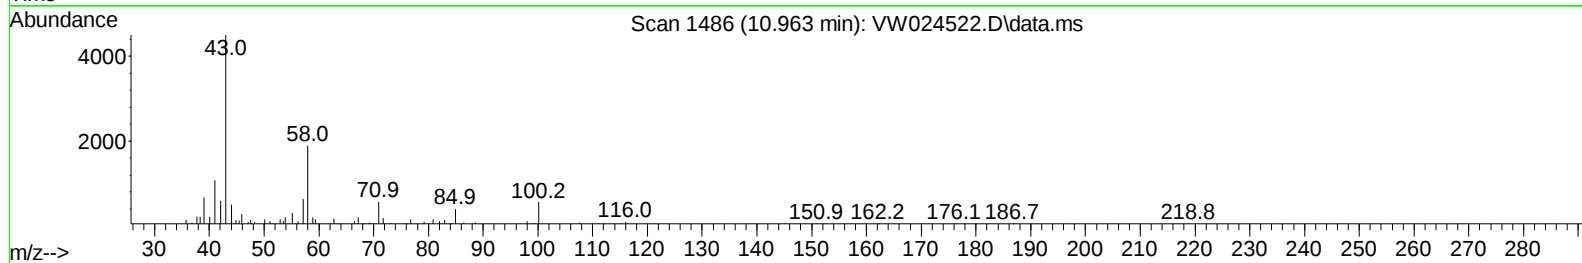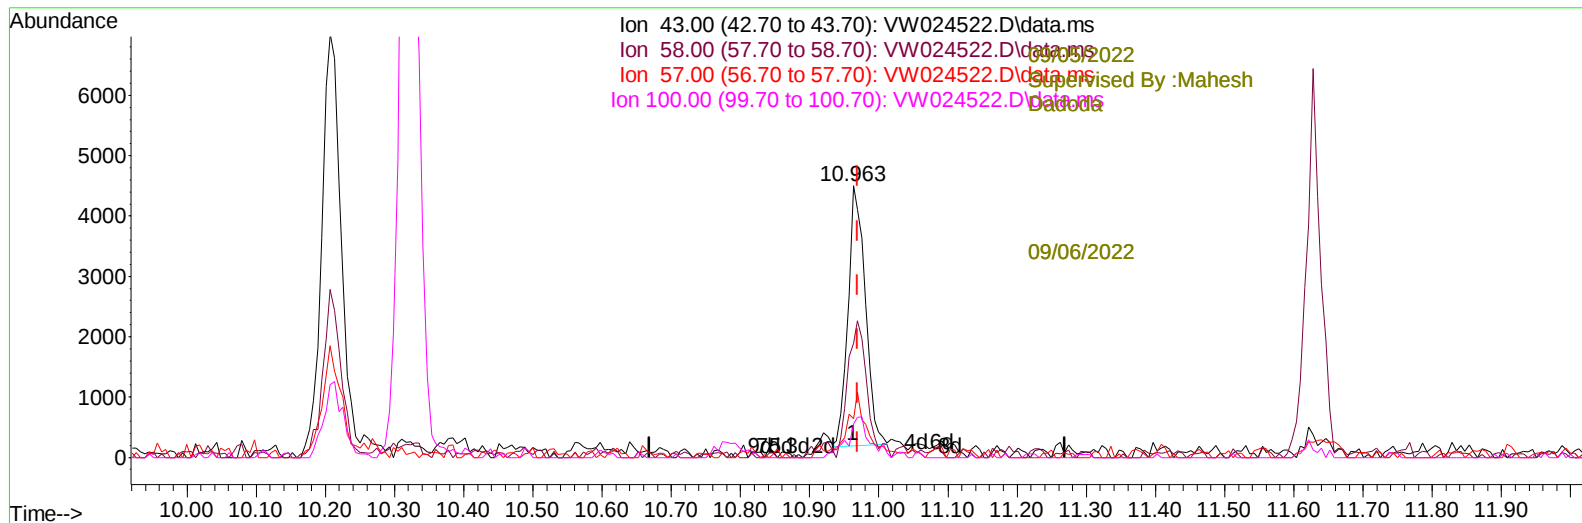

TIC: VW024522.D\data.ms

(48) 2-Hexanone (T)

10.963min (-0.006) 4.15 ug/L

response 7449

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	55.20	56.24
57.00	19.40	18.24
100.00	14.30	13.69




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090222\
Data File : VW024522.D
Acq On : 02 Sep 2022 09:35
Operator : SY/VA
Sample : VSTD2.525
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VSTD2.5425

Manual IntegrationsAPPROVED

Quant Time: Sep 02 23:32:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 02 23:31:46 2022
Response via : Initial Calibration

Reviewed By :Semsettin
Yesilyurt

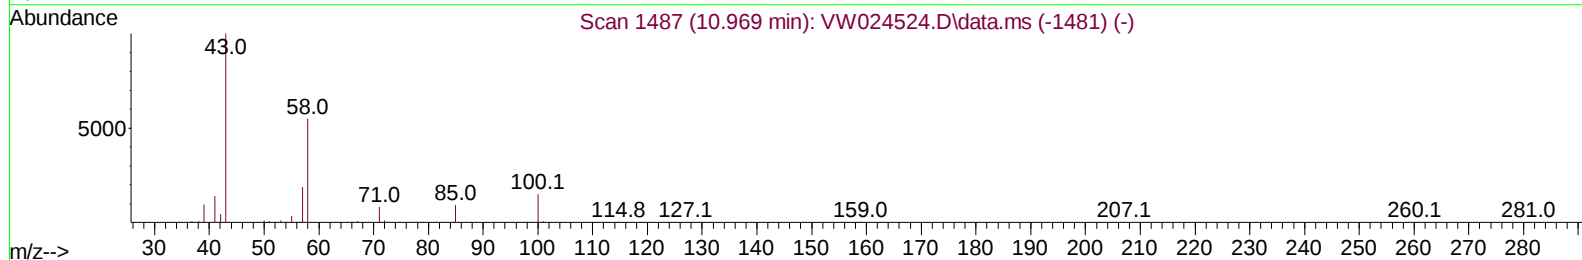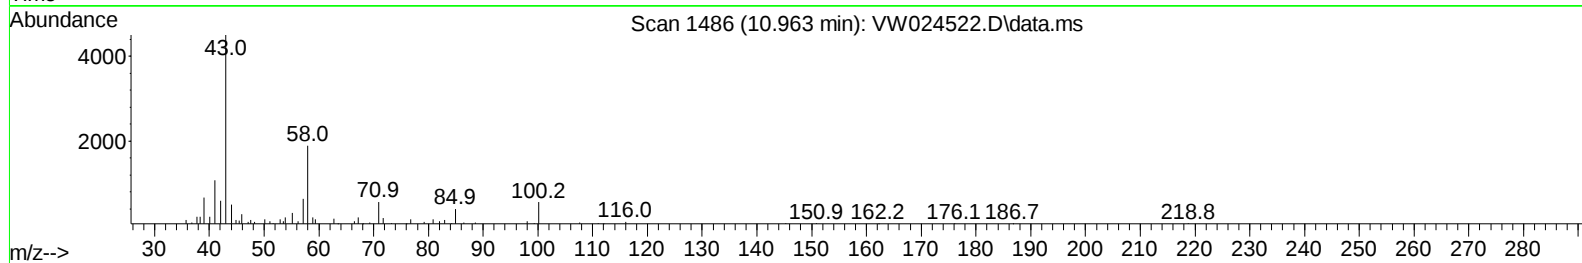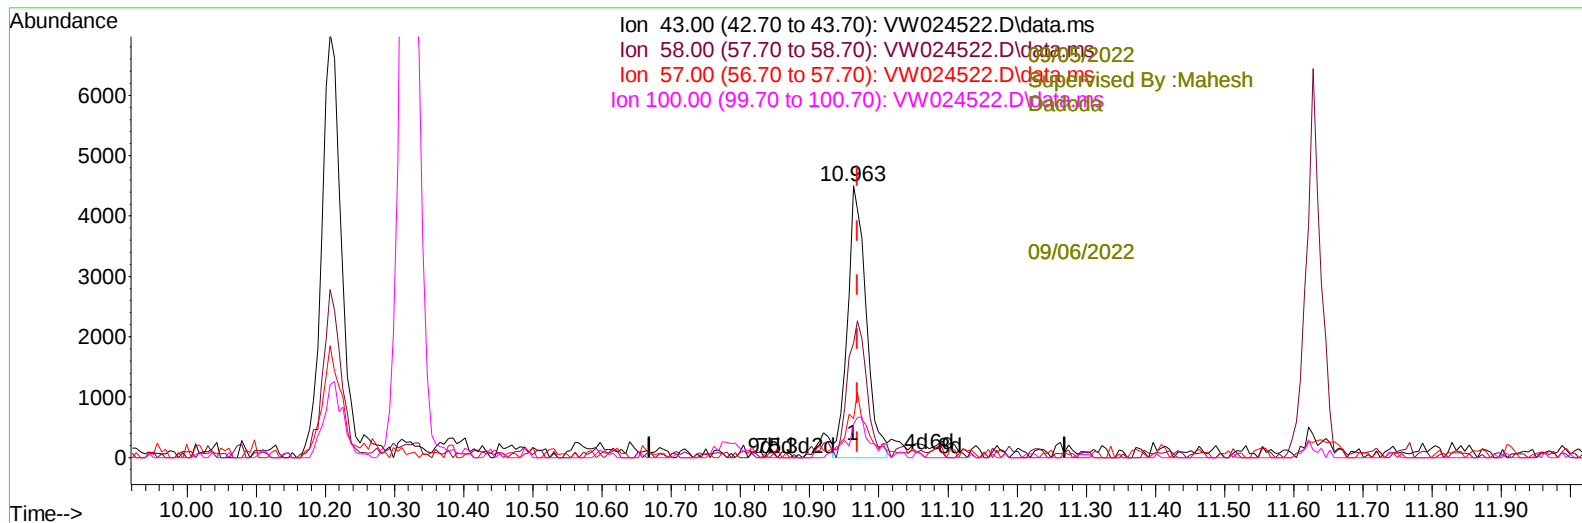

TIC: VW024522.D\data.ms

(48) 2-Hexanone (T)

10.963min (-0.006) 4.67 ug/L m

response 8395

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	55.20	49.90
57.00	19.40	16.19
100.00	14.30	12.15

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090222\
 Data File : VW024522.D
 Acq On : 02 Sep 2022 09:35
 Operator : SY/VA
 Sample : VSTD2.525
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VSTD2.5425

Manual IntegrationsAPPROVED

Quant Time: Sep 02 23:32:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 02 23:31:46 2022
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----09/05/2022						
Supervised By :Mahesh						
Padoda						
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	329030	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	309477	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	149719	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	16366	2.492	ug/L	0.00
7) Chloroethane-d5	2.873	69	12151	2.485	ug/L	0.00
11) 1,1-Dichloroethene-d2	4.007	63	20209	2.613	ug/L	0.00
21) 2-Butanone-d5	7.092	46	5777	5.505	ug/L	0.02
24) Chloroform-d	7.647	84	24212	2.763	ug/L	0.00
26) 1,2-Dichloroethane-d4	8.305	65	13444	2.841	ug/L	0.00
32) Benzene-d6	8.275	84	43246	2.679	ug/L	0.00
36) 1,2-Dichloropropane-d6	9.274	67	13309	2.817	ug/L	0.00
41) Toluene-d8	10.323	98	38169	2.483	ug/L	0.00
43) trans-1,3-Dichloroprop...	10.573	79	5309	2.576	ug/L	0.00
47) 2-Hexanone-d5	10.927	63	3800	4.696	ug/L	0.00
56) 1,1,2,2-Tetrachloroeth...	12.688	84	11838	2.757	ug/L	0.00
66) 1,2-Dichlorobenzene-d4	13.853	152	13072	2.669	ug/L	0.00
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	2.001	85	1915m	2.132	ug/L	
3) Chloromethane	2.215	50	12384	2.703	ug/L	97
5) Vinyl chloride	2.349	62	23502	2.901	ug/L	92
6) Bromomethane	2.769	94	15534	2.816	ug/L	89
8) Chloroethane	2.904	64	11729	2.727	ug/L	96
9) Trichlorofluoromethane	3.239	101	6711m	2.187	ug/L	
10) 1,1,2-Trichloro-1,2,2-...	4.056	101	13024	2.831	ug/L	98
12) 1,1-Dichloroethene	4.038	96	11043m	2.723	ug/L	
13) Acetone	4.117	43	4949	6.141	ug/L	97
14) Carbon disulfide	4.367	76	30677	2.746	ug/L	100
15) Methyl Acetate	4.672	43	5674m	3.097	ug/L	
16) Methylene chloride	4.909	84	14377m	3.087	ug/L	
17) trans-1,2-Dichloroethene	5.415	96	11878	2.636	ug/L	94
18) Methyl tert-butyl Ether	5.421	73	18725	2.399	ug/L #	68
19) 1,1-Dichloroethane	6.208	63	22214	2.722	ug/L	96
20) cis-1,2-Dichloroethene	7.165	96	12862	2.622	ug/L	93
22) 2-Butanone	7.177	43	7394m	5.649	ug/L	
23) Bromochloromethane	7.513	128	6379	2.803	ug/L	80
25) Chloroform	7.671	83	24787	2.766	ug/L	97
27) 1,2-Dichloroethane	8.397	62	15821	2.688	ug/L	97
29) Cyclohexane	7.958	56	16288	2.535	ug/L	93
30) 1,1,1-Trichloroethane	7.872	97	19311	2.759	ug/L	99
31) Carbon tetrachloride	8.073	117	17467	2.752	ug/L	97
33) Benzene	8.323	78	50396	2.738	ug/L	100
34) Trichloroethene	9.085	95	13689	2.802	ug/L	91
35) Methylcyclohexane	9.335	83	19555	2.530	ug/L	97
37) 1,2-Dichloropropane	9.372	63	12196	2.750	ug/L #	90
38) Bromodichloromethane	9.646	83	16156	2.577	ug/L	95
39) cis-1,3-Dichloropropene	10.073	75	15833	2.371	ug/L	97
40) 4-Methyl-2-pentanone	10.207	43	13600	4.931	ug/L	97
42) Toluene	10.384	91	50347	2.512	ug/L	98

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090222\
 Data File : VW024522.D
 Acq On : 02 Sep 2022 09:35
 Operator : SY/VA
 Sample : VSTD2.525
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VSTD2.5425

Manual IntegrationsAPPROVED

Quant Time: Sep 02 23:32:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 02 23:31:46 2022
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)	
44) trans-1,3-Dichloropropene	10.603	75		13593	2.270	ug/L		09/05/2022
45) 1,1,2-Trichloroethane	10.780	97		9829	2.655	ug/L		Supervised By :Mahesh
46) Tetrachloroethene	10.853	164		8928	2.501	ug/L		Padoda
48) 2-Hexanone	10.963	43		8395m	4.672	ug/L		94
49) Dibromochloromethane	11.128	129		10658	2.450	ug/L		91
50) 1,2-Dibromoethane	11.231	107		9050	2.581	ug/L #		95
51) Chlorobenzene	11.658	112		36140	2.657	ug/L		09/06/2022
52) Ethylbenzene	11.725	91		54491	2.429	ug/L		97
53) m,p-Xylene	11.841	106		20587	2.347	ug/L		93
54) o-Xylene	12.164	106		19514	2.324	ug/L		97
55) Styrene	12.176	104		31816	2.181	ug/L		98
57) 1,1,2,2-Tetrachloroethane	12.713	83		12141	2.650	ug/L		94
59) Bromoform	12.347	173		5304	2.440	ug/L #		99
60) Isopropylbenzene	12.463	105		50907	2.405	ug/L		98
61) 1,2,3-Trichloropropane	12.768	75		8307	2.748	ug/L		93
62) 1,3,5-Trimethylbenzene	12.938	105		39882	2.284	ug/L		97
63) 1,2,4-Trimethylbenzene	13.249	105		37421	2.190	ug/L		99
64) 1,3-Dichlorobenzene	13.499	146		23310	2.472	ug/L		97
65) 1,4-Dichlorobenzene	13.579	146		26249	2.718	ug/L		98
67) 1,2-Dichlorobenzene	13.865	146		21493	2.469	ug/L		87
68) 1,2-Dibromo-3-chloropr...	14.475	75		2080	3.040	ug/L #		64
69) 1,3,5-Trichlorobenzene	14.621	180		15242	2.515	ug/L		95
70) 1,2,4-trichlorobenzene	15.127	180		10224	2.206	ug/L		96
71) Naphthalene	15.359	128		19717	2.012	ug/L		99
72) 1,2,3-Trichlorobenzene	15.548	180		9624	2.302	ug/L		98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

