

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW090620\
 Data File : VW016470.D
 Acq On : 06 Sep 2020 09:19
 Operator : SY/VA
 Sample : VW0906SBL01
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Sep 07 04:51:51 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM090320S.M
 Quant Title : VOC Analysis
 QLast Update : Mon Sep 07 04:50:36 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	683474	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	621013	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	284842	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	168669	23.26	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.04%
7) Chloroethane-d5	2.90	69	164733	25.30	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	101.20%
10) 1,1-Dichloroethene-d2	4.03	63	289214	17.35	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	69.40%
20) 2-Butanone-d5	7.09	46	90710	35.03	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	70.06%
24) Chloroform-d	7.65	84	388711	24.28	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	97.12%
26) 1,2-Dichloroethane-d4	8.47	65	115	0.01	ug/L	0.16
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.04%#
29) Benzene-d6	8.28	84	788159	24.96	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	99.84%
33) 1,2-Dichloropropane-d6	9.28	67	221954	23.93	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.72%
37) Toluene-d8	10.33	98	761782	25.39	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	101.56%
38) trans-1,3-Dichloropropene-	10.58	79	106351	22.73	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	90.92%
39) 2-Hexanone-d5	10.93	63	80806	42.63	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.26%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	175199	22.34	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	89.36%
61) 1,2-Dichlorobenzene-d4	13.85	152	261497	26.57	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	106.28%


Target Compounds					Ovalue
42) cis-1,3-Dichloropropene	10.04	75	8702	0.611 ug/L #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW090620\
Data File : VW016470.D
Acq On : 06 Sep 2020 09:19
Operator : SY/VA
Sample : VW0906SBL01
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Sep 07 04:51:51 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM090320S.M
Quant Title : VOC Analysis
QLast Update : Mon Sep 07 04:50:36 2020
Response via : Initial Calibration

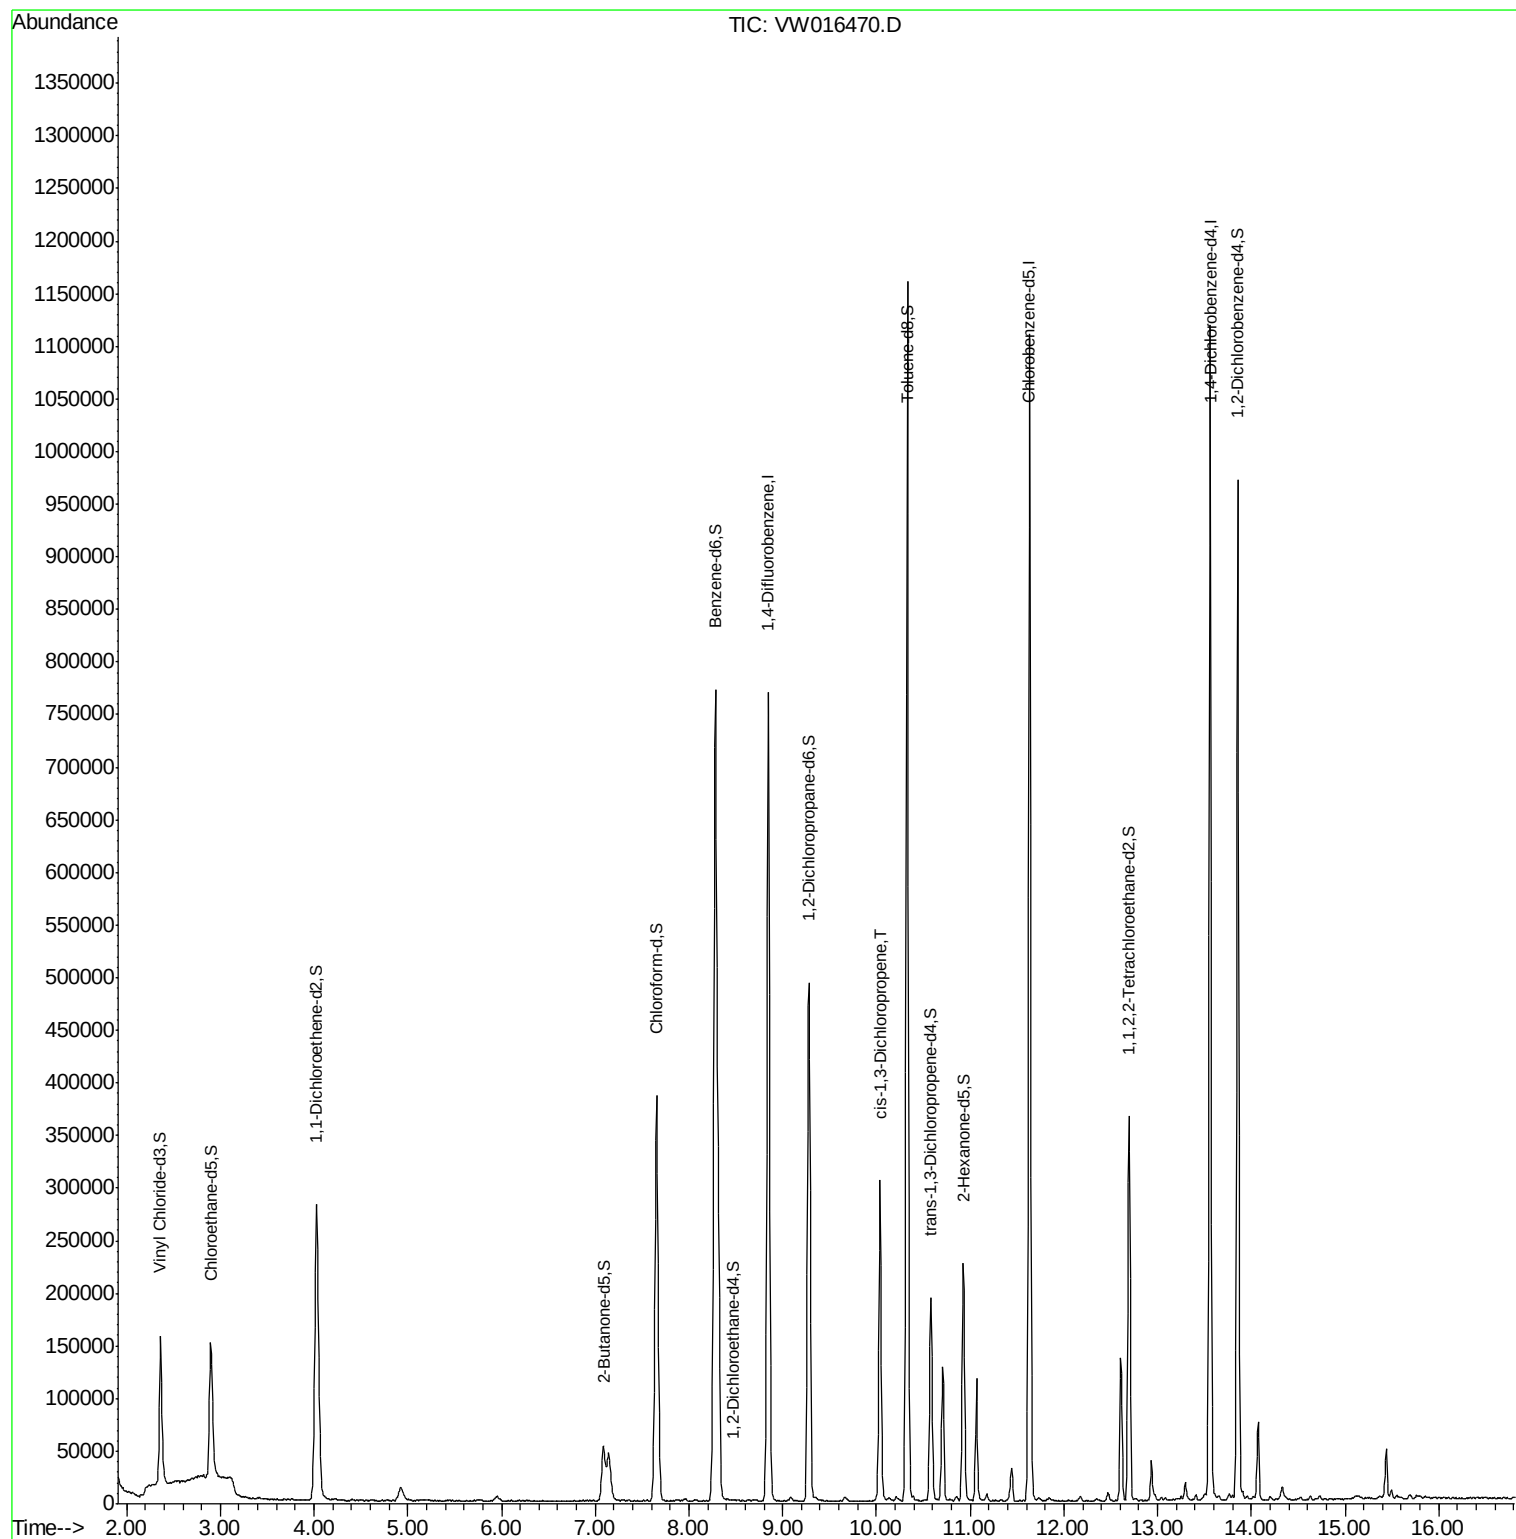

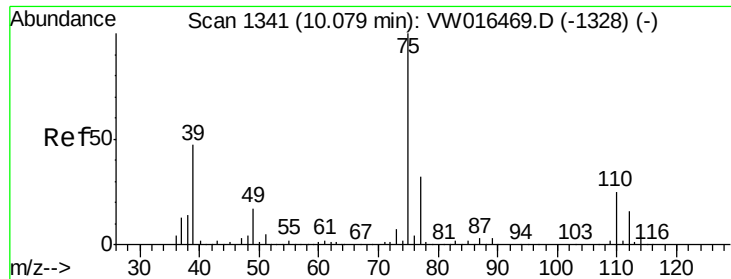

#42
 cis-1,3-Dichloropropene
 Concen: 0.611 ug/L
 RT: 10.04 min Scan# 1334
 Delta R.T. -0.04 min
 Lab File: VW016470.D
 Acq: 06 Sep 2020 09:19

Instrument :
 MSVOA_W
 ClientSampleId :

Tot Ion: 75 Resp: 8702
 Ion Ratio Lower Upper
 75 100
 77 46.5 20.9 38.7#

