

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW090620\
 Data File : VW016480.D
 Acq On : 06 Sep 2020 13:27
 Operator : SY/VA
 Sample : L3927-11
 Misc : 6.22G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Sep 07 04:52:36 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM090320S.M
 Quant Title : VOC Analysis
 QLast Update : Mon Sep 07 04:50:36 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	710738	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	629026	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	275264	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	204706	27.15	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	108.60%
7) Chloroethane-d5	2.90	69	174555	25.78	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	103.12%
10) 1,1-Dichloroethene-d2	4.03	63	309285	17.84	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	71.36%
20) 2-Butanone-d5	7.08	46	90193	33.49	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	66.98%
24) Chloroform-d	7.65	84	391361	23.51	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.04%
26) 1,2-Dichloroethane-d4	8.31	65	206176	22.65	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	90.60%
29) Benzene-d6	8.28	84	799212	24.99	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	99.96%
33) 1,2-Dichloropropane-d6	9.28	67	222338	23.67	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	94.68%
37) Toluene-d8	10.33	98	774182	25.47	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	101.88%
38) trans-1,3-Dichloropropene-	10.58	79	106589	22.49	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.96%
39) 2-Hexanone-d5	10.93	63	75650	39.40	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	78.80%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	167979	21.14	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	84.56%
61) 1,2-Dichlorobenzene-d4	13.85	152	248982	26.17	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	104.68%


Target Compounds					Ovalue
59) 1,2,3-Trichloropropane	13.56	75	35907	5.980 ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW090620\
Data File : VW016480.D
Acq On : 06 Sep 2020 13:27
Operator : SY/VA
Sample : L3927-11
Misc : 6.22G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Sep 07 04:52:36 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM090320S.M
Quant Title : VOC Analysis
QLast Update : Mon Sep 07 04:50:36 2020
Response via : Initial Calibration

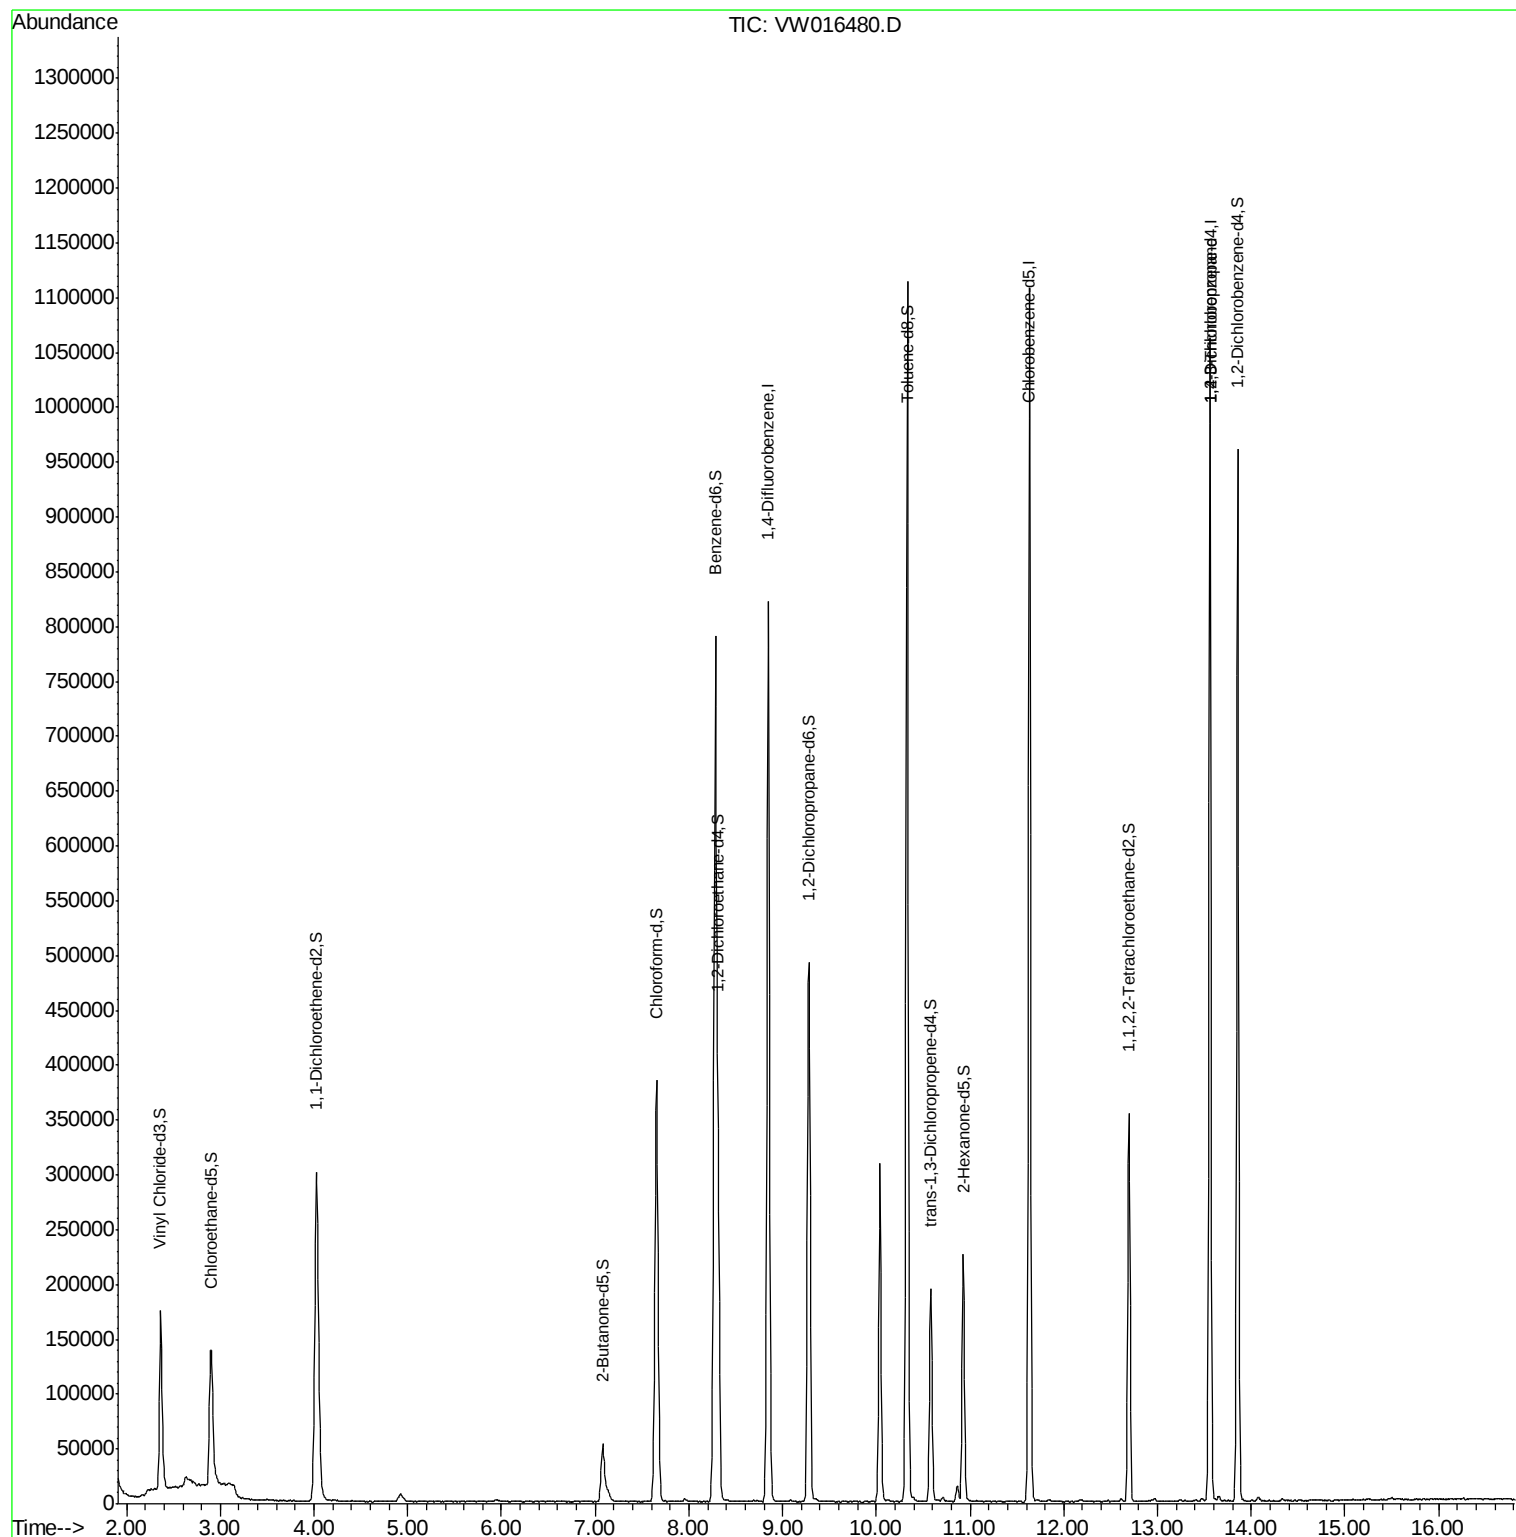

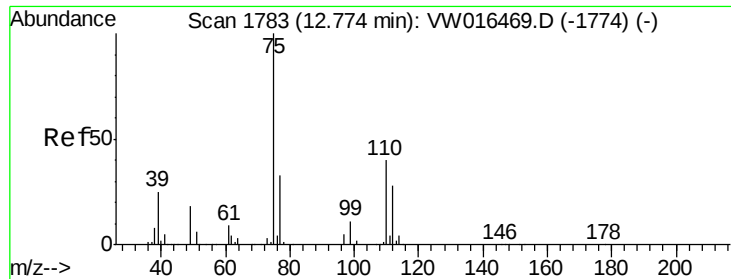

#59

1,2,3-Trichloropropane

Concen: 5.980 ug/L

RT: 13.56 min Scan# 1912

Delta R.T. 0.79 min

Lab File: VW016480.D

Acq: 06 Sep 2020 13:27

Instrument :

MSVOA_W

ClientSampleId :

Tot Ion: 75 Resp: 35907

Ion Ratio Lower Upper

75 100

77 37.4 26.0 39.0

