

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW090620\
 Data File : VW016482.D
 Acq On : 06 Sep 2020 14:14
 Operator : SY/VA
 Sample : L3927-13
 Misc : 5.61G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Sep 07 04:52:46 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM090320S.M
 Quant Title : VOC Analysis
 QLast Update : Mon Sep 07 04:50:36 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	703453	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	612566	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	265117	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	210578	28.22	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	112.88%
7) Chloroethane-d5	2.90	69	174809	26.08	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	104.32%
10) 1,1-Dichloroethene-d2	4.03	63	317128	18.48	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	73.92%
20) 2-Butanone-d5	7.08	46	73344	27.52	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	55.04%
24) Chloroform-d	7.65	84	396142	24.04	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.16%
26) 1,2-Dichloroethane-d4	8.31	65	192748	21.39	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	85.56%
29) Benzene-d6	8.28	84	808585	25.97	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	103.88%
33) 1,2-Dichloropropane-d6	9.28	67	219527	24.00	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.00%
37) Toluene-d8	10.33	98	771915	26.08	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	104.32%
38) trans-1,3-Dichloropropene-	10.58	79	96611	20.93	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.72%
39) 2-Hexanone-d5	10.93	63	63024	33.70	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	67.40%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	143718	18.58	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	74.32%
61) 1,2-Dichlorobenzene-d4	13.85	152	234716	25.62	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	102.48%


Target Compounds					Ovalue
59) 1,2,3-Trichloropropane	13.56	75	33065	5.654 ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW090620\
Data File : VW016482.D
Acq On : 06 Sep 2020 14:14
Operator : SY/VA
Sample : L3927-13
Misc : 5.61G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Sep 07 04:52:46 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM090320S.M
Quant Title : VOC Analysis
QLast Update : Mon Sep 07 04:50:36 2020
Response via : Initial Calibration

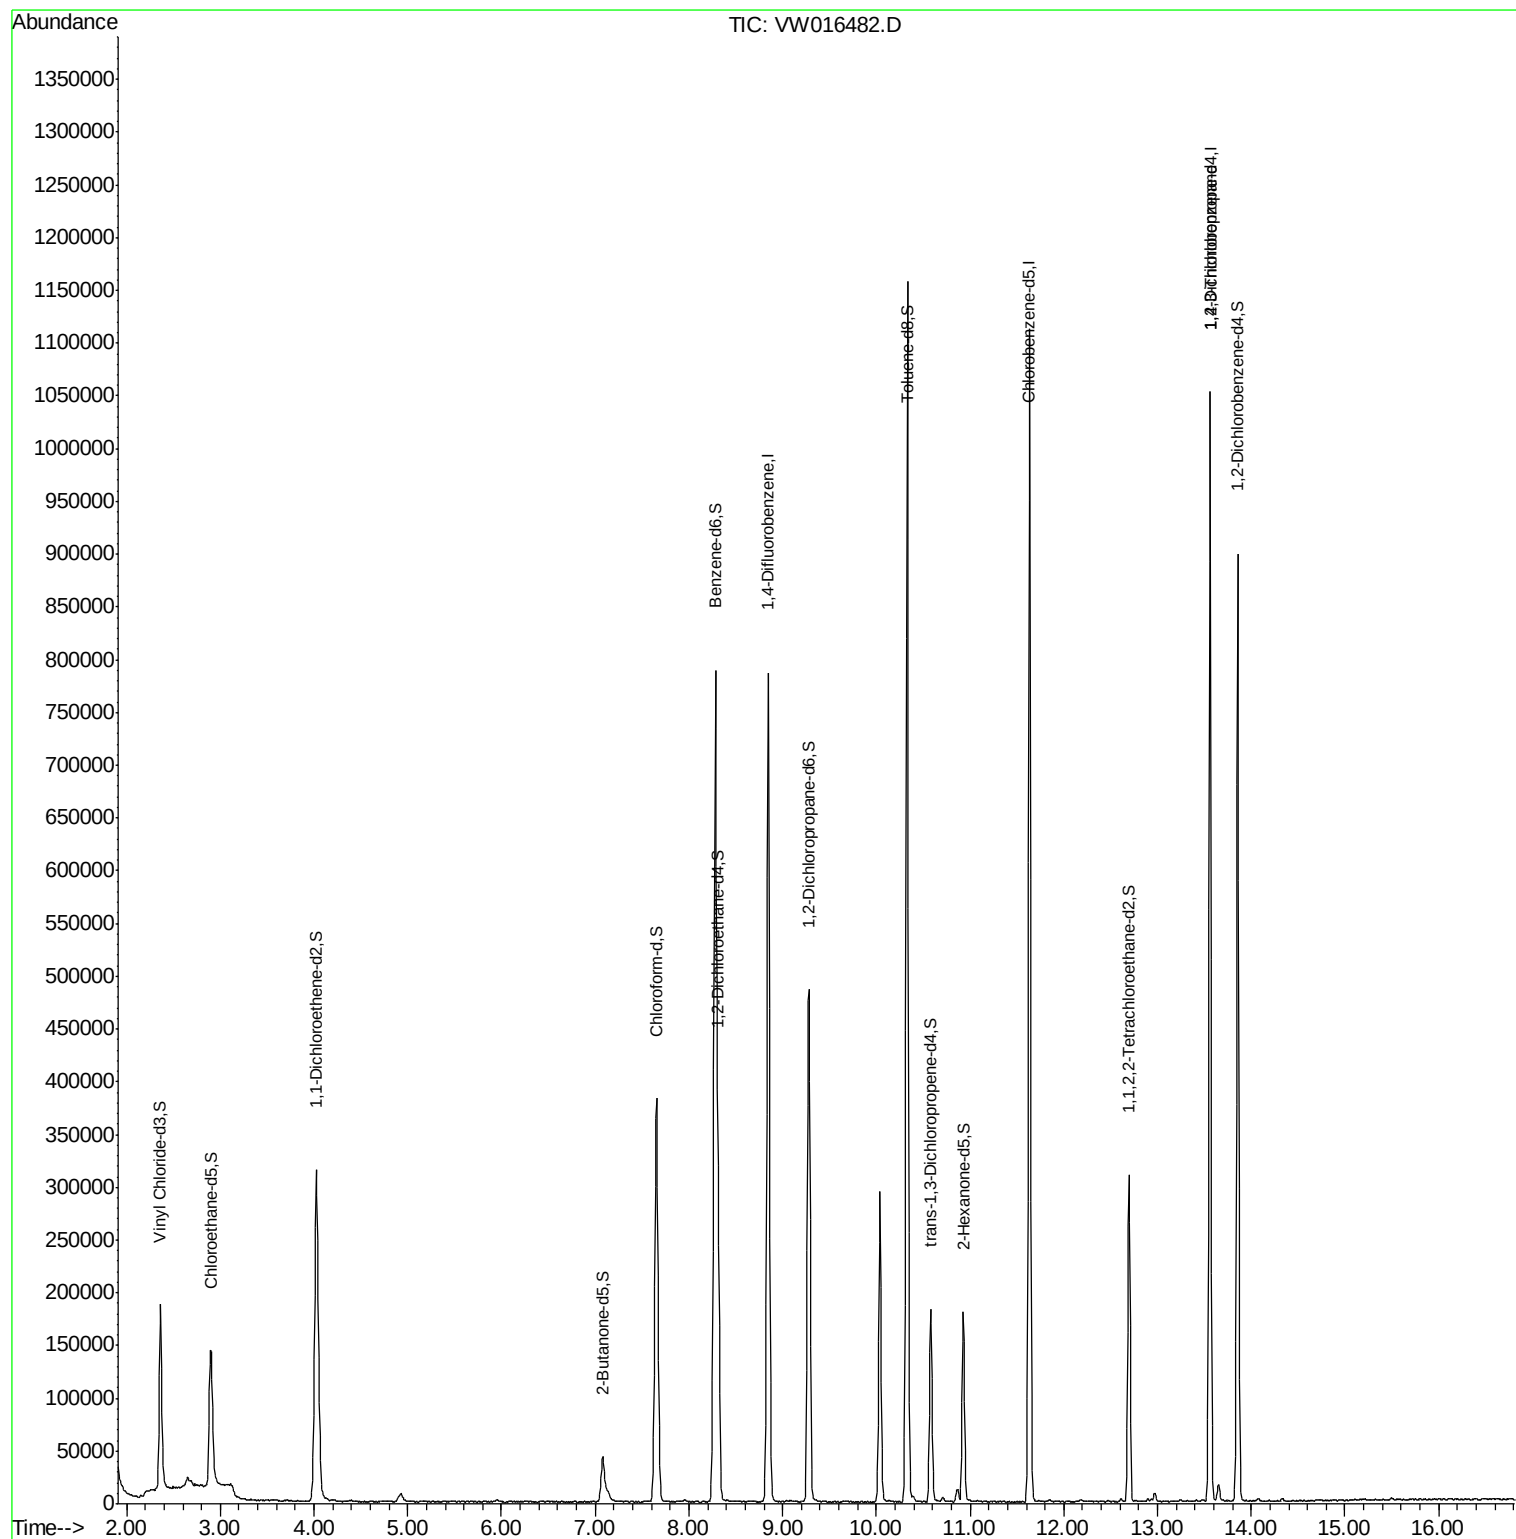

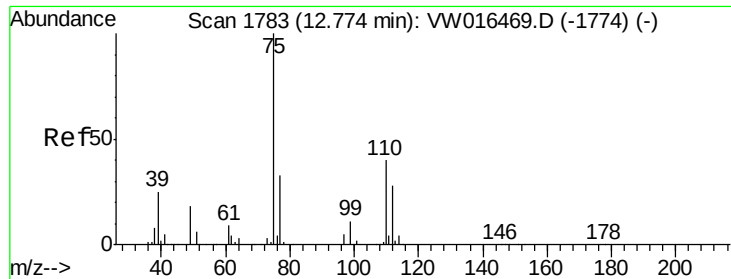

#59

1,2,3-Trichloropropane

Concen: 5.654 ug/L

RT: 13.56 min Scan# 1912

Delta R.T. 0.79 min

Lab File: VW016482.D

Acq: 06 Sep 2020 14:14

Instrument :

MSVOA_W

ClientSampleId :

Tot Ion: 75 Resp: 33065

Ion Ratio Lower Upper

75 100

77 38.9 26.0 39.0

