

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW090719\
 Data File : VW012753.D
 Acq On : 08 Sep 2019 07:33
 Operator : SY/VA
 Sample : K4636-07
 Misc : 5.04G/5ML/MSVOA W/SOIL
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 SB-22-6.5-7.0

Quant Time: Sep 09 04:34:51 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W090719S.M
 Quant Title : SW846 8260
 QLast Update : Sun Sep 08 05:04:40 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	213390	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	330419	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	265679	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.56	152	71432	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.31	65	129218	54.20	ug/l	0.00
Spiked Amount	50.000		Recovery	=	108.40%	
35) Dibromofluoromethane	7.88	113	99454	50.63	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.26%	
50) Toluene-d8	10.32	98	410567	53.35	ug/l	0.00
Spiked Amount	50.000		Recovery	=	106.70%	
62) 4-Bromofluorobenzene	12.62	95	101364	36.28	ug/l	0.00
Spiked Amount	50.000		Recovery	=	72.56%	


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW090719\
Data File : VW012753.D
Acq On : 08 Sep 2019 07:33
Operator : SY/VA
Sample : K4636-07
Misc : 5.04G/5ML/MSVOA W/SOIL
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
SB-22-6.5-7.0

Quant Time: Sep 09 04:34:51 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W090719S.M
Quant Title : SW846 8260
QLast Update : Sun Sep 08 05:04:40 2019
Response via : Initial Calibration

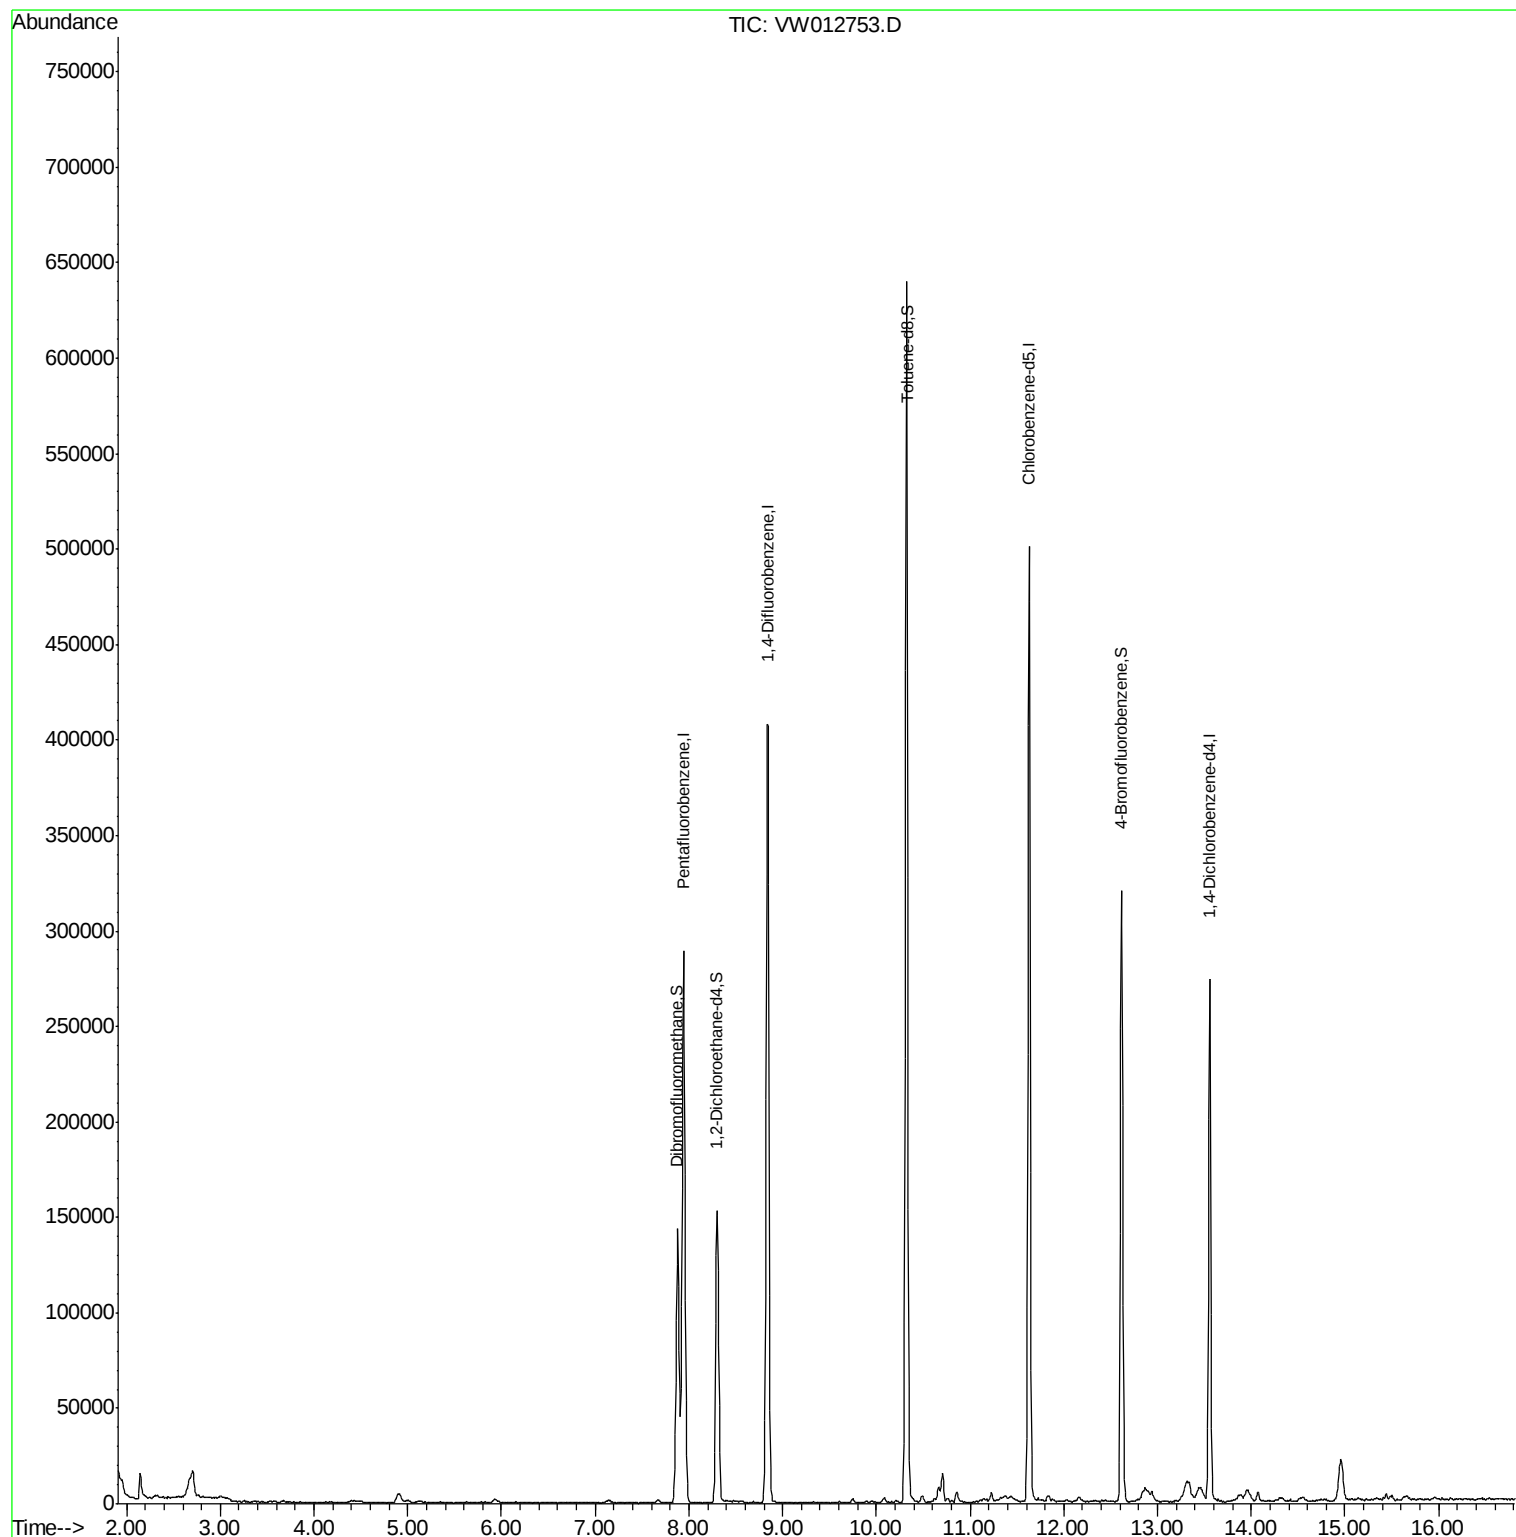



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 991

Delta R.T. 0.00 min

Lab File: VW012753.D

Acq: 08 Sep 2019 07:33

Instrument :

MSVOA_W

ClientSampleId :


SB-22-6.5-7.0

Tot Ion:168 Resp: 213390

Ion Ratio Lower Upper

168 100

99 58.2 47.8 71.6

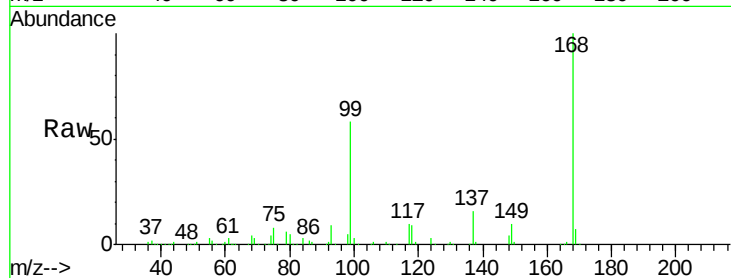

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

7.95

100000

80000



60000

40000

20000

0

Time-->

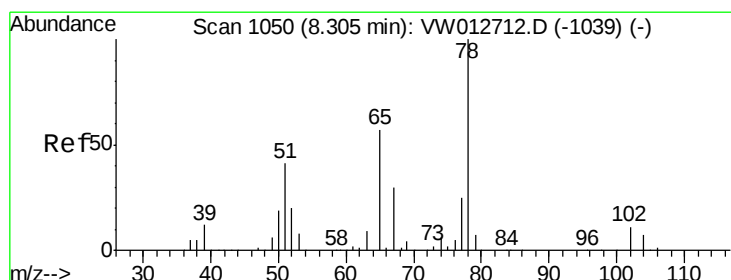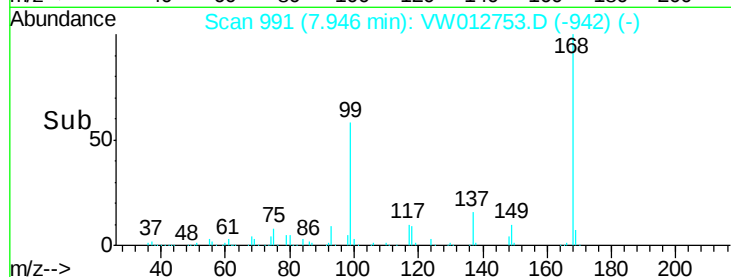

#33

1,2-Dichloroethane-d4

Concen: 54.196 ug/l

RT: 8.31 min Scan# 1050

Delta R.T. 0.00 min

Lab File: VW012753.D


Acq: 08 Sep 2019 07:33

Tgt Ion: 65 Resp: 129218

Ion Ratio Lower Upper

65 100

67 49.2 0.0 101.8

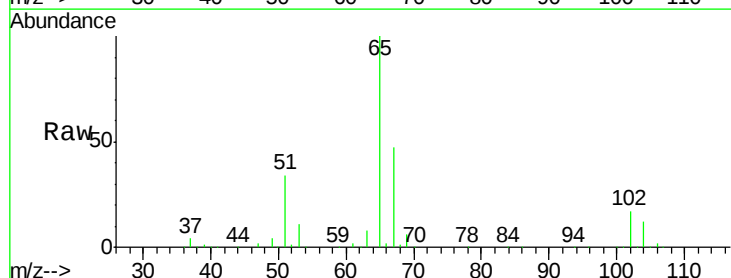

Abundance Ion 64.90 (64.60 to 65.60): VW

Ion 66.90 (66.60 to 67.60): VW

8.31


60000


40000

20000

0

Time-->

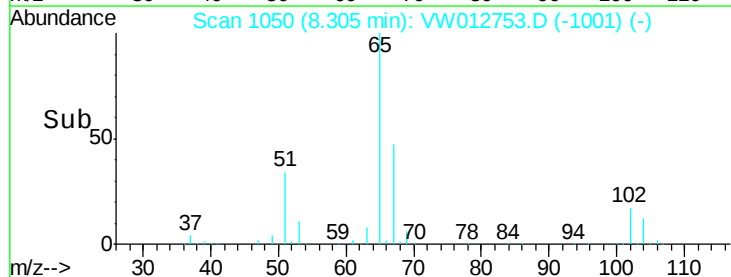

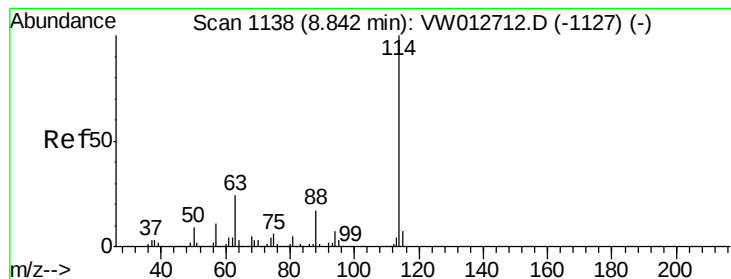

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.84 min Scan# 1138

Delta R.T. 0.00 min

Lab File: VW012753.D

Acq: 08 Sep 2019 07:33

Instrument :

MSVOA_W

ClientSampleId :

SB-22-6.5-7.0


Tot Ion:114 Resp: 330419

Ion Ratio Lower Upper

114 100

63 22.9 0.0 47.2




88 16.7 0.0 34.0

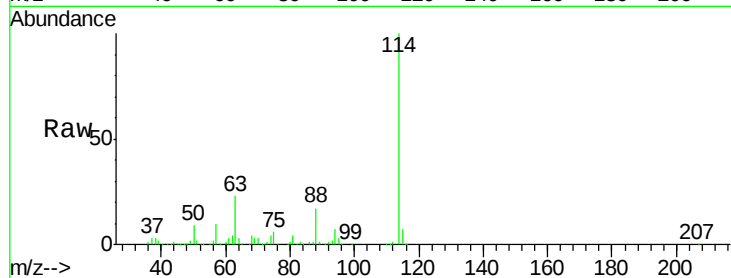

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VW

Ion 87.90 (87.60 to 88.60): VW

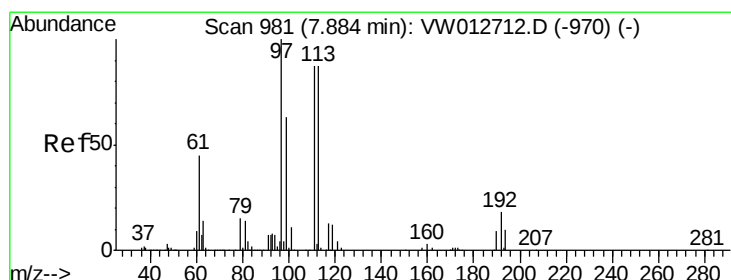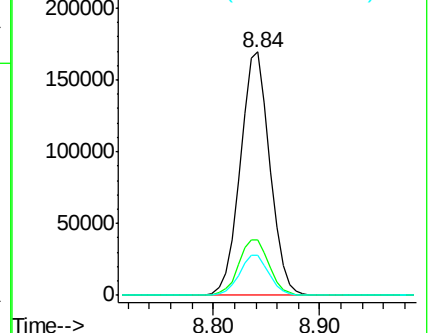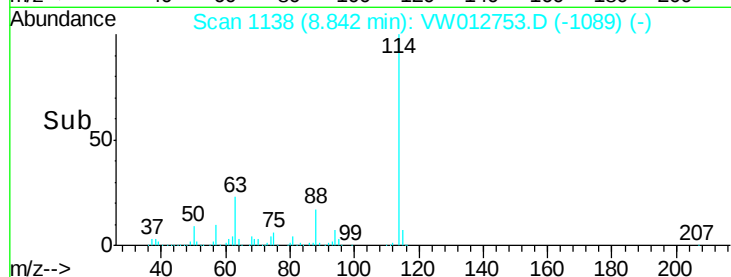

#35

Dibromofluoromethane

Concen: 50.627 ug/l

RT: 7.88 min Scan# 980

Delta R.T. -0.01 min

Lab File: VW012753.D

Acq: 08 Sep 2019 07:33


Tgt Ion:113 Resp: 99454

Ion Ratio Lower Upper

113 100

111 102.4 80.2 120.4



192 22.2 17.3 25.9

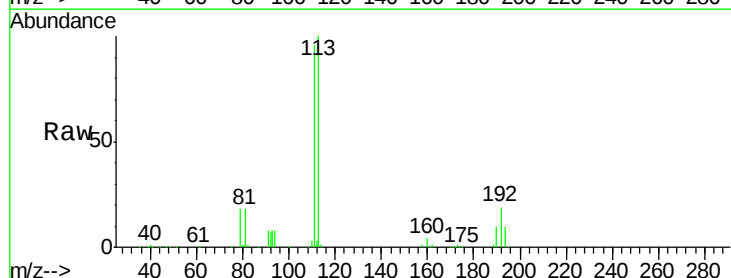


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

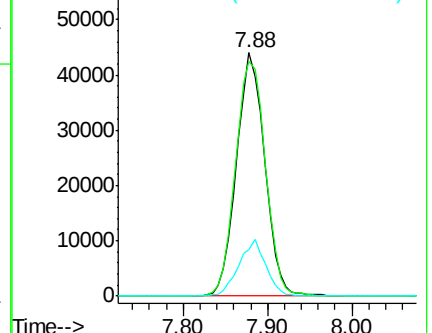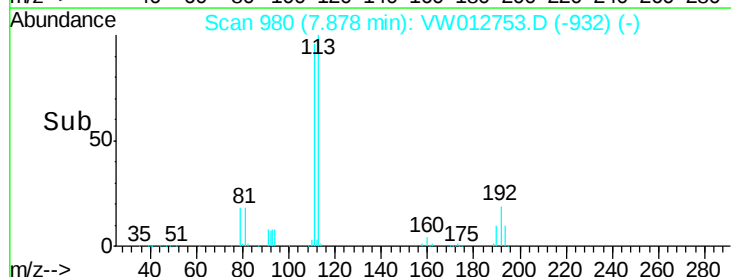

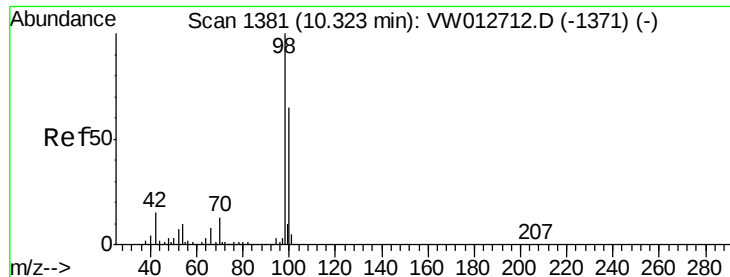

#50

Toluene-d8

Concen: 53.347 ug/l

RT: 10.32 min Scan# 1381

Delta R.T. 0.00 min

Lab File: VW012753.D

Acq: 08 Sep 2019 07:33

Instrument :

MSVOA_W

ClientSampleId :





SB-22-6.5-7.0

Tot Ion: 98 Resp: 410567

Ion Ratio Lower Upper

98 100

100 64.8 52.2 78.4

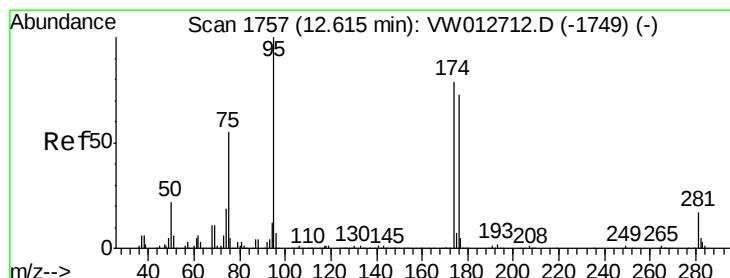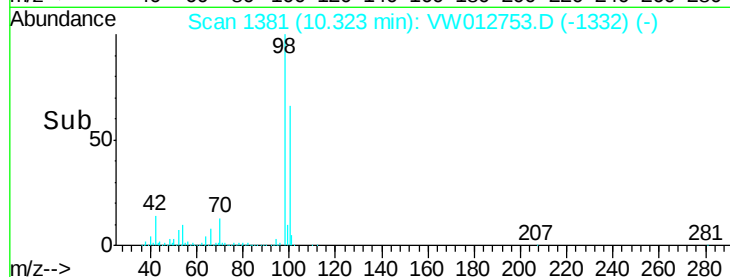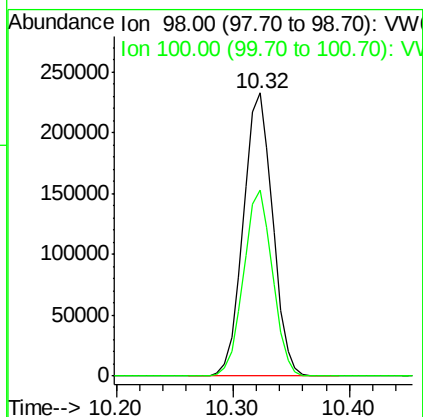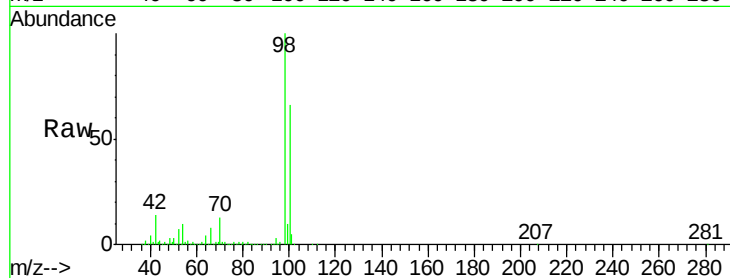

#62

4-Bromofluorobenzene

Concen: 36.280 ug/l

RT: 12.62 min Scan# 1757

Delta R.T. 0.00 min

Lab File: VW012753.D

Acq: 08 Sep 2019 07:33




Tgt Ion: 95 Resp: 101364


Ion Ratio Lower Upper

95 100

174 80.9 0.0 161.0

176 77.6 0.0 156.4

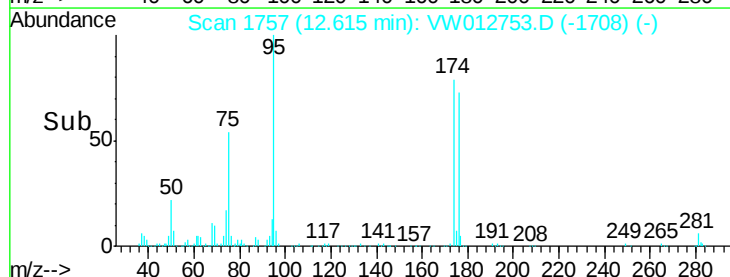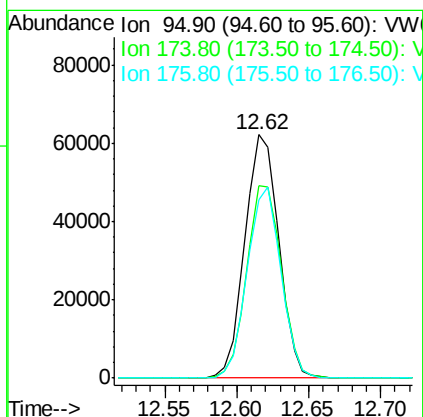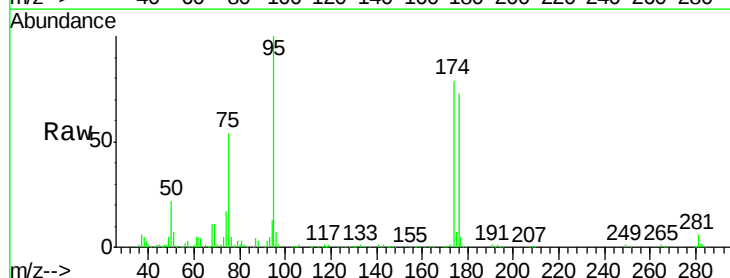

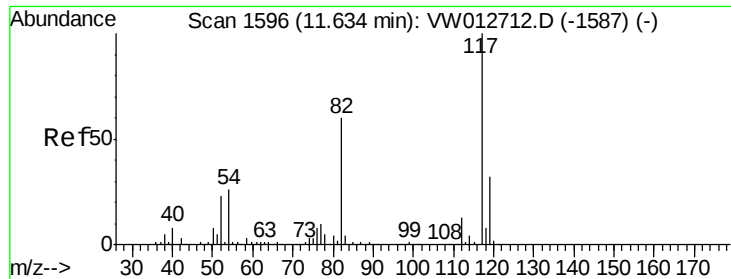

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.63 min Scan# 1595

Delta R.T. -0.01 min

Lab File: VW012753.D

Acq: 08 Sep 2019 07:33

Instrument :

MSVOA_W

ClientSampleId :

SB-22-6.5-7.0


Tot Ion:117 Resp: 265679

Ion Ratio Lower Upper

117 100

82 59.5 48.2 72.4




119 30.5 25.8 38.6

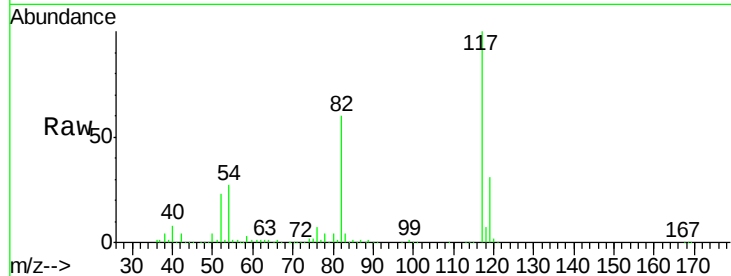

Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): V

Ion 118.90 (118.60 to 119.60): V

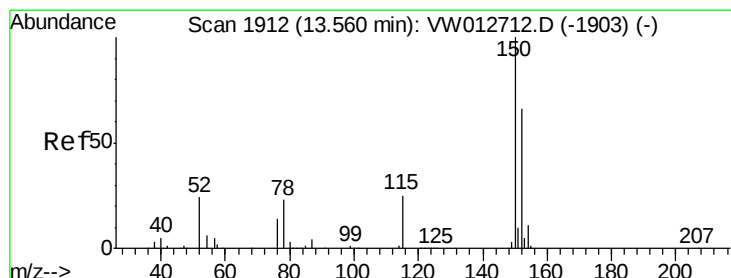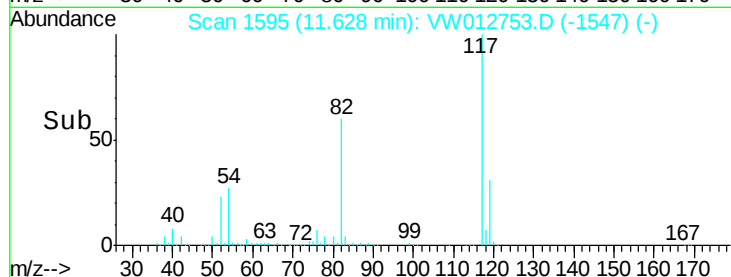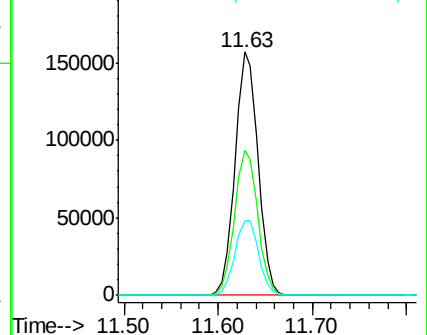

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.56 min Scan# 1912

Delta R.T. 0.00 min

Lab File: VW012753.D

Acq: 08 Sep 2019 07:33


Tgt Ion:152 Resp: 71432

Ion Ratio Lower Upper

152 100

115 58.2 30.0 90.1

150 154.6 0.0 349.0

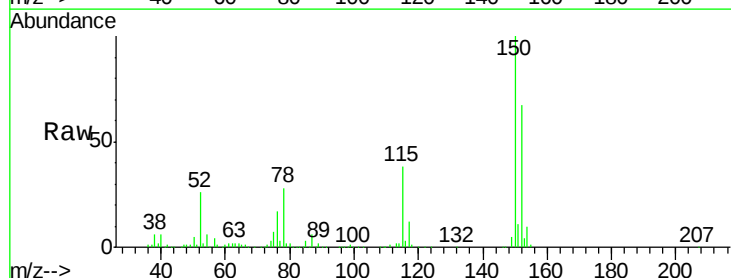

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

