

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090723\
 Data File : VW027007.D
 Acq On : 07 Sep 2023 16:13
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Sep 08 01:35:59 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 08 01:32:52 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	727461	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	719067	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	395072	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	206893	15.919	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	63.680%
7) Chloroethane-d5	2.893	69	181087	17.264	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	69.040%
11) 1,1-Dichloroethene-d2	4.027	65	82996	17.328	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	69.320%
21) 2-Butanone-d5	7.081	46	106418	42.496	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.000%
24) Chloroform-d	7.648	84	401238	18.536	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	74.160%
26) 1,2-Dichloroethane-d4	8.471	65	229	0.020	ug/L	0.16
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.080%#
32) Benzene-d6	8.276	84	857627	18.184	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	72.720%
36) 1,2-Dichloropropane-d6	9.276	67	254455	18.377	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	73.520%
41) Toluene-d8	10.325	98	772271	18.085	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	72.360%
43) trans-1,3-Dichloroprop...	10.575	79	99105	18.444	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	73.760%
47) 2-Hexanone-d5	10.928	63	60546	46.837	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.680%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	224236	20.868	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	83.480%
66) 1,2-Dichlorobenzene-d4	13.854	152	266659	19.515	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	78.080%
Target Compounds						
13) Acetone	4.143	43	8011	3.654	ug/L	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090723\
Data File : VW027007.D
Acq On : 07 Sep 2023 16:13
Operator : SY/MD
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Sep 08 01:35:59 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 08 01:32:52 2023
Response via : Initial Calibration

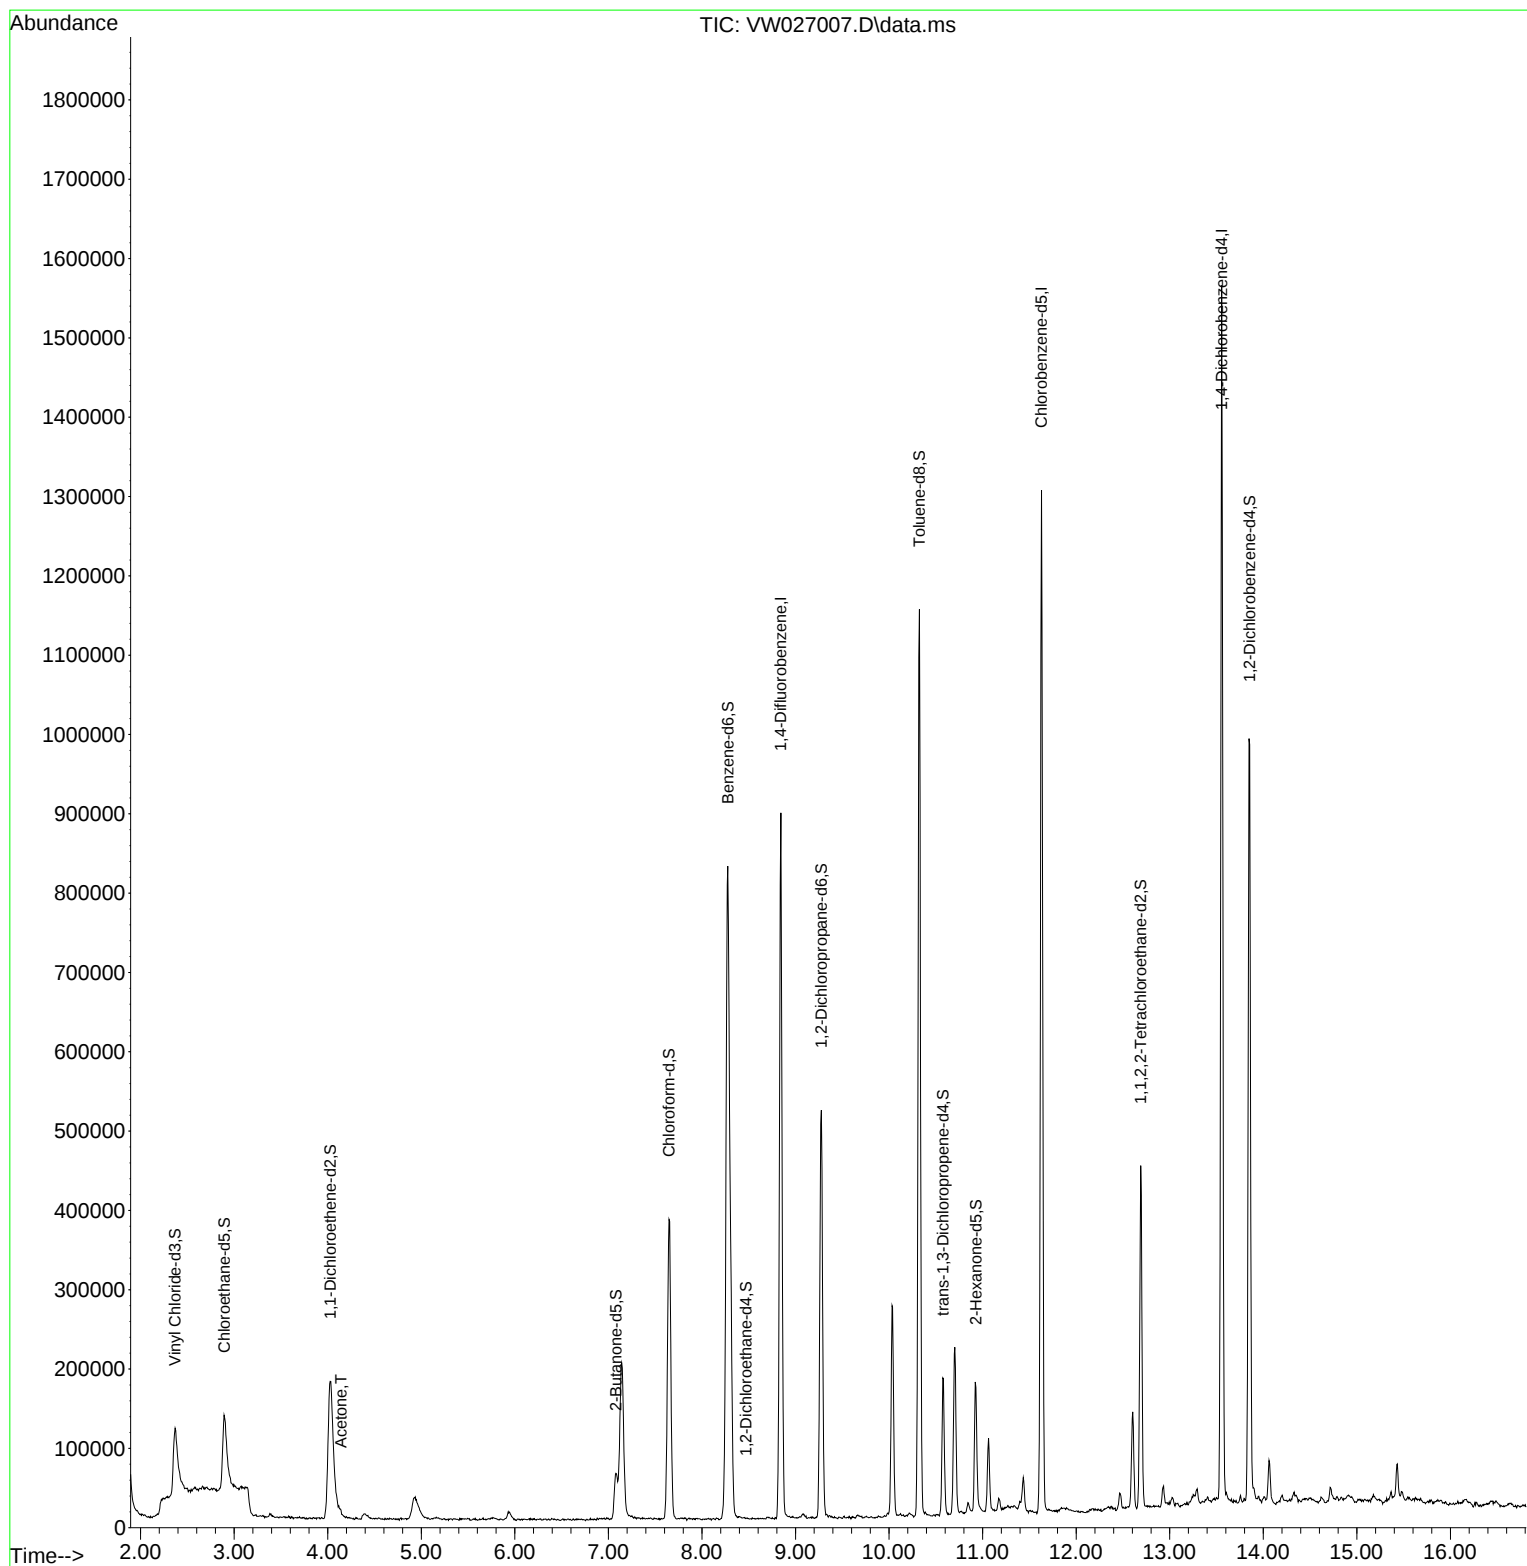

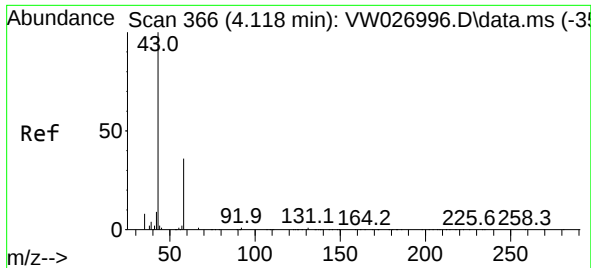

#13

Acetone

Concen: 3.654 ug/L

RT: 4.143 min Scan# 31

Delta R.T. 0.024 min


Lab File: VW027007.D

Acq: 07 Sep 2023 16:13

Instrument :

MSVOA_W

ClientSampleId :

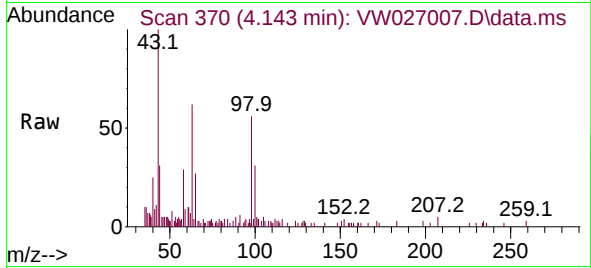

Tgt Ion: 43 Resp: 8011

Ion Ratio Lower Upper

43 100

58 36.8 0.0 66.4

