




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090723\
 Data File : VW026998.D
 Acq On : 07 Sep 2023 12:36
 Operator : SY/MD
 Sample : 04330-01
 Misc : 6.03g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EYZG2

Manual IntegrationsAPPROVED

Quant Time: Sep 08 01:33:30 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 08 01:32:52 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/08/2023
 Supervised By :Mahesh Dadoda 09/08/2023

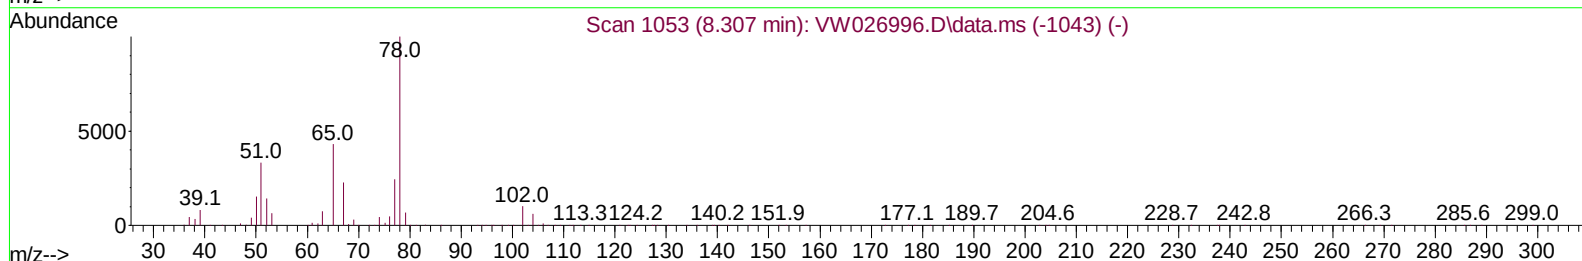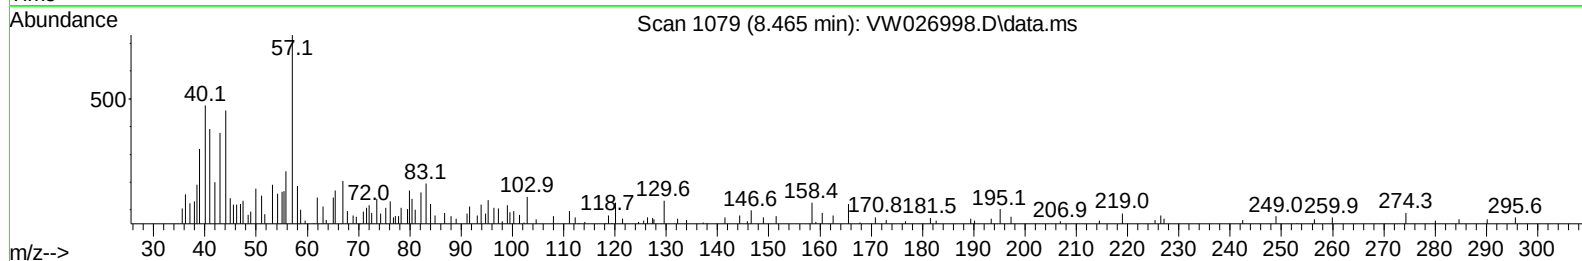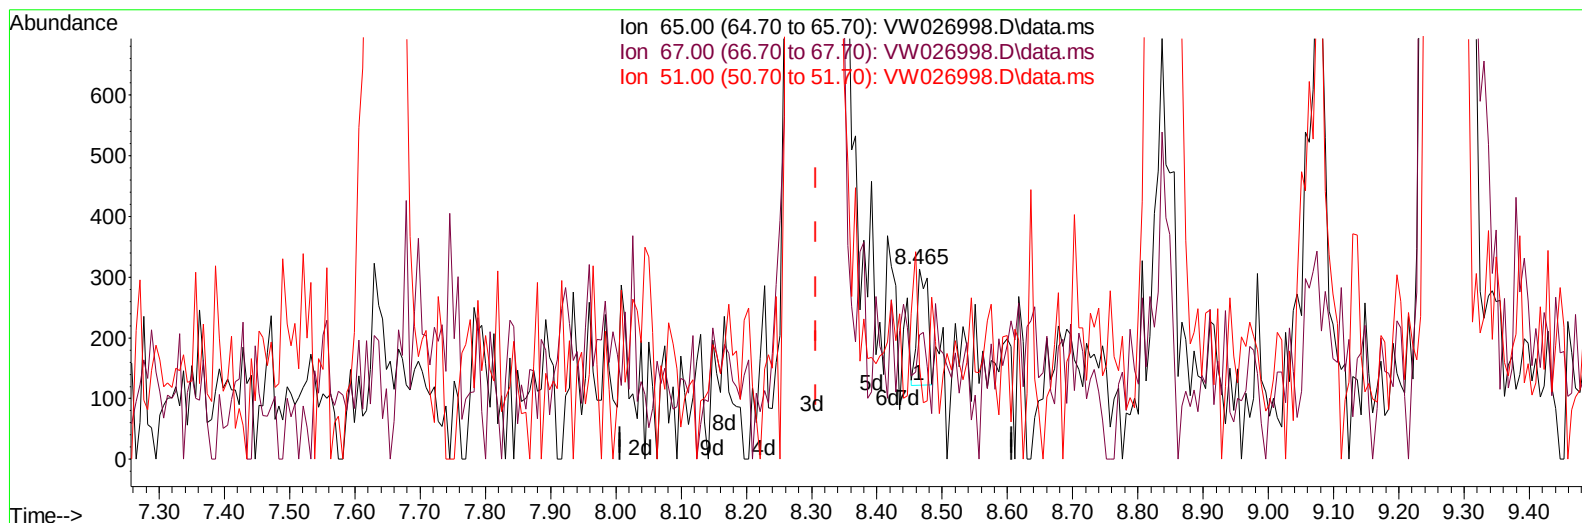

TIC: VW026998.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.465min (+ 0.158) 0.02 ug/L

response 215

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	54.50	69.77
51.00	110.30	79.53
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090723\
 Data File : VW026998.D
 Acq On : 07 Sep 2023 12:36
 Operator : SY/MD
 Sample : 04330-01
 Misc : 6.03g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZYG2

Manual IntegrationsAPPROVED

Quant Time: Sep 08 01:33:30 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 08 01:32:52 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/08/2023
 Supervised By :Mahesh Dadoda 09/08/2023

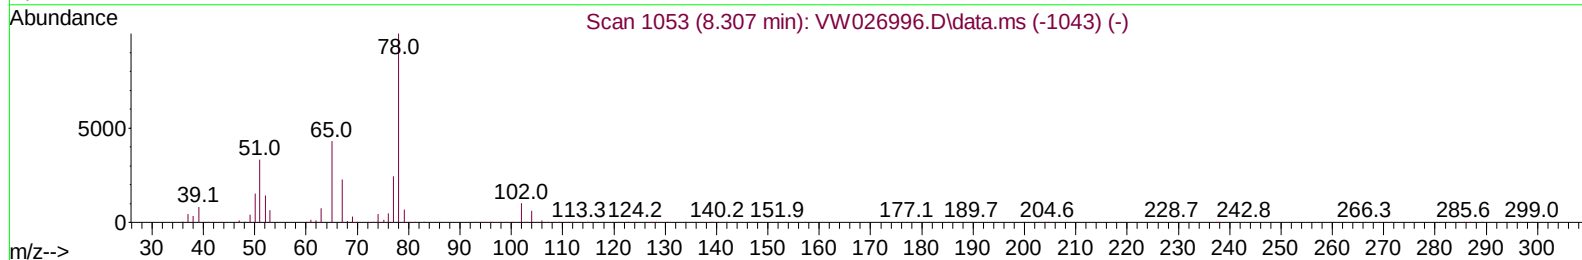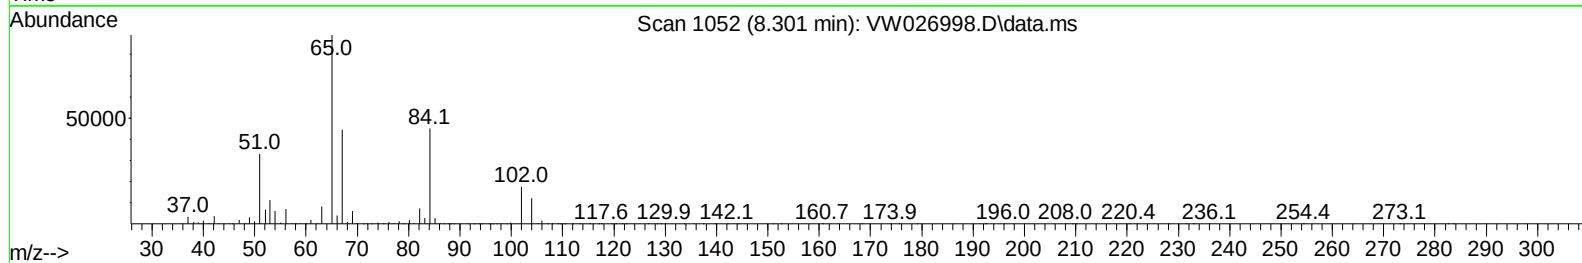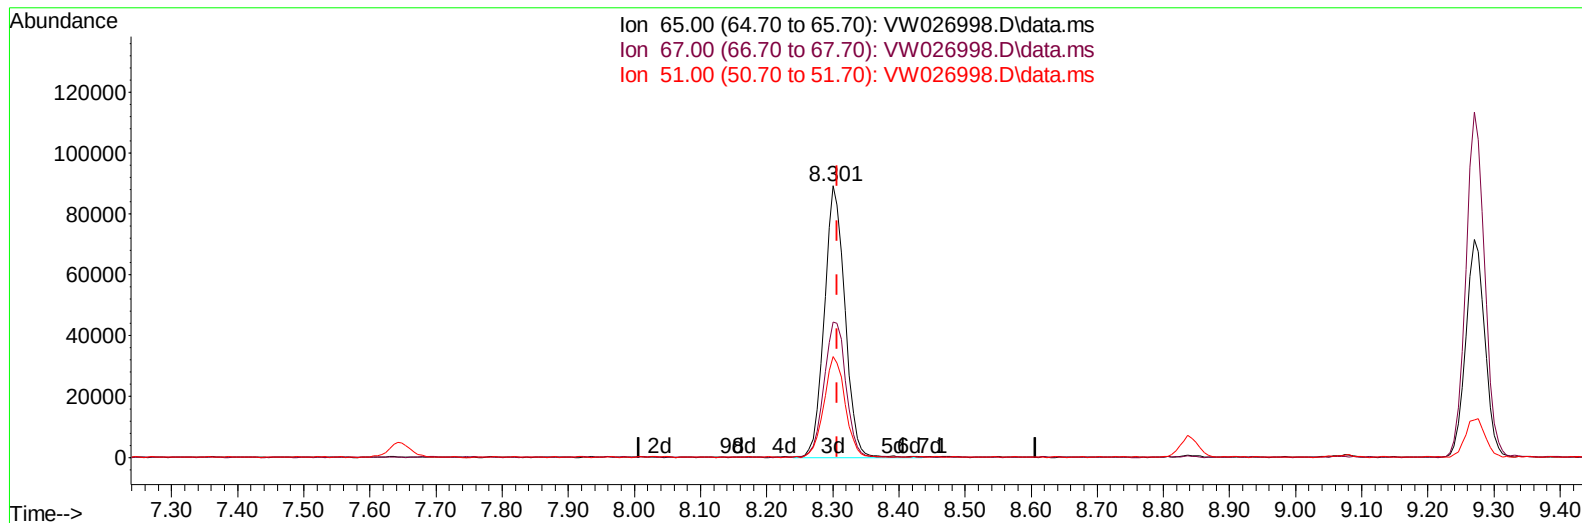

TIC: VW026998.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.301min (-0.006) 18.61 ug/L m

response 193548

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	54.50	0.08#
51.00	110.30	0.09#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090723\
 Data File : VW026998.D
 Acq On : 07 Sep 2023 12:36
 Operator : SY/MD
 Sample : 04330-01
 Misc : 6.03g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZYG2

Manual IntegrationsAPPROVED

Quant Time: Sep 08 01:33:30 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 08 01:32:52 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/08/2023
 Supervised By :Mahesh Dadoda 09/08/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		664978	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		501535	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		138844	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.369	65		161130	13.563	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	54.240%		
7) Chloroethane-d5	2.893	69		153539	16.013	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	64.040%		
11) 1,1-Dichloroethene-d2	4.015	65		60492	13.816	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110		Recovery =	55.280%		
21) 2-Butanone-d5	7.069	46		94075	41.097	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	82.200%		
24) Chloroform-d	7.642	84		294418	14.879	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	59.520%		
26) 1,2-Dichloroethane-d4	8.301	65		193548m	18.609	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	74.440%		
32) Benzene-d6	8.270	84		661763	20.116	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	80.480%		
36) 1,2-Dichloropropane-d6	9.270	67		222831	23.073	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	92.280%		
41) Toluene-d8	10.319	98		486014	16.318	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	65.280%		
43) trans-1,3-Dichloroprop...	10.575	79		70588	18.834	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	75.320%		
47) 2-Hexanone-d5	10.922	63		45871	50.876	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	101.760%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		98564	13.151	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	52.600%		
66) 1,2-Dichlorobenzene-d4	13.848	152		85703	17.847	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	71.400%#		
Target Compounds							
						Qvalue	
13) Acetone	4.125	43		51523	25.706	ug/L	98
14) Carbon disulfide	4.387	76		37352	1.240	ug/L #	93
22) 2-Butanone	7.173	43		23542	7.300	ug/L	92
25) Chloroform	7.673	83		60642	3.190	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090723\
Data File : VW026998.D
Acq On : 07 Sep 2023 12:36
Operator : SY/MD
Sample : 04330-01
Misc : 6.03g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EZYG2

Manual IntegrationsAPPROVED

Quant Time: Sep 08 01:33:30 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 08 01:32:52 2023
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/08/2023
Supervised By :Mahesh Dadoda 09/08/2023

