




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090723\
 Data File : VW027002.D
 Acq On : 07 Sep 2023 14:13
 Operator : SY/MD
 Sample : 04330-07
 Misc : 5.26g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZYX8

Manual IntegrationsAPPROVED

Quant Time: Sep 08 01:34:35 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 08 01:32:52 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/08/2023
 Supervised By :Mahesh Dadoda 09/08/2023

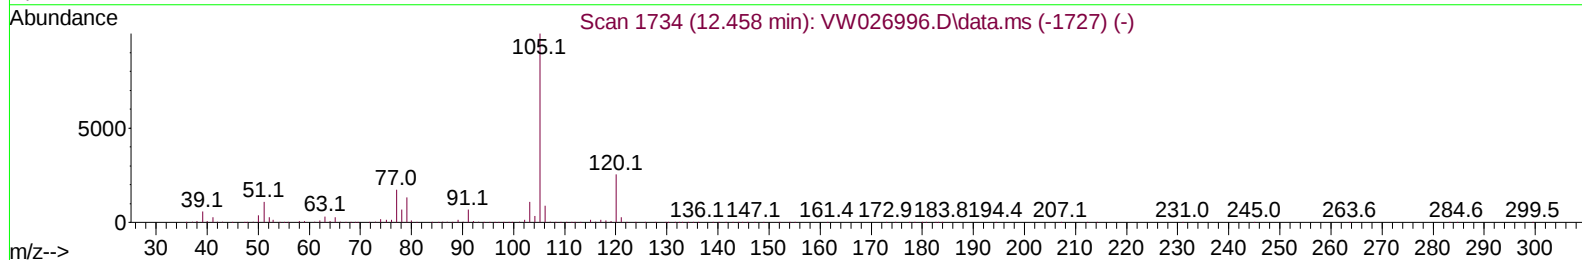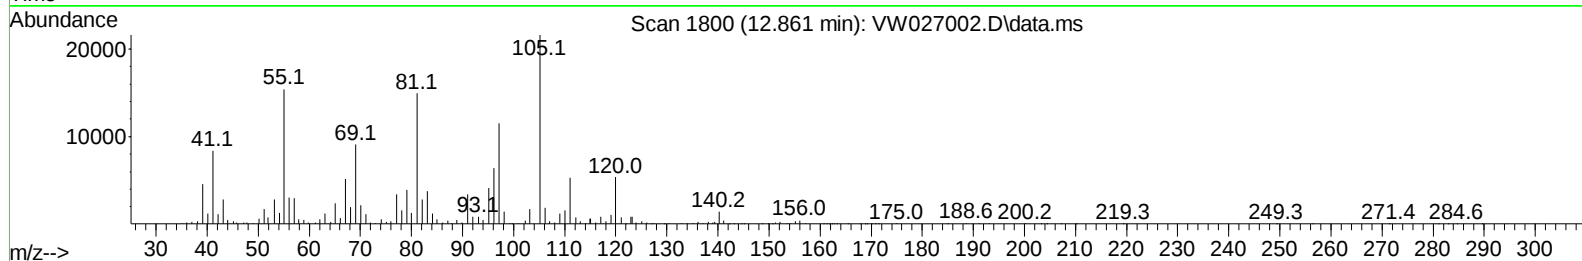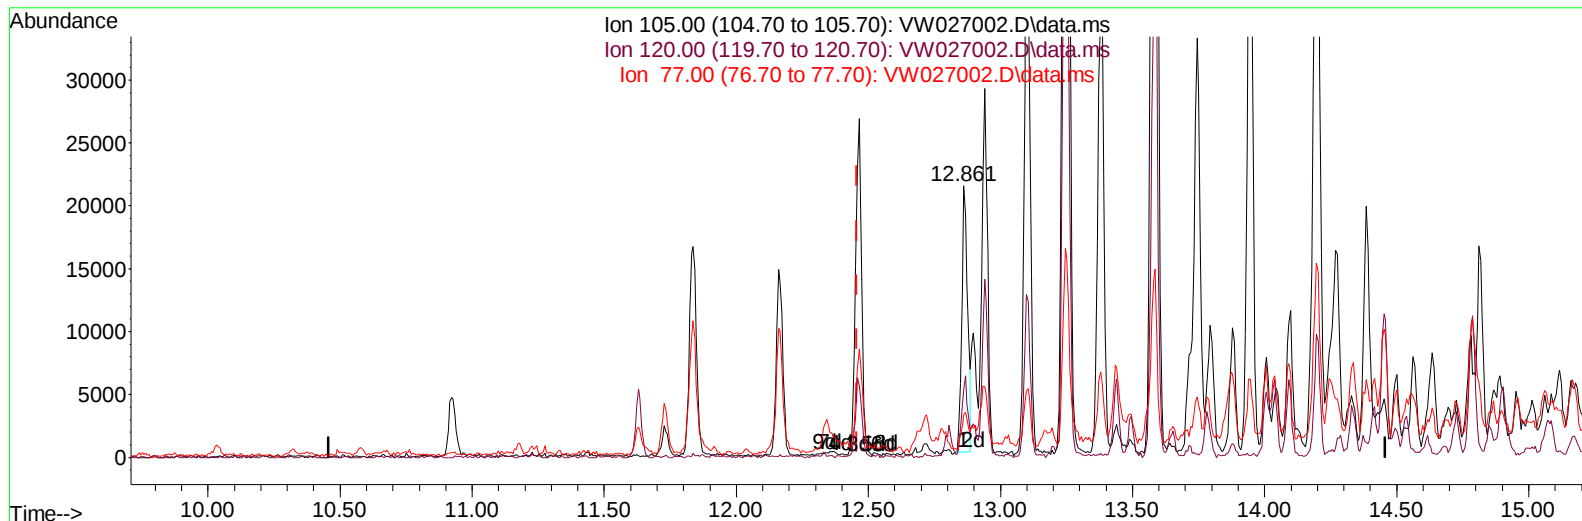

TIC: VW027002.D\data.ms

(60) Isopropylbenzene

12.861min (+ 0.402) 2.46 ug/L

response 32460

Ion	Exp%	Act%
105.00	100.00	100.00
120.00	26.70	30.09
77.00	16.00	16.47
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090723\
Data File : VW027002.D
Acq On : 07 Sep 2023 14:13
Operator : SY/MD
Sample : 04330-07
Misc : 5.26g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EZYX8

Manual IntegrationsAPPROVED

Quant Time: Sep 08 01:34:35 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 08 01:32:52 2023
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/08/2023
Supervised By :Mahesh Dadoda 09/08/2023

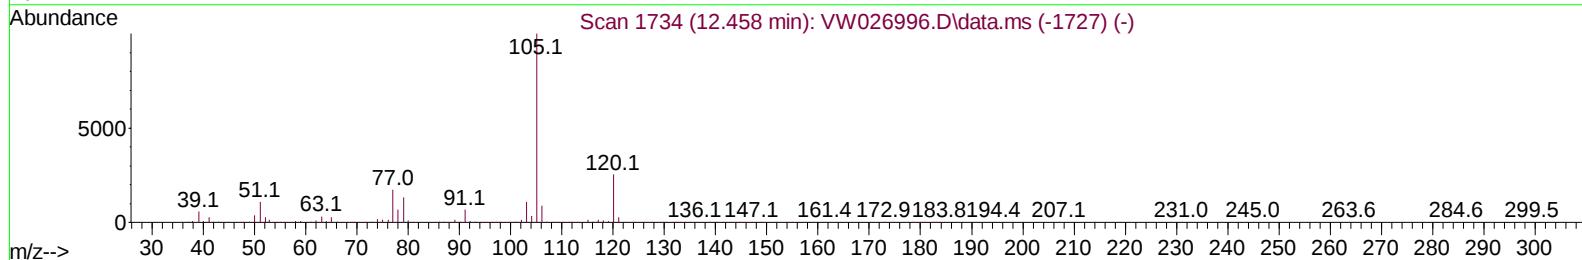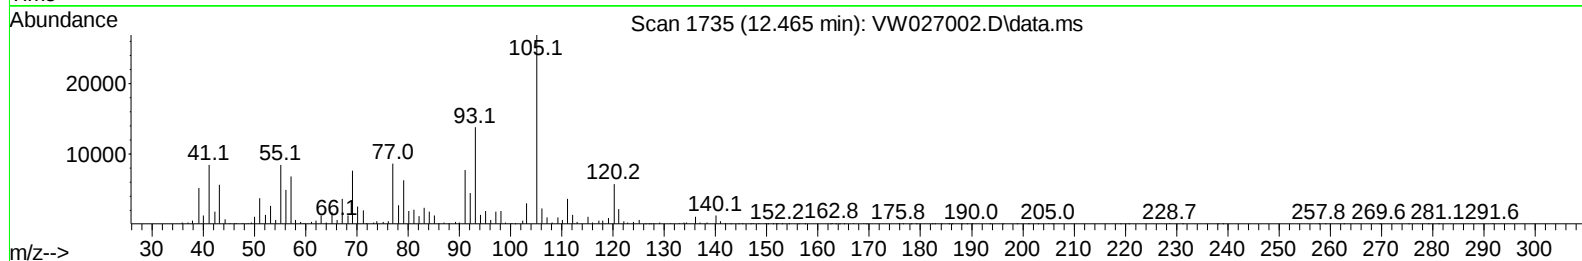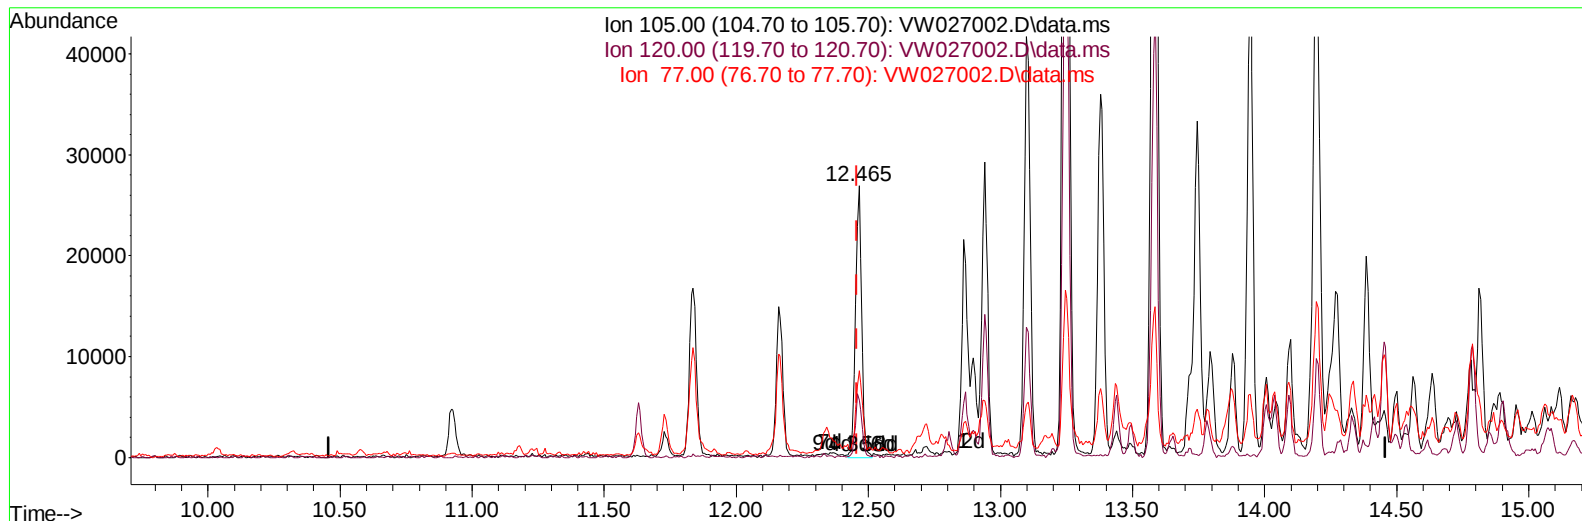

TIC: VW027002.D\data.ms

(60) Isopropylbenzene

12.465min (+ 0.006) 3.18 ug/L m

response 41881

Ion	Exp%	Act%
105.00	100.00	100.00
120.00	26.70	23.32
77.00	16.00	12.76#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090723\
 Data File : VW027002.D
 Acq On : 07 Sep 2023 14:13
 Operator : SY/MD
 Sample : 04330-07
 Misc : 5.26g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZYX8

Manual IntegrationsAPPROVED

Quant Time: Sep 08 01:34:35 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 08 01:32:52 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/08/2023
 Supervised By :Mahesh Dadoda 09/08/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	551724	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	392456	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	96240	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	131623	13.353	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	53.400%	
7) Chloroethane-d5	2.887	69	132751	16.687	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	66.760%	
11) 1,1-Dichloroethene-d2	4.027	65	49862	13.726	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	54.920%	
21) 2-Butanone-d5	7.081	46	102842	54.149	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	108.300%	
24) Chloroform-d	7.648	84	302590	18.431	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	73.720%	
26) 1,2-Dichloroethane-d4	8.307	65	159204	18.449	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	73.800%	
32) Benzene-d6	8.276	84	569610	22.128	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	88.520%	
36) 1,2-Dichloropropane-d6	9.276	67	200849	26.577	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	106.320%	
41) Toluene-d8	10.325	98	405364	17.393	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	69.560%	
43) trans-1,3-Dichloroprop...	10.581	79	39376	13.426	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	53.720%	
47) 2-Hexanone-d5	10.922	63	46677	66.158	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	132.320%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	172585	29.428	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	117.720%	
66) 1,2-Dichlorobenzene-d4	13.855	152	73403	22.052	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	88.200%	
Target Compounds					Qvalue	
13) Acetone	4.125	43	50020	30.078	ug/L	95
14) Carbon disulfide	4.381	76	136711	5.468	ug/L	96
20) cis-1,2-Dichloroethene	7.173	96	35438	3.774	ug/L	89
22) 2-Butanone	7.173	43	13616	5.089	ug/L	82
33) Benzene	8.325	78	23897	0.890	ug/L	100
34) Trichloroethene	9.093	95	14529	2.107	ug/L	90
35) Methylcyclohexane	9.331	83	17020	1.453	ug/L #	81
42) Toluene	10.386	91	29707	1.076	ug/L	96
52) Ethylbenzene	11.727	91	67735	2.212	ug/L	99
53) m,p-Xylene	11.837	106	65172	5.627	ug/L	91
54) o-Xylene	12.166	106	60128	5.548	ug/L	95
60) Isopropylbenzene	12.465	105	41881m	3.177	ug/L	
62) 1,3,5-Trimethylbenzene	12.940	105	42535	4.043	ug/L	100
63) 1,2,4-Trimethylbenzene	13.245	105	193278	18.792	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090723\
Data File : VW027002.D
Acq On : 07 Sep 2023 14:13
Operator : SY/MD
Sample : 04330-07
Misc : 5.26g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EZYX8

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/08/2023
Supervised By :Mahesh Dadoda 09/08/2023

Quant Time: Sep 08 01:34:35 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 08 01:32:52 2023
Response via : Initial Calibration

