




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090723\
 Data File : VW027009.D
 Acq On : 07 Sep 2023 17:02
 Operator : SY/MD
 Sample : 04332-03
 Misc : 3.14g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AC1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/08/2023
 Supervised By :Mahesh Dadoda 09/08/2023

Quant Time: Sep 08 01:36:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 08 01:32:52 2023
 Response via : Initial Calibration

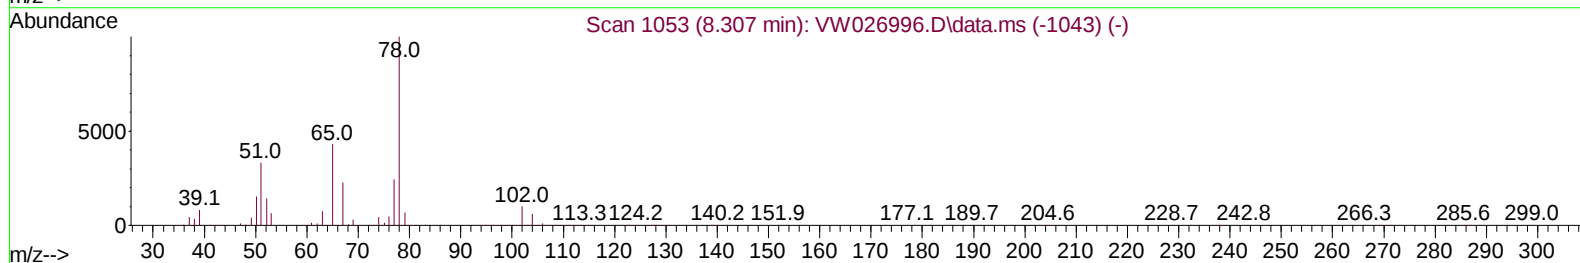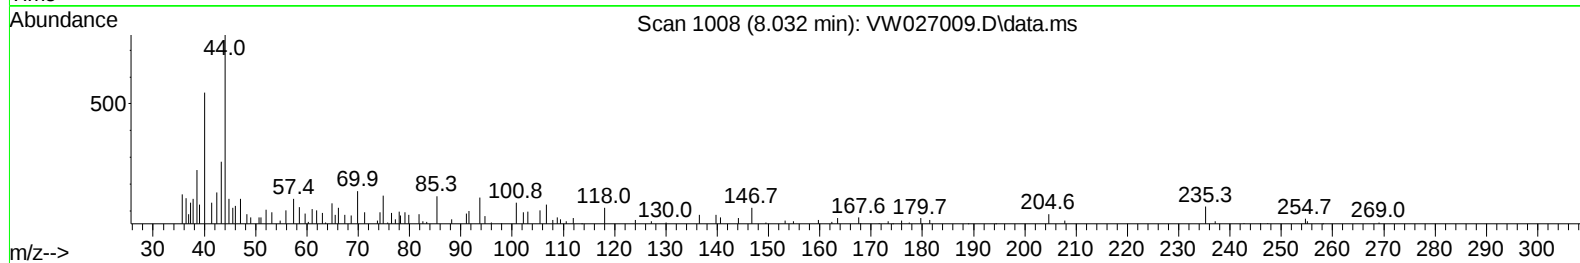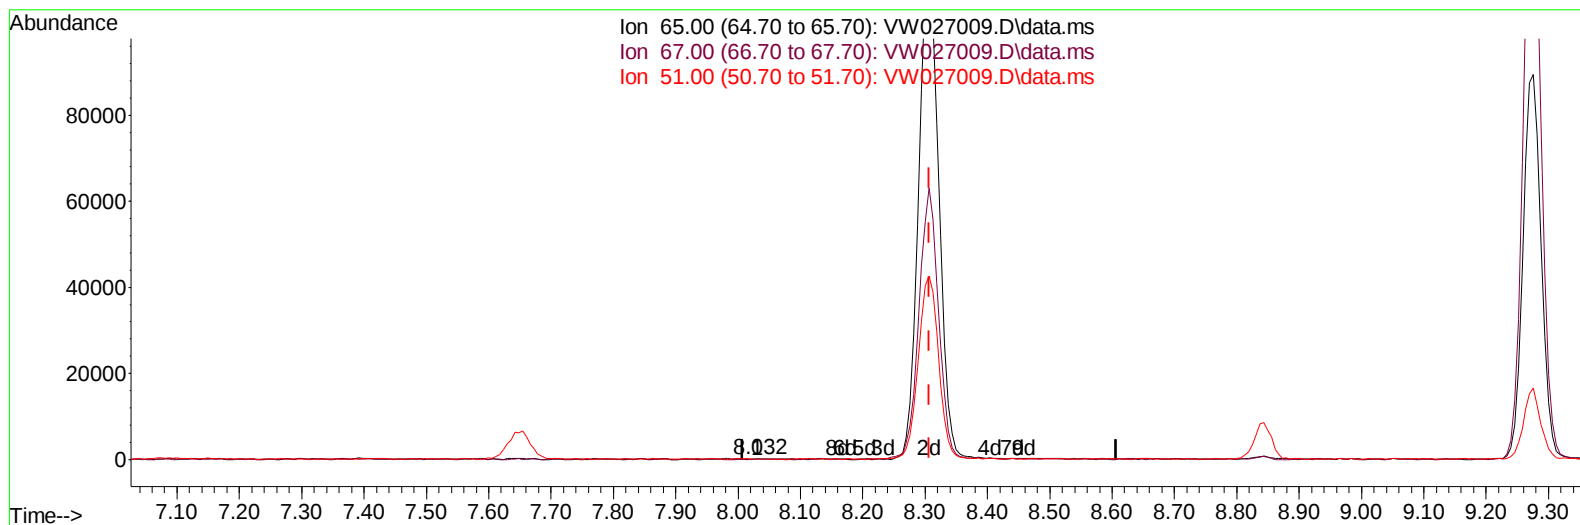

TIC: VW027009.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.032min (-0.275) 0.01 ug/L

response 133

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	54.50	66.92
51.00	110.30	108.27
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090723\
 Data File : VW027009.D
 Acq On : 07 Sep 2023 17:02
 Operator : SY/MD
 Sample : 04332-03
 Misc : 3.14g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AC1

Manual IntegrationsAPPROVED

Quant Time: Sep 08 01:36:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 08 01:32:52 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/08/2023
 Supervised By :Mahesh Dadoda 09/08/2023

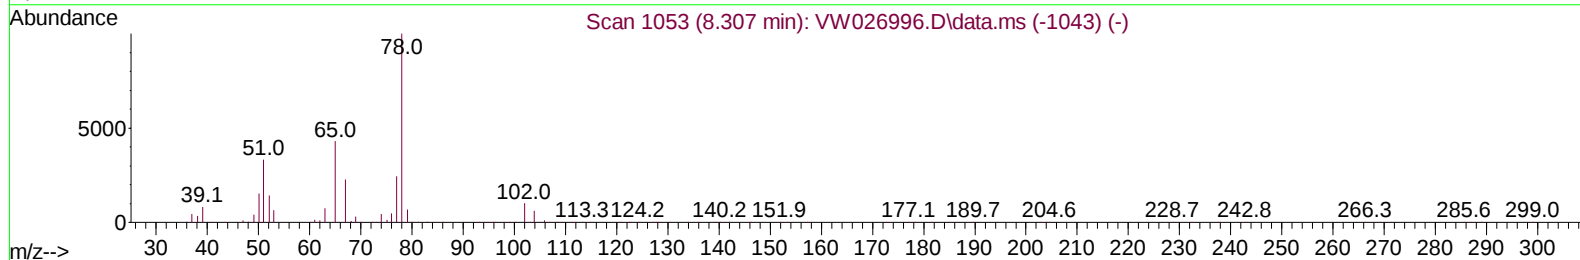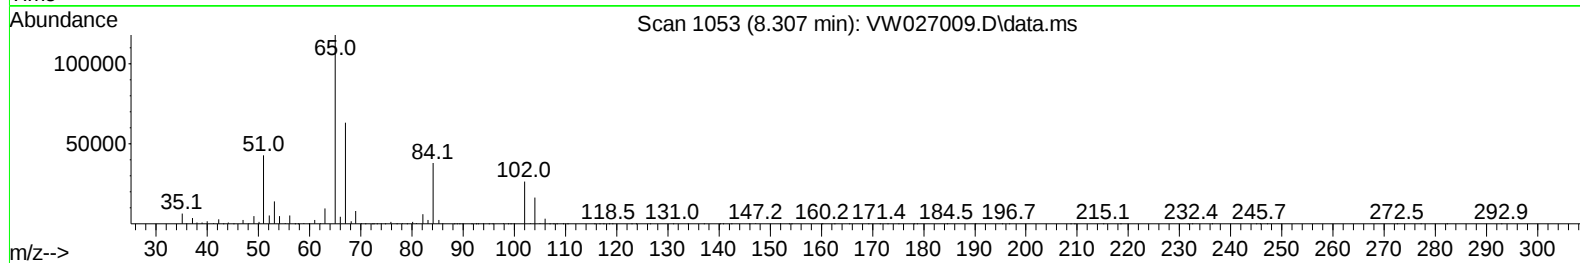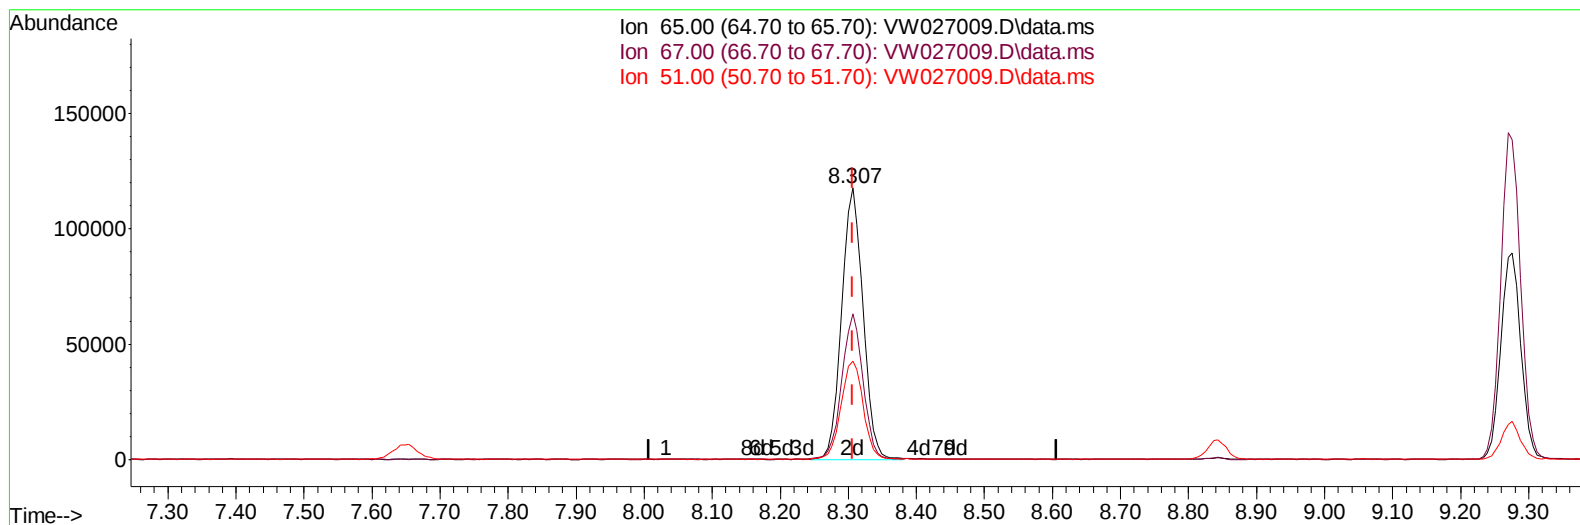

TIC: VW027009.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (-0.000) 18.81 ug/L m

response 255672

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	54.50	0.03#
51.00	110.30	0.06#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090723\
 Data File : VW027009.D
 Acq On : 07 Sep 2023 17:02
 Operator : SY/MD
 Sample : 04332-03
 Misc : 3.14g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AC1

Manual IntegrationsAPPROVED

Quant Time: Sep 08 01:36:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 08 01:32:52 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/08/2023
 Supervised By :Mahesh Dadoda 09/08/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.849	114		869123	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		650917	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		198660	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.369	65		205635	13.243	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	52.960%		
7) Chloroethane-d5	2.893	69		202695	16.174	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	64.680%		
11) 1,1-Dichloroethene-d2	4.027	65		71153	12.434	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	49.720%		
21) 2-Butanone-d5	7.081	46		114763	38.358	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	76.720%		
24) Chloroform-d	7.648	84		453661	17.541	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	70.160%		
26) 1,2-Dichloroethane-d4	8.307	65		255672m	18.808	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	75.240%		
32) Benzene-d6	8.276	84		852024	19.956	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	79.840%		
36) 1,2-Dichloropropane-d6	9.270	67		287339	22.924	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	91.680%		
41) Toluene-d8	10.324	98		652904	16.891	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	67.560%		
43) trans-1,3-Dichloroprop...	10.574	79		61510	12.646	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	50.600%		
47) 2-Hexanone-d5	10.922	63		29170	24.928	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	49.860%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		224920	23.123	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	92.480%		
66) 1,2-Dichlorobenzene-d4	13.848	152		119788	17.434	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	69.720%#		
Target Compounds							
						Qvalue	
13) Acetone	4.124	43		30115	11.496	ug/L	97
16) Methylene chloride	4.935	84		34059	2.023	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090723\
Data File : VW027009.D
Acq On : 07 Sep 2023 17:02
Operator : SY/MD
Sample : 04332-03
Misc : 3.14g/10mL/MSVOA_W/SoIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AC1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/08/2023
Supervised By :Mahesh Dadoda 09/08/2023

Quant Time: Sep 08 01:36:24 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 08 01:32:52 2023
Response via : Initial Calibration

