

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090723\
 Data File : VW027014.D
 Acq On : 07 Sep 2023 19:04
 Operator : SY/MD
 Sample : 04332-10
 Misc : 3.96g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 COAH2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/08/2023
 Supervised By :Mahesh Dadoda 09/08/2023

09/08/2023
 Supervised By :Mahesh
 Dadoda

Quant Time: Sep 08 01:37:26 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 08 01:32:52 2023
 Response via : Initial Calibration

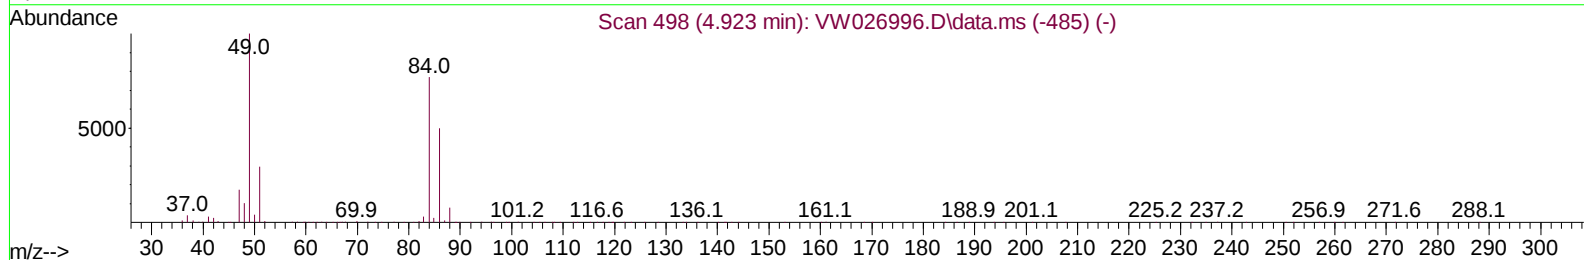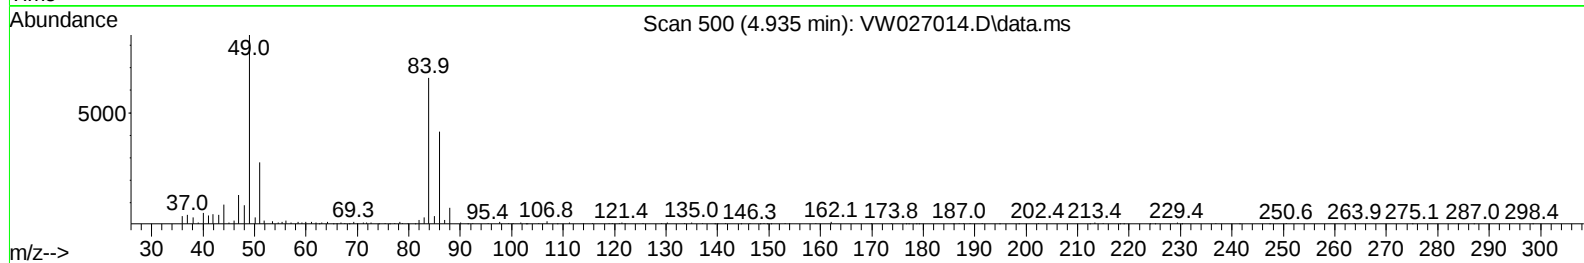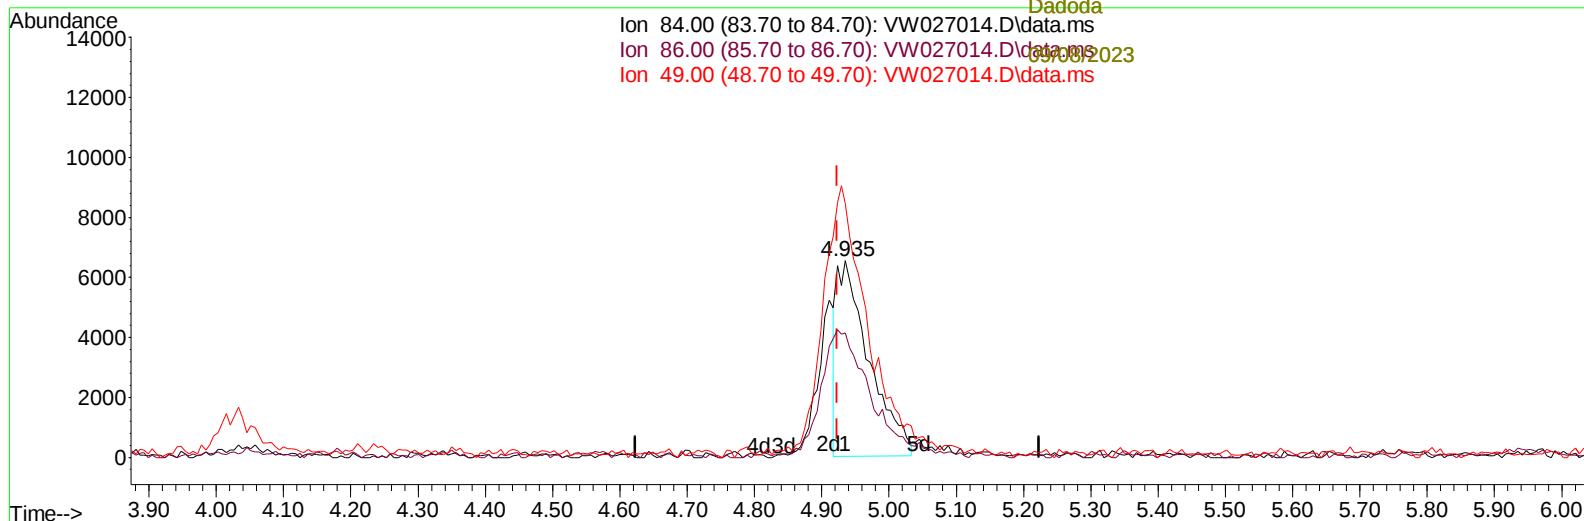

TIC: VW027014.D\data.ms

(16) Methylene chloride (T)

4.935min (+ 0.012) 1.56 ug/L

response 21681

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.00	63.32
49.00	117.30	129.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090723\
 Data File : VW027014.D
 Acq On : 07 Sep 2023 19:04
 Operator : SY/MD
 Sample : 04332-10
 Misc : 3.96g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 COAH2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/08/2023
 Supervised By :Mahesh Dadoda 09/08/2023

Quant Time: Sep 08 01:37:26 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 08 01:32:52 2023
 Response via : Initial Calibration

09/08/2023
 Supervised By :Mahesh
 Dadoda

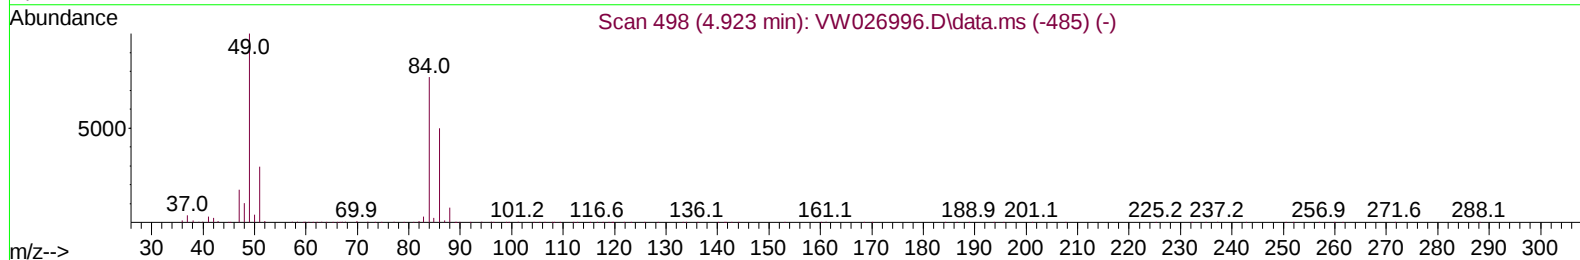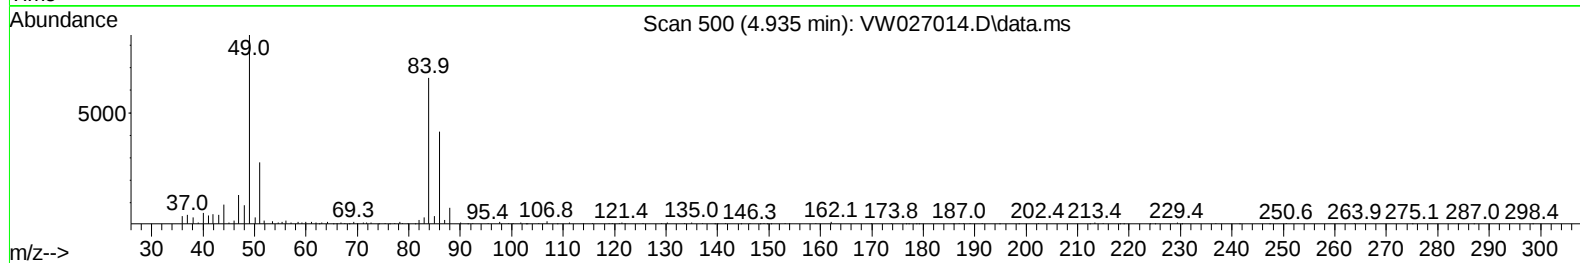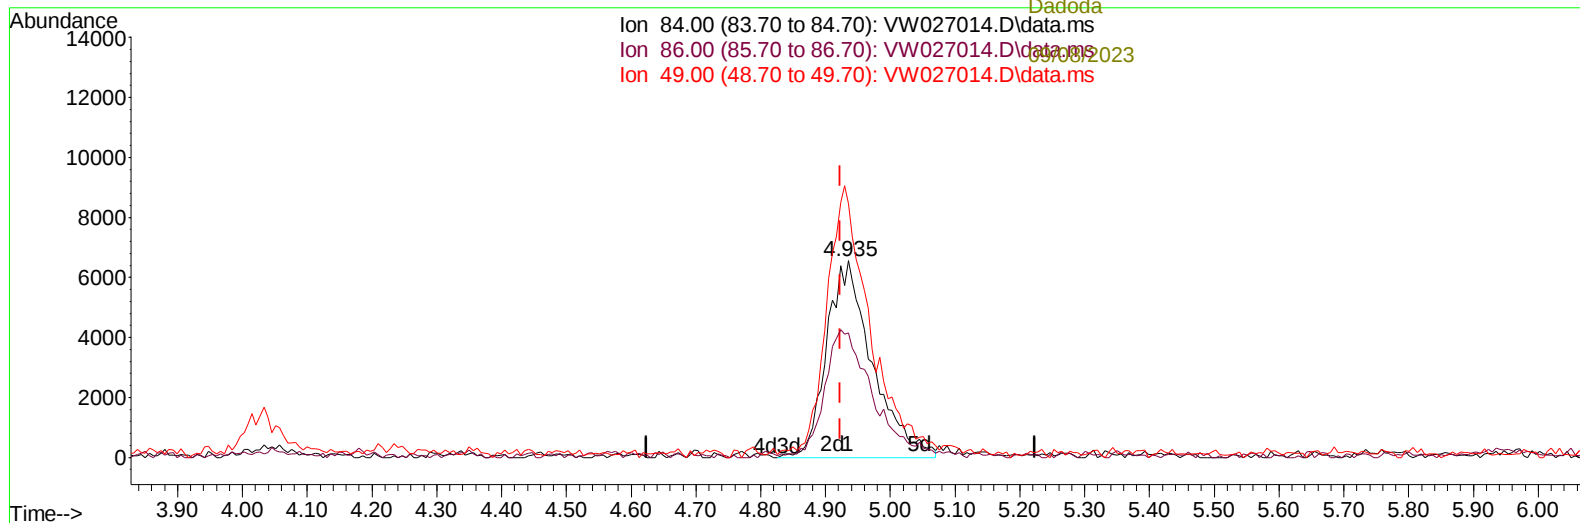

TIC: VW027014.D\data.ms

(16) Methylene chloride (T)

4.935min (+ 0.012) 2.31 ug/L m

response 32043

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.00	63.32
49.00	117.30	129.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090723\
 Data File : VW027014.D
 Acq On : 07 Sep 2023 19:04
 Operator : SY/MD
 Sample : 04332-10
 Misc : 3.96g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AH2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/08/2023
 Supervised By :Mahesh Dadoda 09/08/2023

Quant Time: Sep 08 01:37:26 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 08 01:32:52 2023
 Response via : Initial Calibration

09/08/2023
 Supervised By :Mahesh
 Dadoda

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----09/08/2023						
Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	715370	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	525919	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	146719	25.000	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.363	65	181225	14.180	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	56.720%	
7) Chloroethane-d5	2.893	69	183507	17.791	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	71.160%	
11) 1,1-Dichloroethene-d2	4.027	65	67069	14.239	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	56.960%	
21) 2-Butanone-d5	7.087	46	67869	27.560	ug/L	0.01
Spiked Amount 50.000	Range 20	- 135	Recovery	=	55.120%	
24) Chloroform-d	7.648	84	400993	18.837	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	75.360%	
26) 1,2-Dichloroethane-d4	8.307	65	226222	20.219	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	80.880%	
32) Benzene-d6	8.276	84	730722	21.183	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	84.720%	
36) 1,2-Dichloropropane-d6	9.276	67	261491	25.821	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	103.280%	
41) Toluene-d8	10.325	98	515181	16.495	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	66.000%	
43) trans-1,3-Dichloroprop...	10.574	79	44354	11.286	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	45.160%	
47) 2-Hexanone-d5	10.928	63	21393	22.627	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	45.260%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	197365	25.113	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	100.440%	
66) 1,2-Dichlorobenzene-d4	13.854	152	93404	18.407	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	73.640%#	

Target Compounds

						Qvalue
13) Acetone	4.124	43	10218	4.739	ug/L	94
16) Methylene chloride	4.935	84	32043m	2.312	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090723\
Data File : VW027014.D
Acq On : 07 Sep 2023 19:04
Operator : SY/MD
Sample : 04332-10
Misc : 3.96g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AH2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/08/2023
Supervised By :Mahesh Dadoda 09/08/2023

Quant Time: Sep 08 01:37:26 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 08 01:32:52 2023
Response via : Initial Calibration

09/08/2023
Supervised By :Mahesh
Dadoda

09/08/2023

