

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090723\
 Data File : VW027002.D
 Acq On : 07 Sep 2023 14:13
 Operator : SY/MD
 Sample : 04330-07
 Misc : 5.26g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZYX8

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 09/08/2023
 Supervised By :Mahesh Dadoda 09/08/2023

Quant Time: Sep 08 01:34:35 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 08 01:32:52 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	551724	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	392456	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	96240	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	131623	13.353	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	53.400%		
7) Chloroethane-d5	2.887	69	132751	16.687	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	66.760%		
11) 1,1-Dichloroethene-d2	4.027	65	49862	13.726	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	54.920%		
21) 2-Butanone-d5	7.081	46	102842	54.149	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	108.300%		
24) Chloroform-d	7.648	84	302590	18.431	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	73.720%		
26) 1,2-Dichloroethane-d4	8.307	65	159204	18.449	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	73.800%		
32) Benzene-d6	8.276	84	569610	22.128	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	88.520%		
36) 1,2-Dichloropropane-d6	9.276	67	200849	26.577	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	106.320%		
41) Toluene-d8	10.325	98	405364	17.393	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	69.560%		
43) trans-1,3-Dichloroprop...	10.581	79	39376	13.426	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	53.720%		
47) 2-Hexanone-d5	10.922	63	46677	66.158	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	132.320%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	172585	29.428	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	117.720%		
66) 1,2-Dichlorobenzene-d4	13.855	152	73403	22.052	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	88.200%		
Target Compounds						Qvalue
13) Acetone	4.125	43	50020	30.078	ug/L	95
14) Carbon disulfide	4.381	76	136711	5.468	ug/L	96
20) cis-1,2-Dichloroethene	7.173	96	35438	3.774	ug/L	89
22) 2-Butanone	7.173	43	13616	5.089	ug/L	82
33) Benzene	8.325	78	23897	0.890	ug/L	100
34) Trichloroethene	9.093	95	14529	2.107	ug/L	90
35) Methylcyclohexane	9.331	83	17020	1.453	ug/L #	81
42) Toluene	10.386	91	29707	1.076	ug/L	96
52) Ethylbenzene	11.727	91	67735	2.212	ug/L	99
53) m,p-Xylene	11.837	106	65172	5.627	ug/L	91
54) o-Xylene	12.166	106	60128	5.548	ug/L	95
60) Isopropylbenzene	12.465	105	41881m	3.177	ug/L	
62) 1,3,5-Trimethylbenzene	12.940	105	42535	4.043	ug/L	100
63) 1,2,4-Trimethylbenzene	13.245	105	193278	18.792	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090723\
Data File : VW027002.D
Acq On : 07 Sep 2023 14:13
Operator : SY/MD
Sample : 04330-07
Misc : 5.26g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EZYX8

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 09/08/2023
Supervised By : Mahesh Dadoda 09/08/2023

Quant Time: Sep 08 01:34:35 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 08 01:32:52 2023
Response via : Initial Calibration

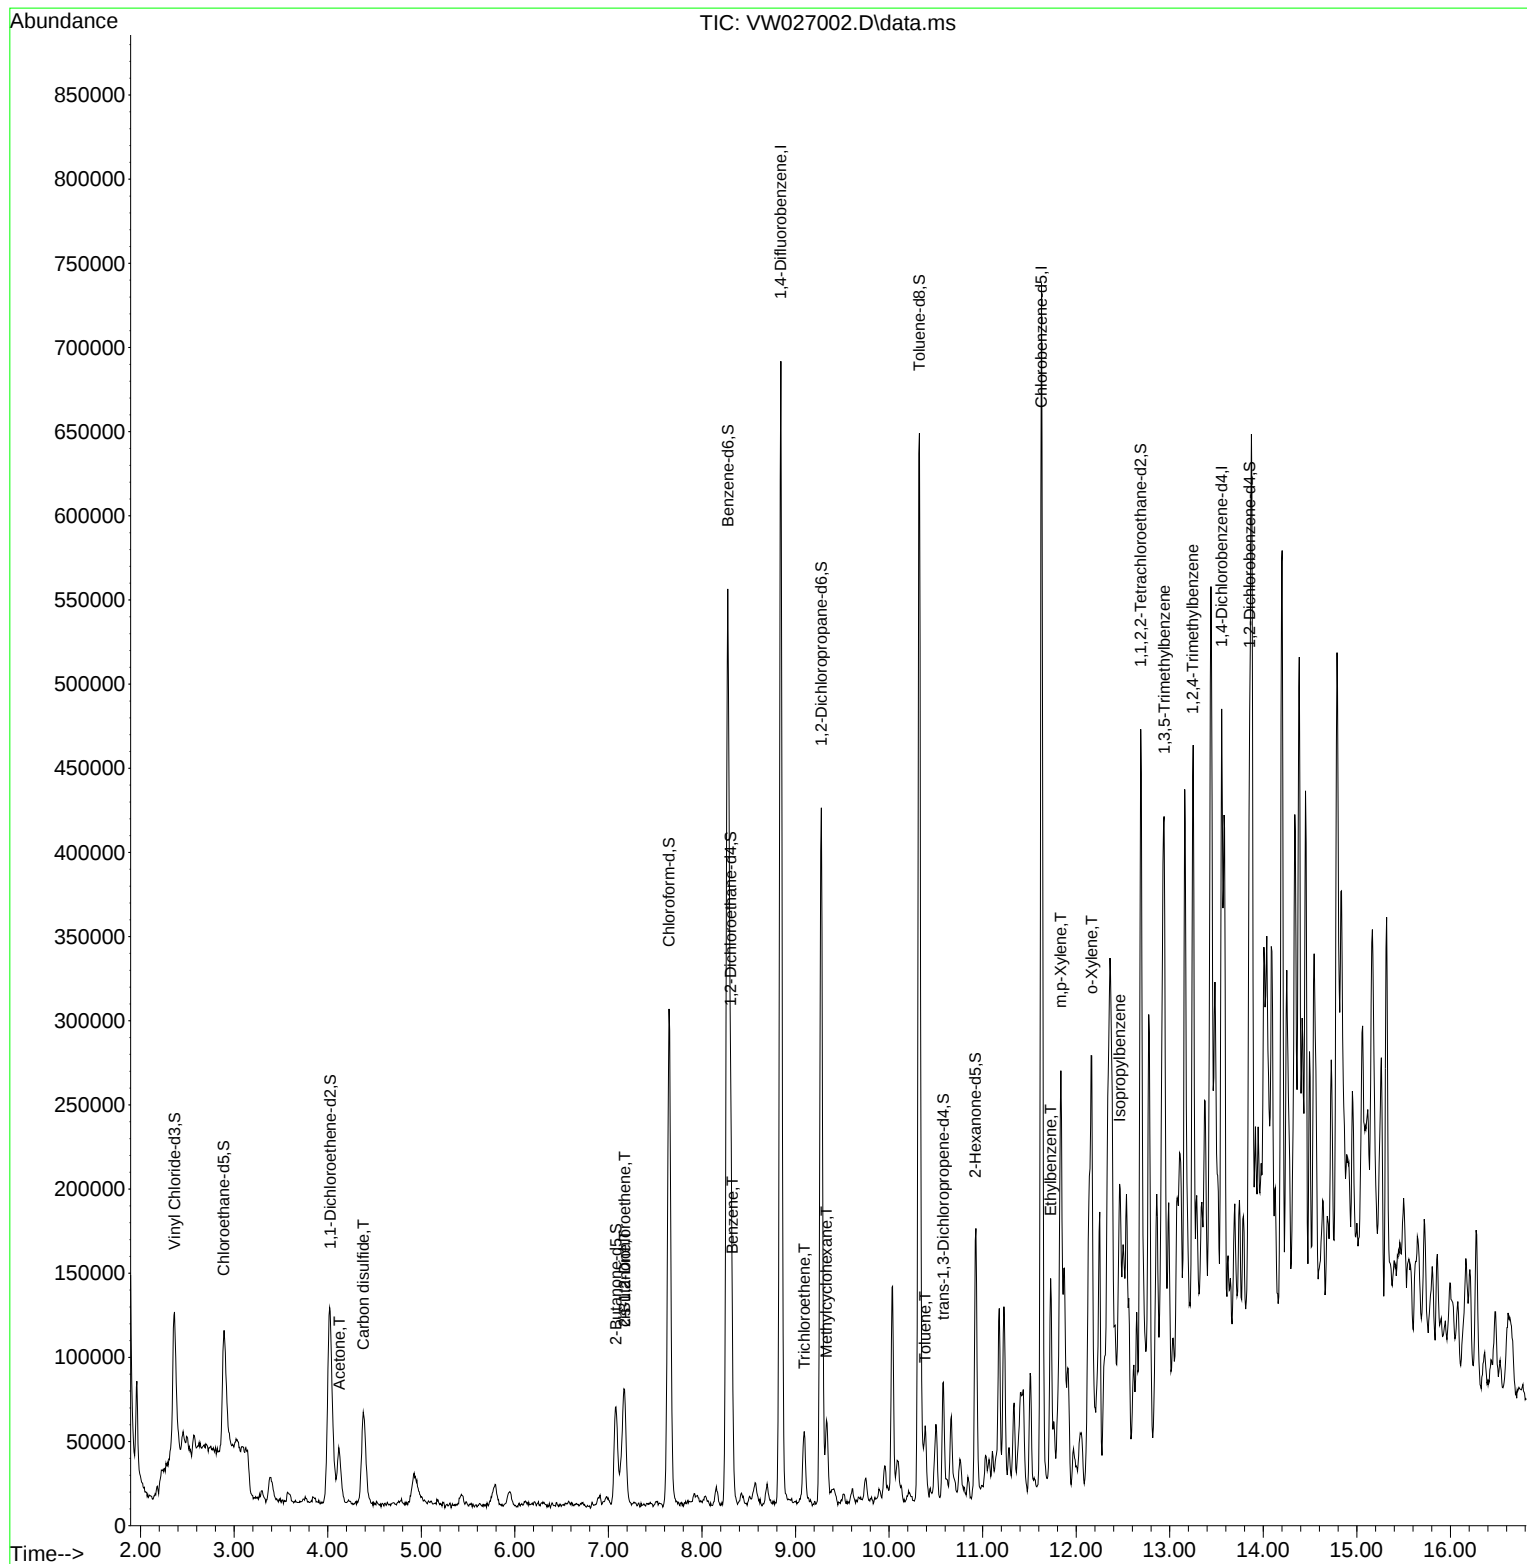







#13
Acetone
Concen: 30.078 ug/L
RT: 4.125 min Scan# 30
Delta R.T. 0.006 min
Lab File: VW027002.D
Acq: 07 Sep 2023 14:13

Instrument :
MSVOA_W
ClientSampleId :
EZYX8

Tgt Ion: 43 Resp: 50020
Ion Ratio Lower Upper
43 100
58 30.2 0.0 66.4




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 09/08/2023
Supervised By :Mahesh Dadoda 09/08/2023

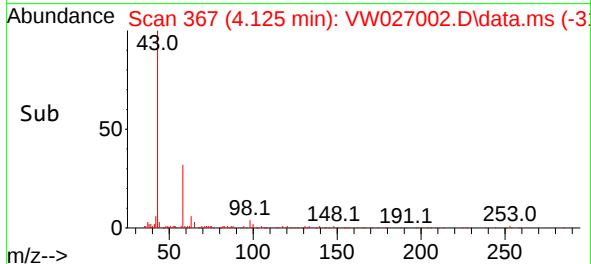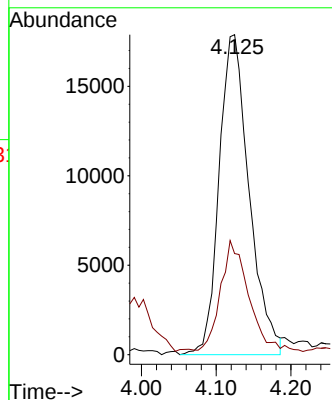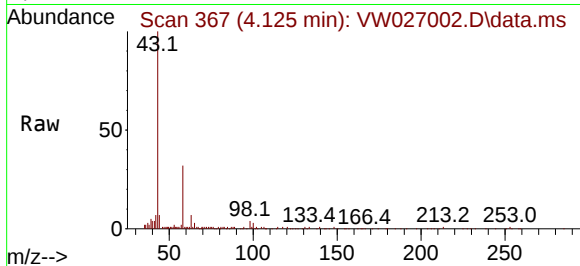

#14
Carbon disulfide
Concen: 5.468 ug/L
RT: 4.381 min Scan# 409
Delta R.T. -0.018 min
Lab File: VW027002.D
Acq: 07 Sep 2023 14:13

Tgt Ion: 76 Resp: 136711
Ion Ratio Lower Upper
76 100
78 8.4 7.8 11.8

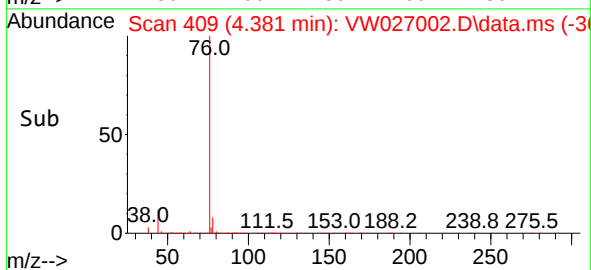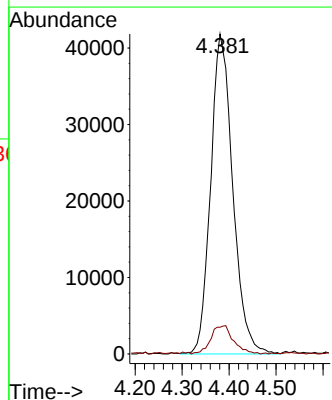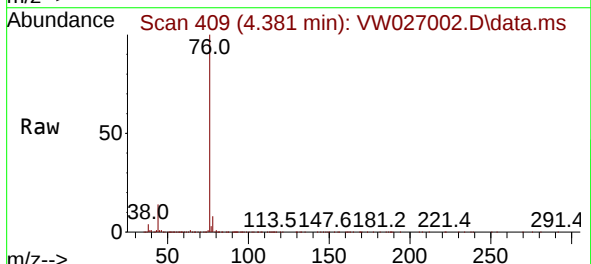







#20
 cis-1,2-Dichloroethene
 Concen: 3.774 ug/L
 RT: 7.173 min Scan# 867
 Delta R.T. -0.000 min
 Lab File: VW027002.D
 Acq: 07 Sep 2023 14:13

Instrument :
 MSVOA_W
 ClientSampleId :
 EYZX8

Tgt Ion: 96 Resp: 35438
 Ion Ratio Lower Upper
 96 100
 61 141.6 89.0 165.4
 98 67.8 43.6 81.0




Manual Integrations
 APPROVED


Reviewed By :Semsettin Yesilyurt 09/08/2023
 Supervised By :Mahesh Dadoda 09/08/2023

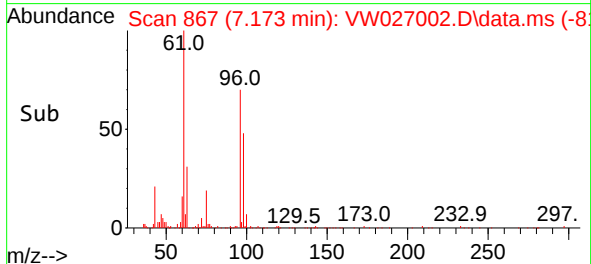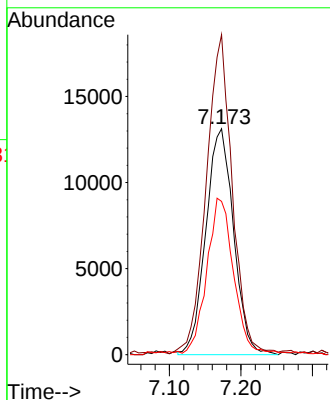

#22
 2-Butanone
 Concen: 5.089 ug/L
 RT: 7.173 min Scan# 867
 Delta R.T. -0.000 min
 Lab File: VW027002.D
 Acq: 07 Sep 2023 14:13

Tgt Ion: 43 Resp: 13616
 Ion Ratio Lower Upper
 43 100
 72 19.0 14.4 43.0

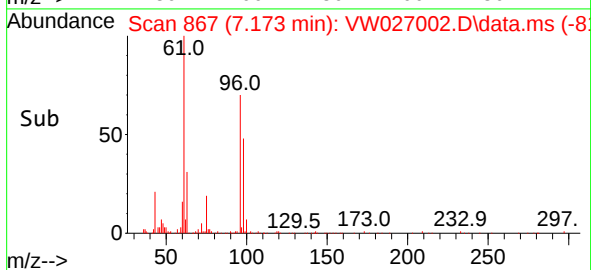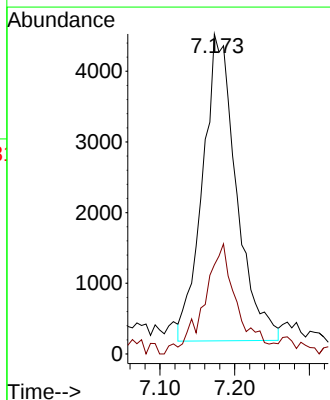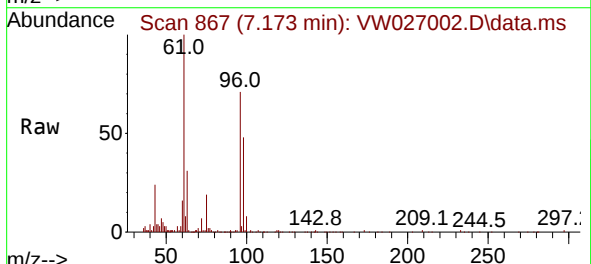

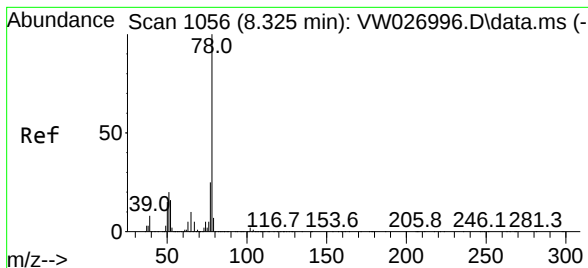

#33

Benzene

Concen: 0.890 ug/L

RT: 8.325 min Scan# 1056

Delta R.T. -0.000 min

Lab File: VW027002.D

Acq: 07 Sep 2023 14:13

Instrument :

MSVOA_W

ClientSampleId :

EZYX8





Tgt Ion: 78 Resp: 2389

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 09/08/2023

Supervised By :Mahesh Dadoda 09/08/2023

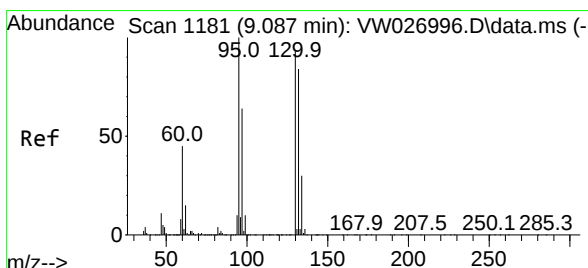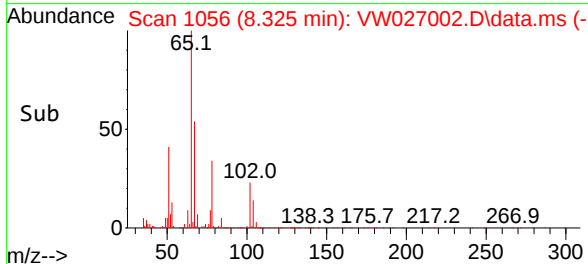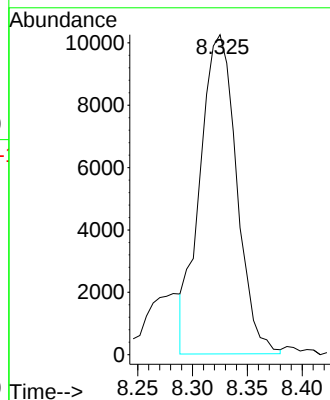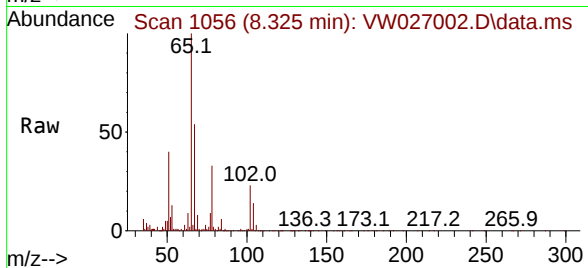

#34

Trichloroethene

Concen: 2.107 ug/L

RT: 9.093 min Scan# 1182

Delta R.T. 0.006 min

Lab File: VW027002.D

Acq: 07 Sep 2023 14:13

Tgt Ion: 95 Resp: 14529




Ion Ratio Lower Upper


95 100

97 66.7 42.4 78.8

132 102.2 63.1 117.3


130 107.4 69.7 129.5

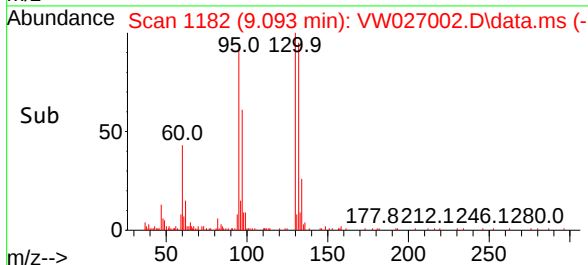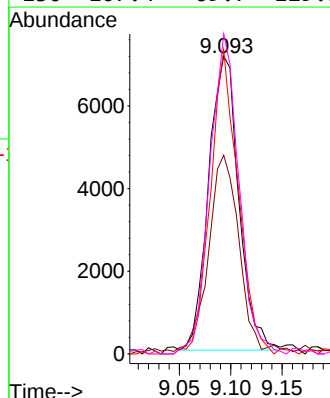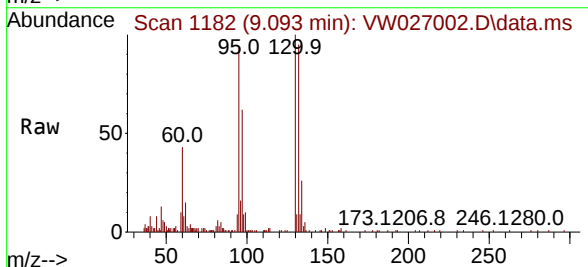

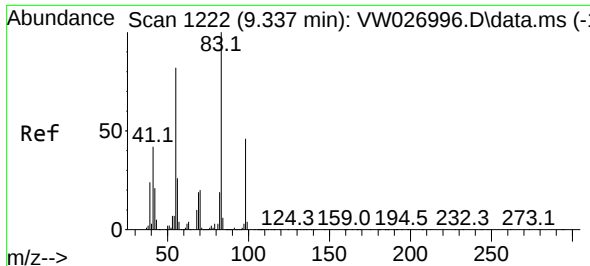

#35
Methylcyclohexane
Concen: 1.453 ug/L
RT: 9.331 min Scan# 1222
Delta R.T. -0.006 min
Lab File: VW027002.D
Acq: 07 Sep 2023 14:13




Instrument :
MSVOA_W
ClientSampleId :
EZYX8

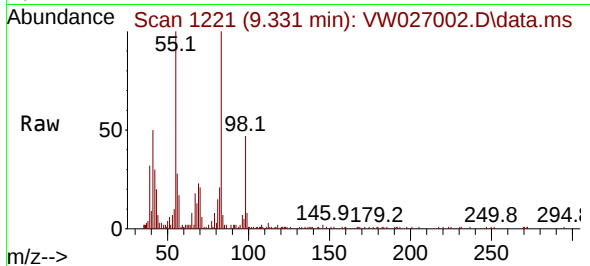

Tgt Ion: 83 Resp: 17020
Ion Ratio Lower Upper
83 100
55 100.5 61.7 92.5
98 51.2 38.3 57.5




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 09/08/2023
Supervised By :Mahesh Dadoda 09/08/2023

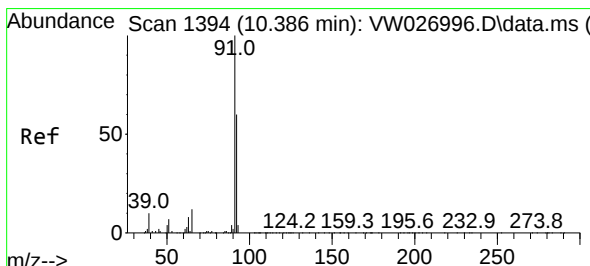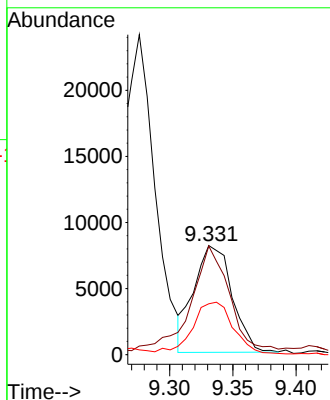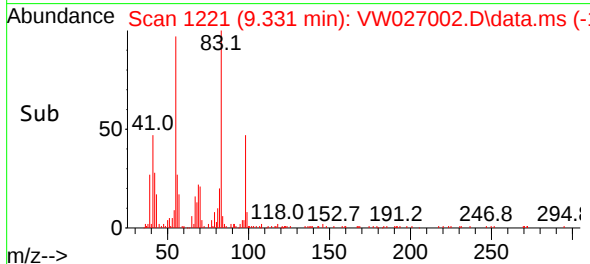

#42
Toluene
Concen: 1.076 ug/L
RT: 10.386 min Scan# 1394
Delta R.T. -0.000 min
Lab File: VW027002.D
Acq: 07 Sep 2023 14:13


Tgt Ion: 91 Resp: 29707
Ion Ratio Lower Upper
91 100
92 56.7 41.6 77.2

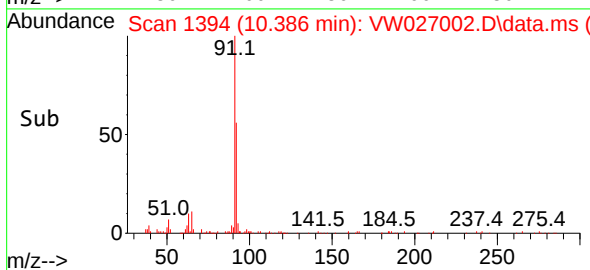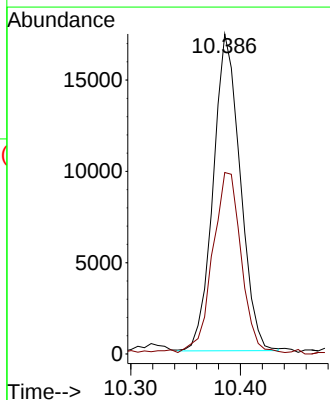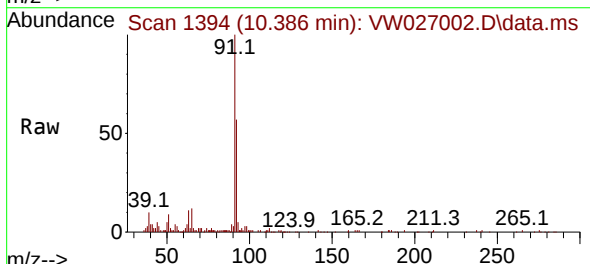

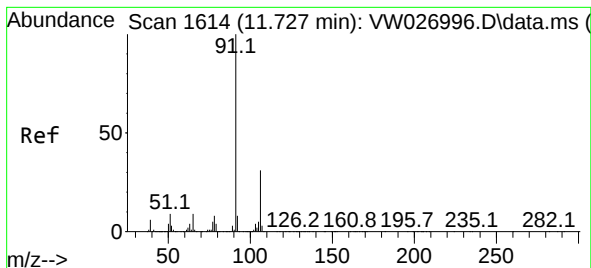

#52
Ethylbenzene
Concen: 2.212 ug/L
RT: 11.727 min Scan# 1614
Delta R.T. -0.000 min
Lab File: VW027002.D
Acq: 07 Sep 2023 14:13




Instrument :
MSVOA_W
ClientSampleId :
EZYX8

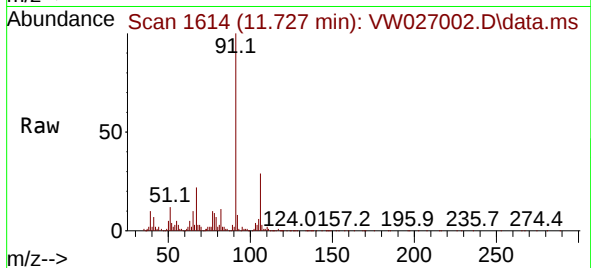


Tgt Ion: 91 Resp: 67738
Ion Ratio Lower Upper
91 100
106 29.4 21.1 39.3

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 09/08/2023
Supervised By :Mahesh Dadoda 09/08/2023

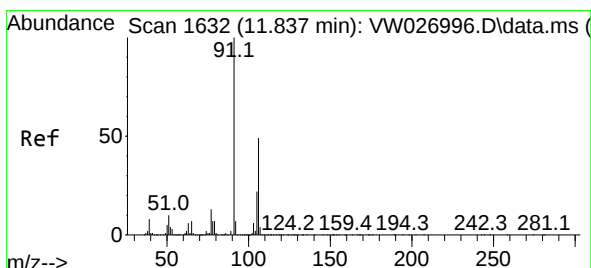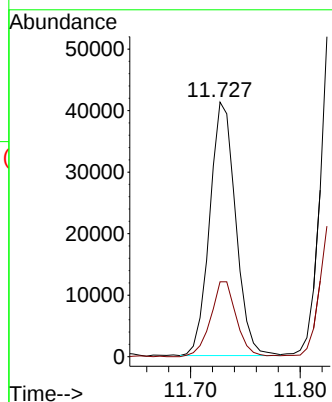


#53
m,p-Xylene
Concen: 5.627 ug/L
RT: 11.837 min Scan# 1632
Delta R.T. -0.000 min
Lab File: VW027002.D
Acq: 07 Sep 2023 14:13




Tgt Ion:106 Resp: 65172
Ion Ratio Lower Upper
106 100
91 213.7 139.6 259.2

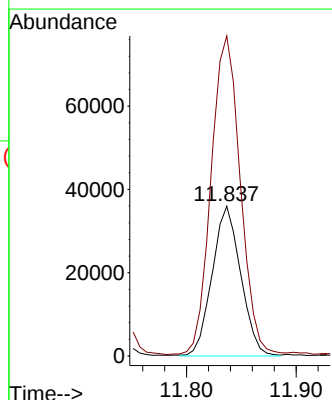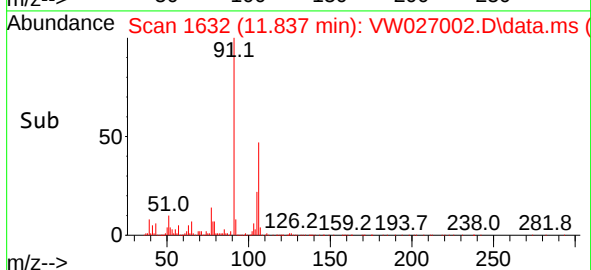



#54
o-Xylene
Concen: 5.548 ug/L
RT: 12.166 min Scan# 106
Delta R.T. -0.000 min
Lab File: VW027002.D
Acq: 07 Sep 2023 14:13




Instrument :
MSVOA_W
ClientSampleId :
EZYX8




Tgt Ion:106 Resp: 60128
Ion Ratio Lower Upper
106 100
91 212.3 154.0 286.0

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 09/08/2023
Supervised By :Mahesh Dadoda 09/08/2023

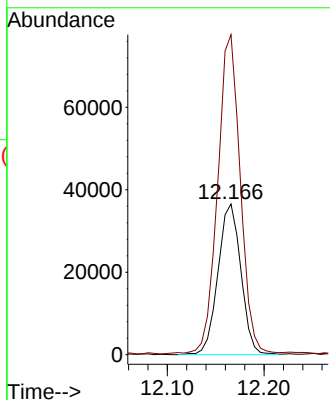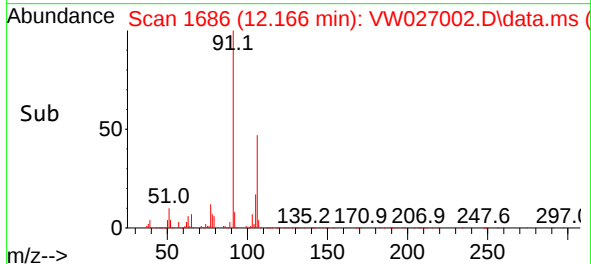


#60
Isopropylbenzene
Concen: 3.177 ug/L m
RT: 12.465 min Scan# 1735
Delta R.T. 0.006 min
Lab File: VW027002.D
Acq: 07 Sep 2023 14:13

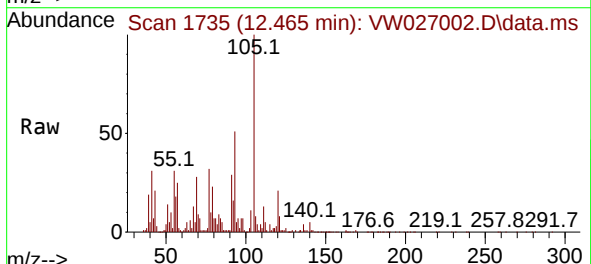

Tgt Ion:105 Resp: 41881
Ion Ratio Lower Upper
105 100
120 23.3 21.4 32.0
77 12.8 12.8 19.2#

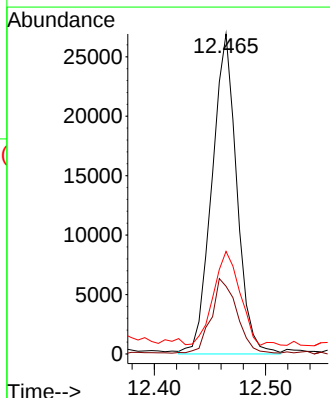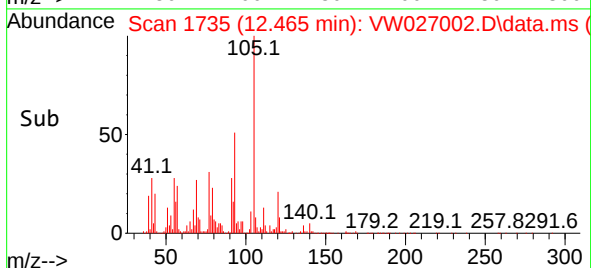

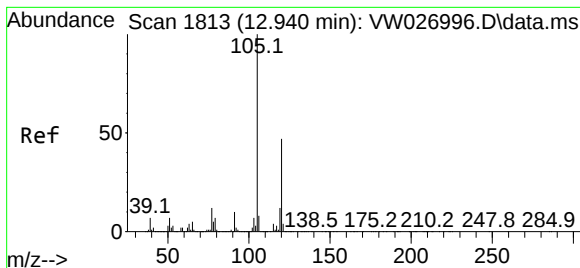

#62

1,3,5-Trimethylbenzene

Concen: 4.043 ug/L

RT: 12.940 min Scan# 1813

Delta R.T. -0.000 min

Lab File: VW027002.D

Acq: 07 Sep 2023 14:13

Instrument :

MSVOA_W

ClientSampleId :

EZYX8

Tgt Ion:105 Resp: 42538

Ion Ratio Lower Upper

105 100





120 48.9 39.0 58.6

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 09/08/2023

Supervised By :Mahesh Dadoda 09/08/2023

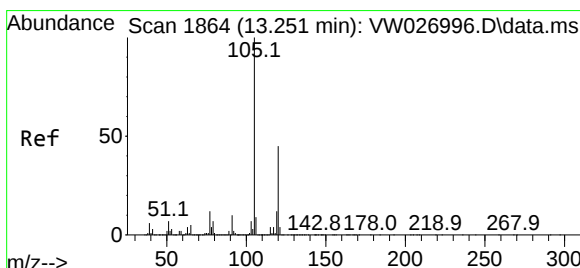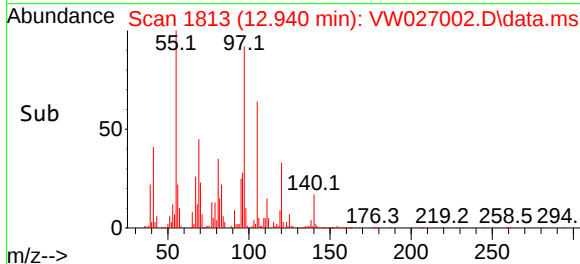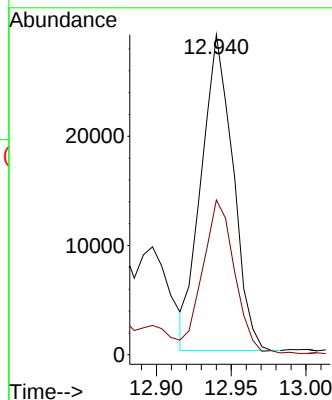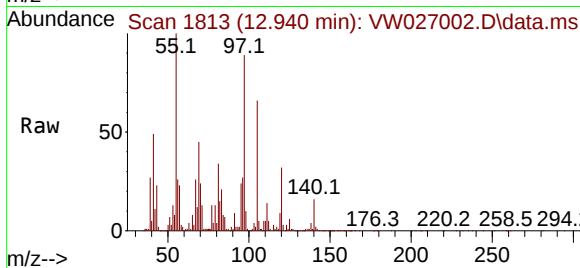

#63

1,2,4-Trimethylbenzene

Concen: 18.792 ug/L

RT: 13.245 min Scan# 1863

Delta R.T. -0.006 min

Lab File: VW027002.D

Acq: 07 Sep 2023 14:13

Tgt Ion:105 Resp: 193278

Ion Ratio Lower Upper

105 100

120 46.9 36.3 54.5

