

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090822\
 Data File : VW024584.D
 Acq On : 08 Sep 2022 11:58
 Operator : SY/VA
 Sample : VW0908SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK598

Quant Time: Sep 08 22:24:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Sep 08 22:22:19 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	292668	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	288607	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	127954	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	157947	26.140	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 104.560%			
7) Chloroethane-d5	2.879	69	120280	26.771	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 107.080%			
11) 1,1-Dichloroethene-d2	4.007	63	111861	17.547	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 70.200%			
21) 2-Butanone-d5	7.074	46	44286	45.433	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 90.860%			
24) Chloroform-d	7.647	84	180319	24.191	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 96.760%			
26) 1,2-Dichloroethane-d4	8.305	65	110711	26.343	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 105.360%			
32) Benzene-d6	8.275	84	368315	25.944	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 103.760%			
36) 1,2-Dichloropropane-d6	9.274	67	104134	24.879	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 99.520%			
41) Toluene-d8	10.323	98	347408	25.102	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 100.400%			
43) trans-1,3-Dichloroprop...	10.579	79	44368	23.653	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 94.600%			
47) 2-Hexanone-d5	10.920	63	36169	47.011	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 94.020%			
56) 1,1,2,2-Tetrachloroeth...	12.688	84	89120	22.215	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 88.840%			
66) 1,2-Dichlorobenzene-d4	13.853	152	107901	26.624	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 106.480%			
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.037	75	4275	0.715	ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090822\
Data File : VW024584.D
Acq On : 08 Sep 2022 11:58
Operator : SY/VA
Sample : VW0908SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK598

Quant Time: Sep 08 22:24:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090622SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Sep 08 22:22:19 2022
Response via : Initial Calibration

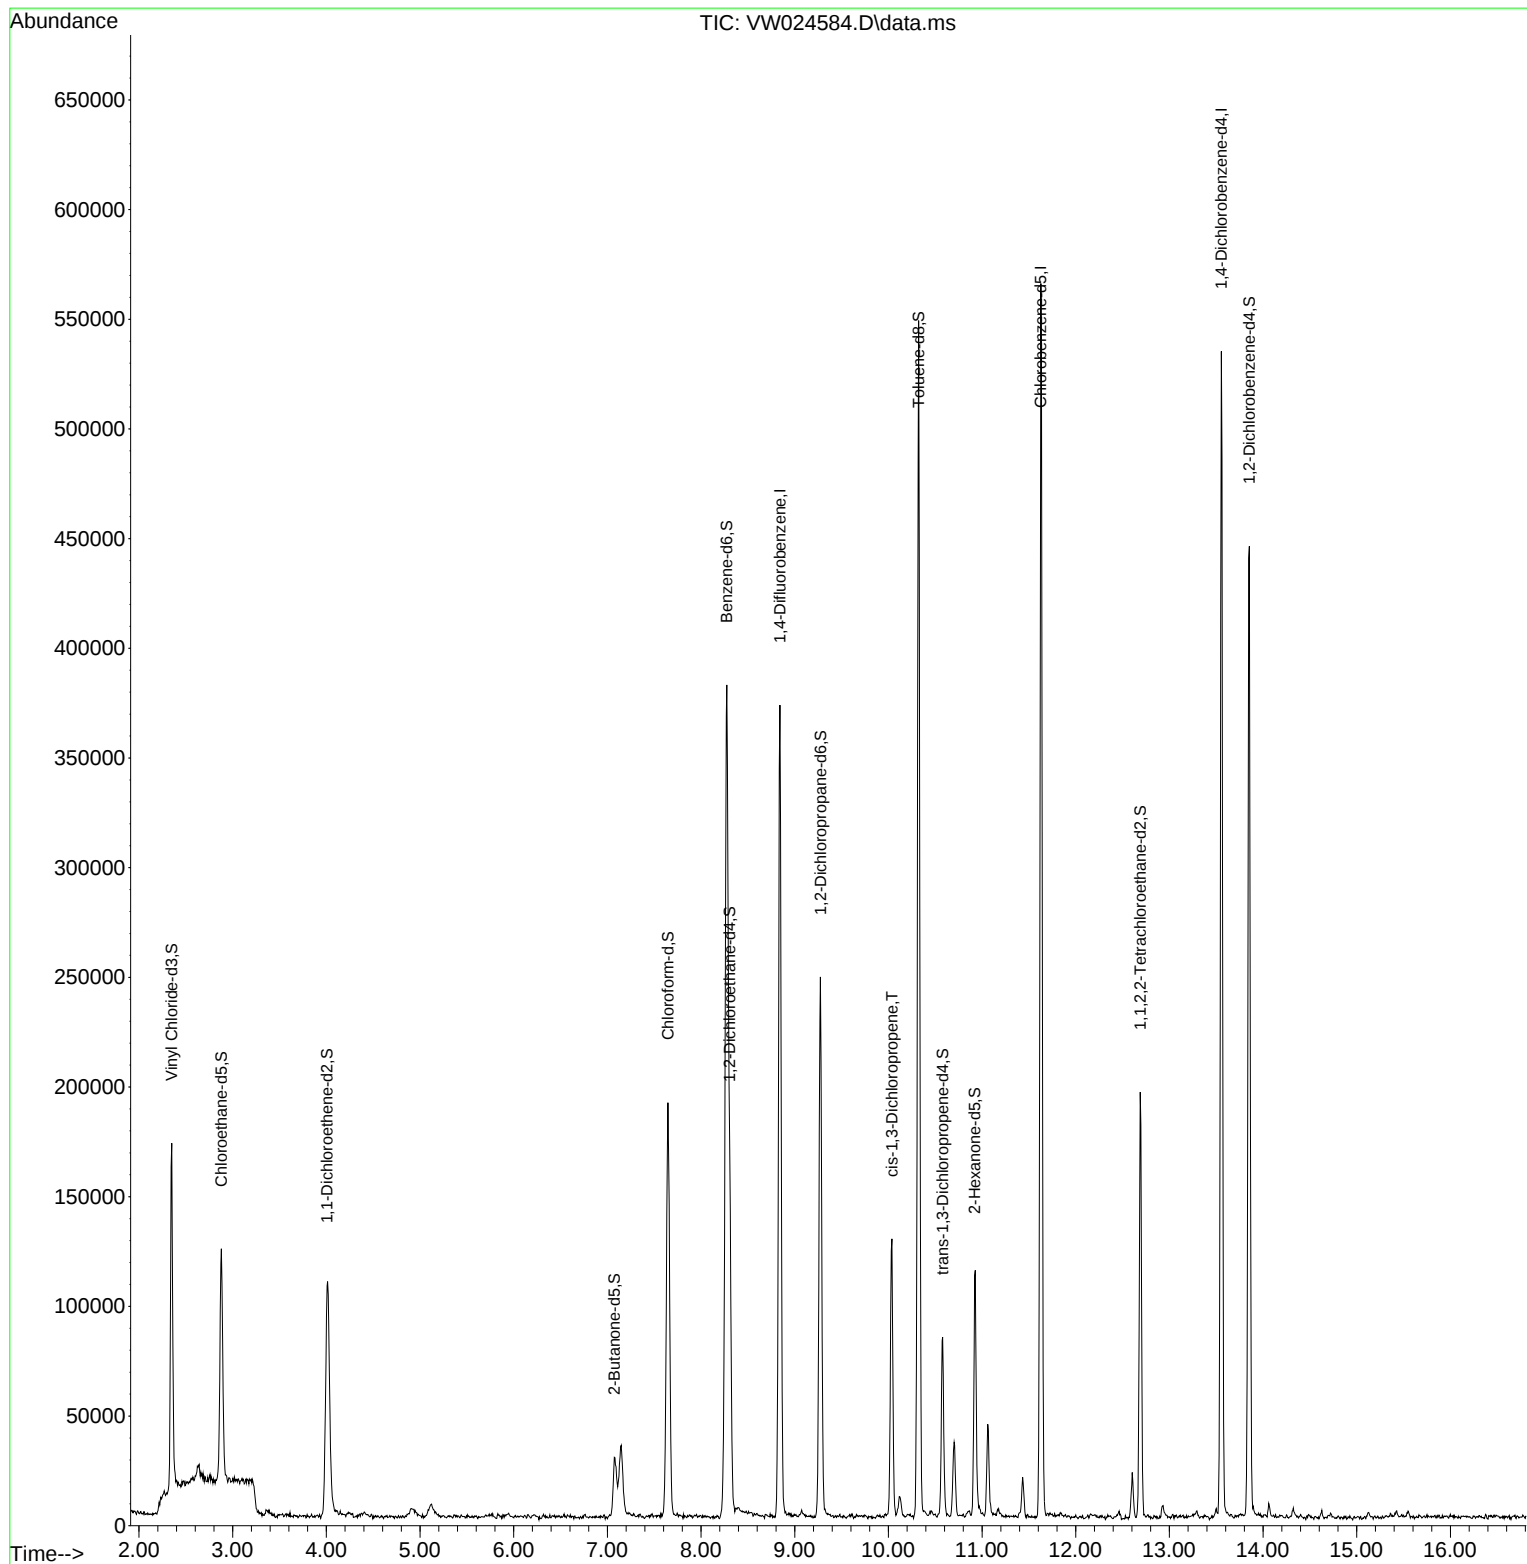

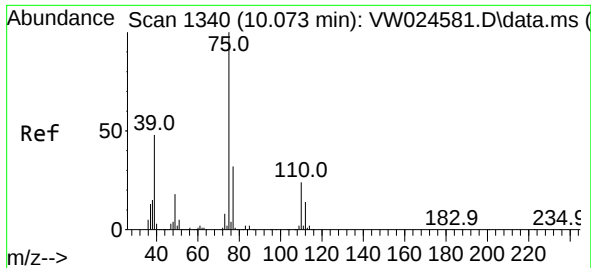

#39
 cis-1,3-Dichloropropene
 Concen: 0.715 ug/L
 RT: 10.037 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW024584.D
 Acq: 08 Sep 2022 11:58

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK598

Tgt Ion: 75 Resp: 4275
 Ion Ratio Lower Upper
 75 100
 77 38.2 21.9 40.7

