

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090823\
 Data File : VW027018.D
 Acq On : 08 Sep 2023 12:15
 Operator : SY/MD
 Sample : VW0908SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Sep 09 03:00:22 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Sep 09 02:59:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	463396	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	472598	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	221213	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	184824	22.325	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.280%
7) Chloroethane-d5	2.765	69	229	0.034	ug/L	-0.13
Spiked Amount	25.000	Range	30 - 150	Recovery	=	0.120%#
11) 1,1-Dichloroethene-d2	4.027	65	71757	23.518	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	94.080%
21) 2-Butanone-d5	7.081	46	82731	51.863	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.720%
24) Chloroform-d	7.642	84	355793	25.802	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	103.200%
26) 1,2-Dichloroethane-d4	8.307	65	199122	27.473	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	109.880%
32) Benzene-d6	8.276	84	737858	23.803	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.200%
36) 1,2-Dichloropropane-d6	9.270	67	231068	25.391	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.560%
41) Toluene-d8	10.325	98	642672	22.899	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	91.600%
43) trans-1,3-Dichloroprop...	10.581	79	83774	23.721	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	94.880%
47) 2-Hexanone-d5	10.922	63	39923	46.990	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.980%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	190475	26.971	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	107.880%
66) 1,2-Dichlorobenzene-d4	13.849	152	201510	26.338	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	105.360%
Target Compounds						Qvalue
68) 1,2-Dibromo-3-chloropr...	14.348	75	1028	1.071	ug/L	# 20


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090823\
Data File : VW027018.D
Acq On : 08 Sep 2023 12:15
Operator : SY/MD
Sample : VW0908SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Sep 09 03:00:22 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Sep 09 02:59:49 2023
Response via : Initial Calibration

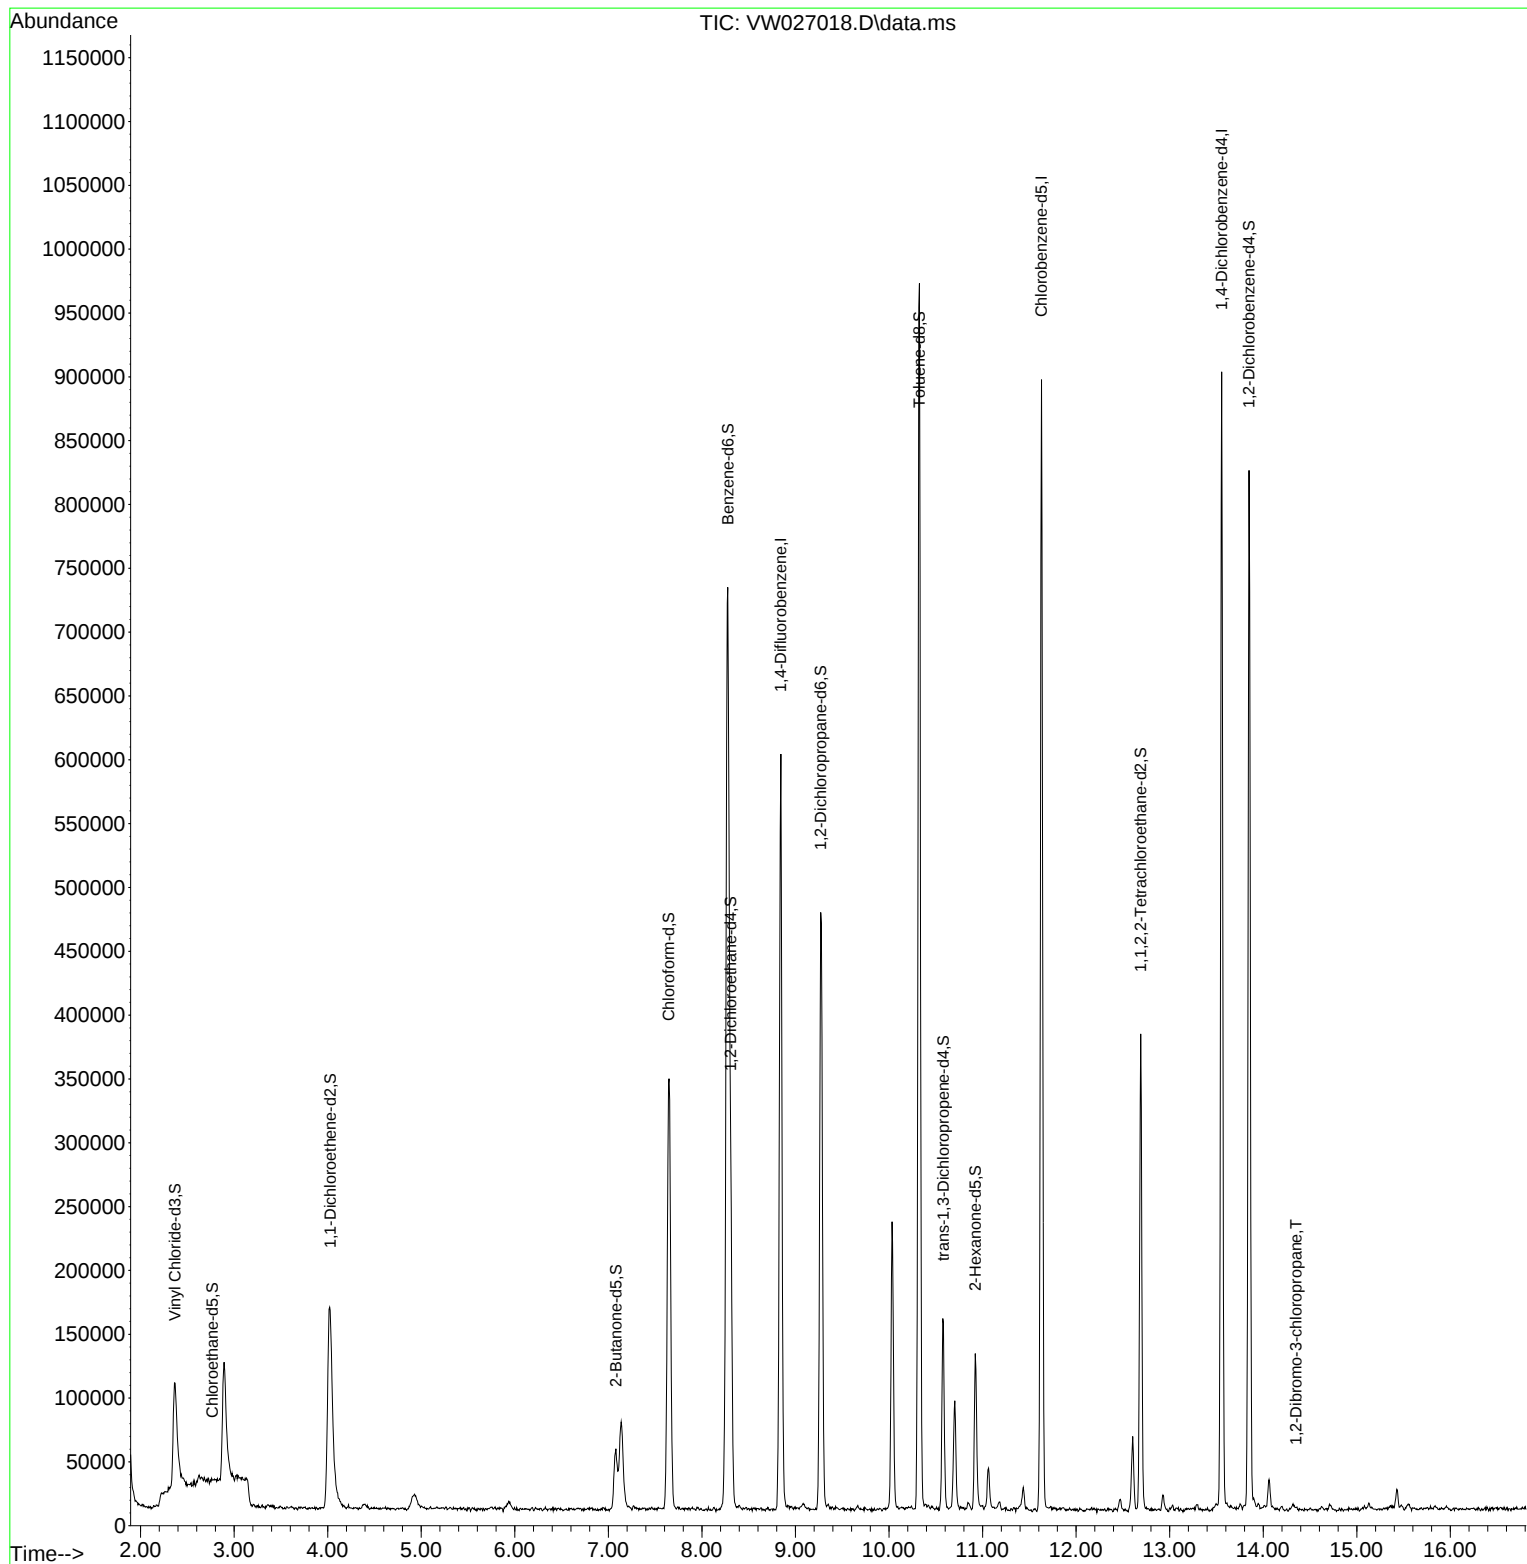

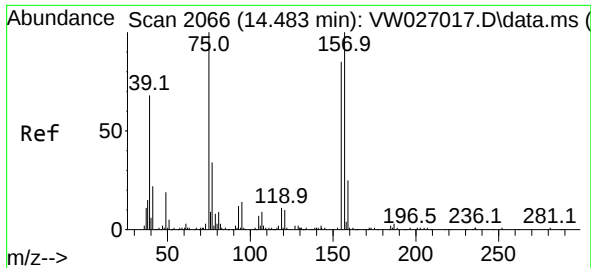

#68
1,2-Dibromo-3-chloropropane
Concen: 1.071 ug/L
RT: 14.348 min Scan# 2066
Delta R.T. -0.134 min
Lab File: VW027018.D
Acq: 08 Sep 2023 12:15

Instrument :
MSVOA_W
ClientSampleId :

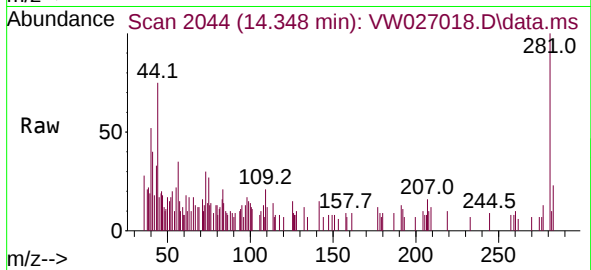

Tgt Ion: 75 Resp: 1028
Ion Ratio Lower Upper
75 100
155 0.0 65.9 98.9#
157 22.3 68.7 103.1#

