




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090823\
 Data File : VW027018.D
 Acq On : 08 Sep 2023 12:15
 Operator : SY/MD
 Sample : VW0908SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK567

Manual IntegrationsAPPROVED

Quant Time: Sep 09 03:00:22 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Sep 09 02:59:49 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/11/2023
 Supervised By :Mahesh Dadoda 09/11/2023

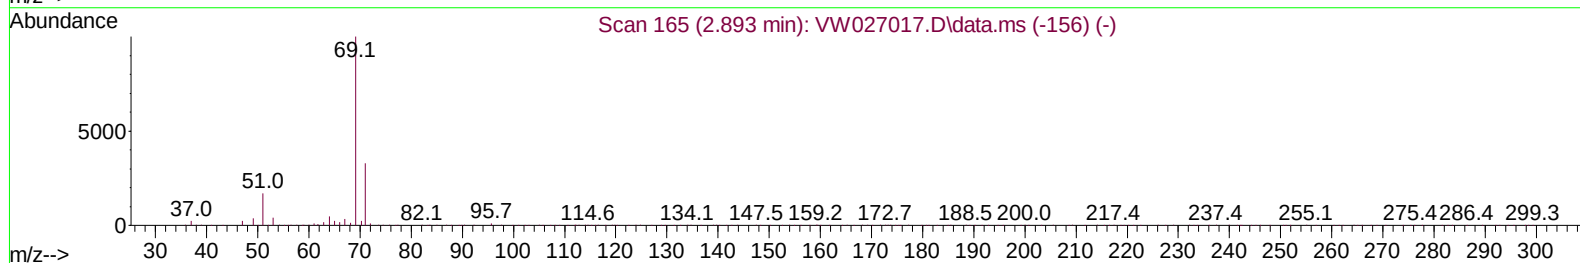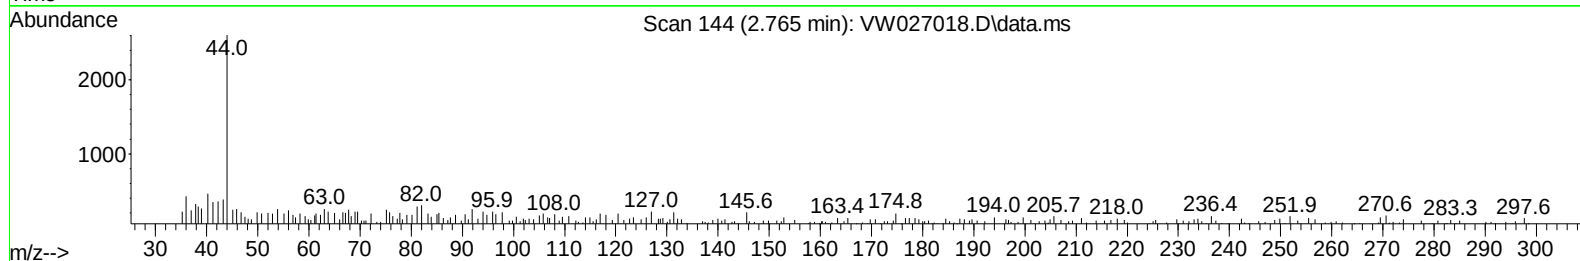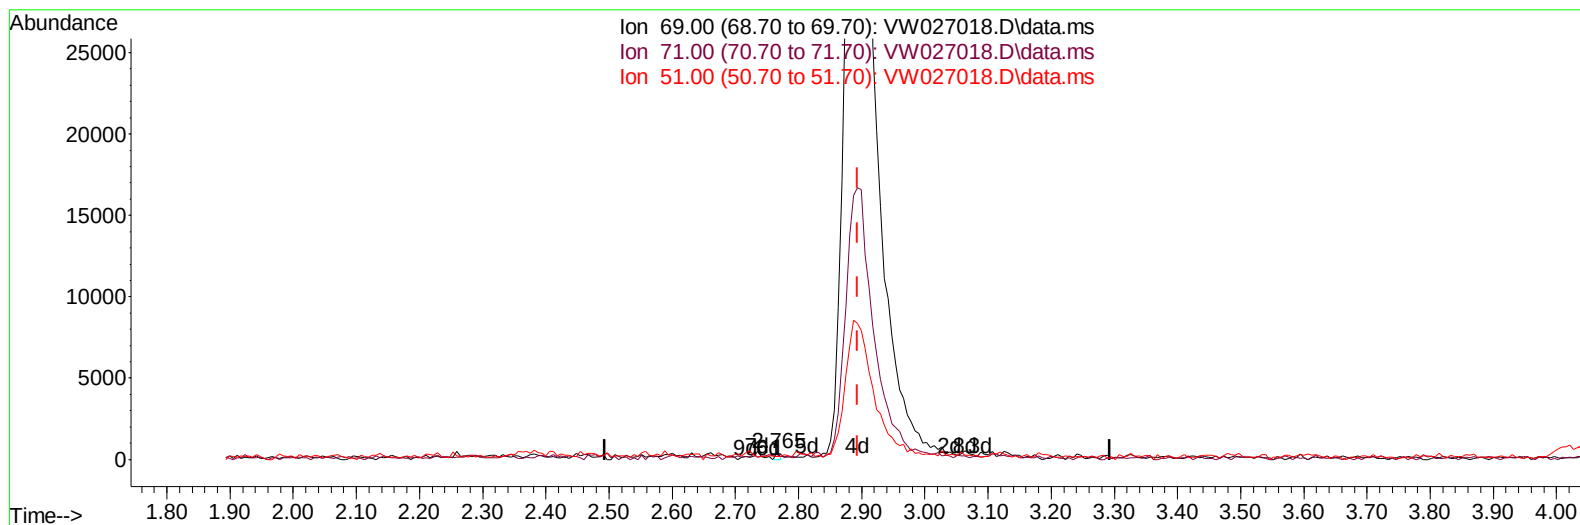

TIC: VW027018.D\data.ms

(7) Chloroethane-d5 (S)

2.765min (-0.128) 0.03 ug/L

response 229

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.80	39.30
51.00	22.50	28.38
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090823\
 Data File : VW027018.D
 Acq On : 08 Sep 2023 12:15
 Operator : SY/MD
 Sample : VW0908SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK567

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/11/2023
 Supervised By :Mahesh Dadoda 09/11/2023

Quant Time: Sep 09 03:00:22 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Sep 09 02:59:49 2023
 Response via : Initial Calibration

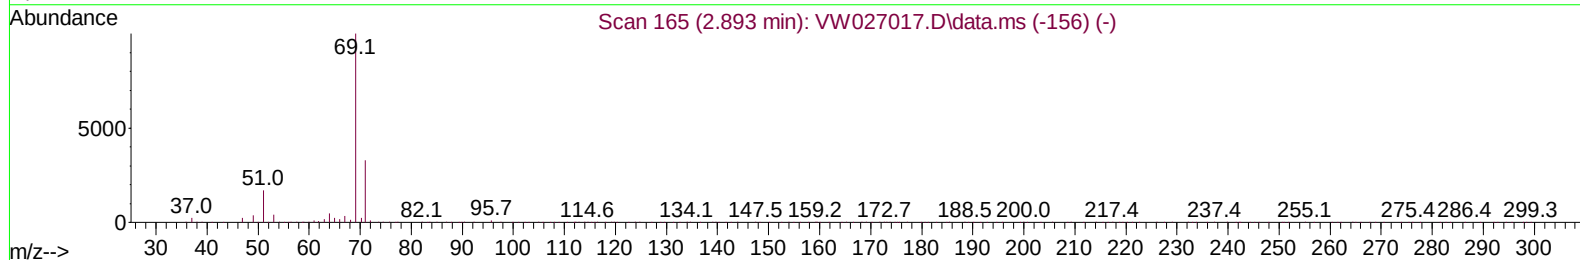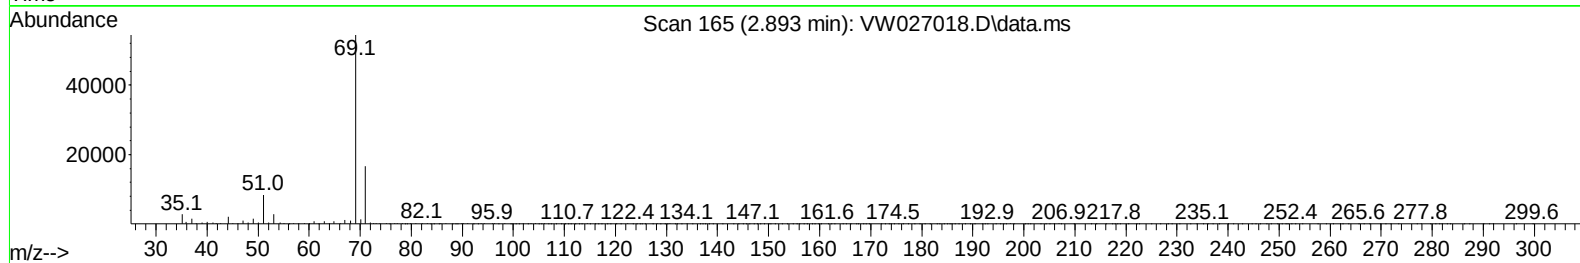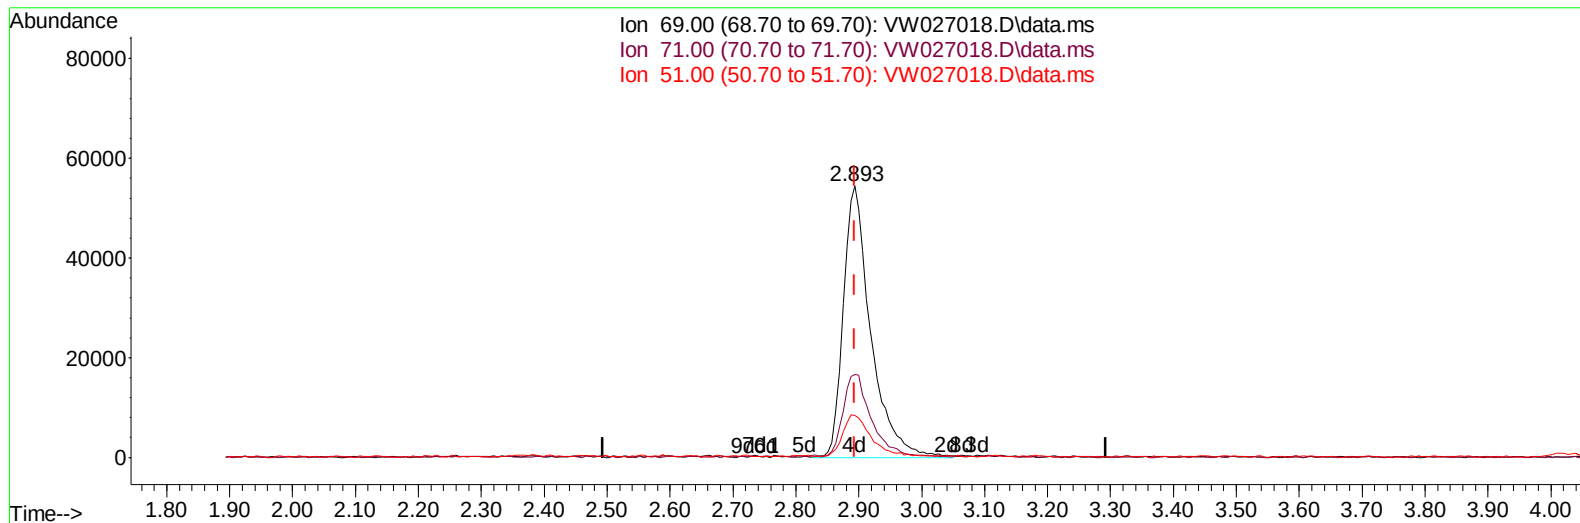

TIC: VW027018.D\data.ms

(7) Chloroethane-d5 (S)

2.893min (+ 0.000) 24.77 ug/L m

response 165522

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.80	0.05#
51.00	22.50	0.04#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090823\
 Data File : VW027018.D
 Acq On : 08 Sep 2023 12:15
 Operator : SY/MD
 Sample : VW0908SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK567

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/11/2023
 Supervised By :Mahesh Dadoda 09/11/2023

Quant Time: Sep 09 03:00:22 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Sep 09 02:59:49 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		463396	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		472598	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		221213	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.369	65		184824	22.325	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	89.280%		
7) Chloroethane-d5	2.893	69		165522m	24.773	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	99.080%		
11) 1,1-Dichloroethene-d2	4.027	65		71757	23.518	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	94.080%		
21) 2-Butanone-d5	7.081	46		82731	51.863	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	103.720%		
24) Chloroform-d	7.642	84		355793	25.802	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	103.200%		
26) 1,2-Dichloroethane-d4	8.307	65		199122	27.473	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	109.880%		
32) Benzene-d6	8.276	84		737858	23.803	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	95.200%		
36) 1,2-Dichloropropane-d6	9.270	67		231068	25.391	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	101.560%		
41) Toluene-d8	10.325	98		642672	22.899	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	91.600%		
43) trans-1,3-Dichloroprop...	10.581	79		83774	23.721	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	94.880%		
47) 2-Hexanone-d5	10.922	63		39923	46.990	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	93.980%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		190475	26.971	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	107.880%		
66) 1,2-Dichlorobenzene-d4	13.849	152		201510	26.338	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	105.360%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090823\
Data File : VW027018.D
Acq On : 08 Sep 2023 12:15
Operator : SY/MD
Sample : VW0908SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK567

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/11/2023
Supervised By :Mahesh Dadoda 09/11/2023

Quant Time: Sep 09 03:00:22 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Sep 09 02:59:49 2023
Response via : Initial Calibration

