




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090823\
 Data File : VW027021.D
 Acq On : 08 Sep 2023 13:28
 Operator : SY/MD
 Sample : 04332-08
 Misc : 4.26g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AC8

Manual IntegrationsAPPROVED

Quant Time: Sep 09 03:01:03 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Sep 09 02:59:49 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/11/2023
 Supervised By :Mahesh Dadoda 09/11/2023

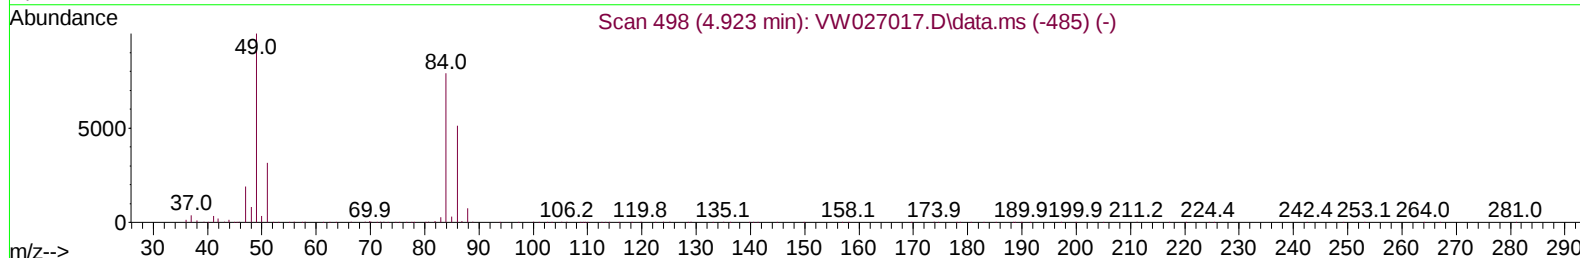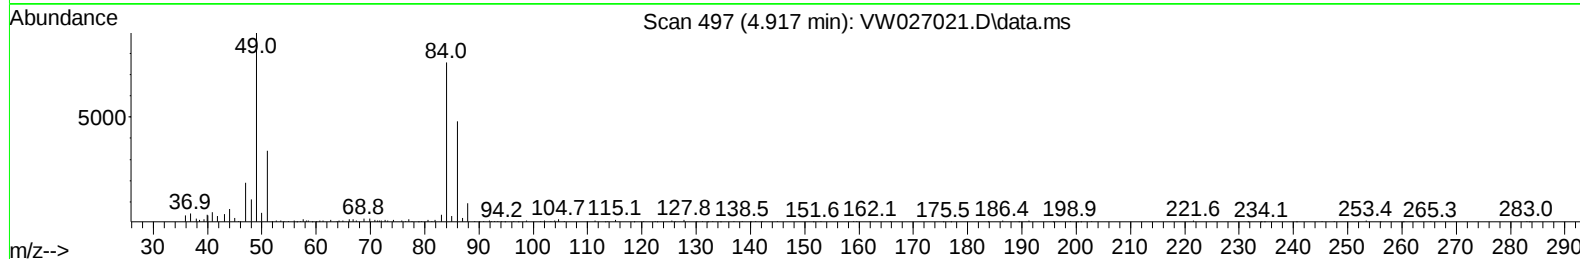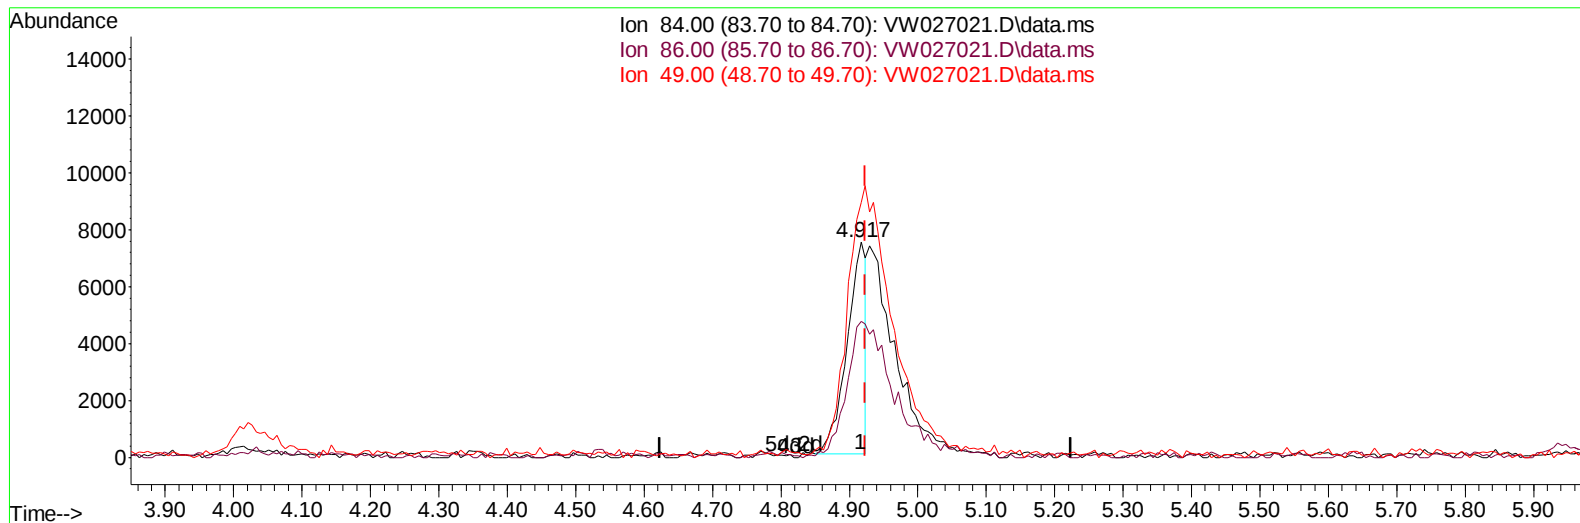

TIC: VW027021.D\data.ms

(16) Methylene chloride (T)

4.917min (-0.006) 1.45 ug/L

response 14404

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.00	63.17
49.00	117.30	118.41
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090823\
Data File : VW027021.D
Acq On : 08 Sep 2023 13:28
Operator : SY/MD
Sample : 04332-08
Misc : 4.26g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AC8

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/11/2023
Supervised By :Mahesh Dadoda 09/11/2023

Quant Time: Sep 09 03:01:03 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Sep 09 02:59:49 2023
Response via : Initial Calibration

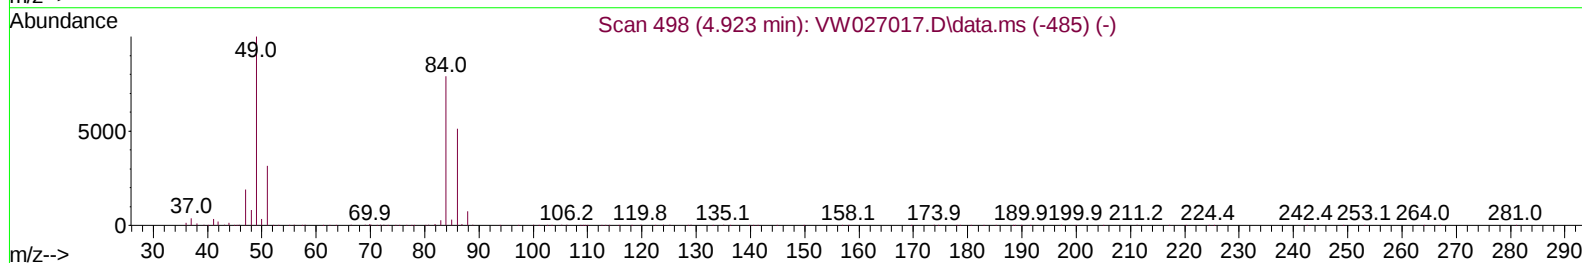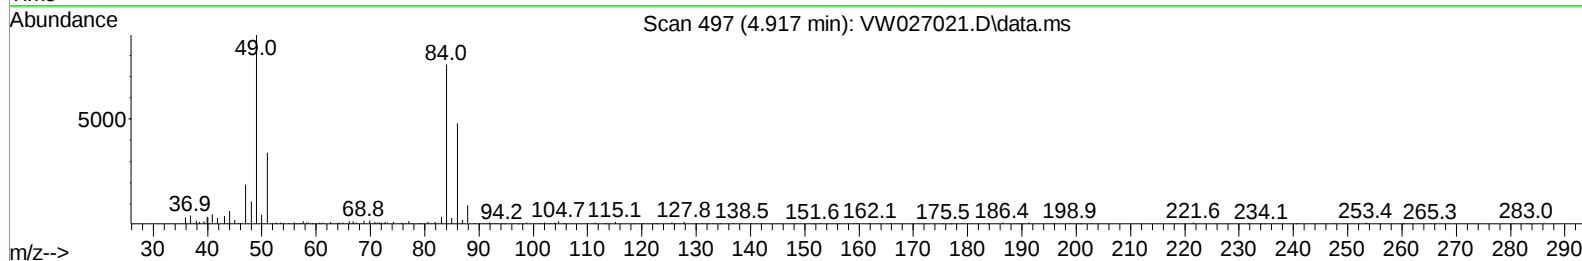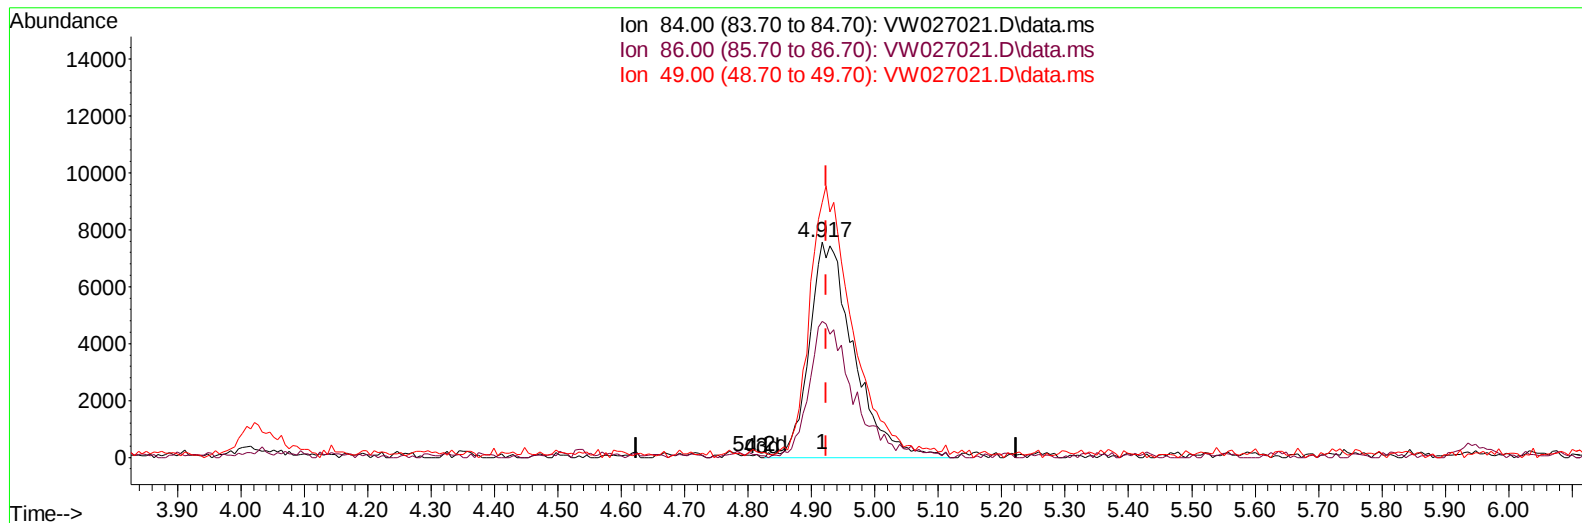

TIC: VW027021.D\data.ms

(16) Methylene chloride (T)

4.917min (-0.006) 3.70 ug/L m

response 36862

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.00	63.17
49.00	117.30	118.41
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090823\
 Data File : VW027021.D
 Acq On : 08 Sep 2023 13:28
 Operator : SY/MD
 Sample : 04332-08
 Misc : 4.26g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AC8

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/11/2023
 Supervised By :Mahesh Dadoda 09/11/2023

Quant Time: Sep 09 03:01:03 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Sep 09 02:59:49 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		514328	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		368941	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		90117	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.369	65		144166	15.689	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	62.760%		
7) Chloroethane-d5	2.893	69		160190	21.600	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	86.400%		
11) 1,1-Dichloroethene-d2	4.027	65		48453	14.308	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	57.240%		
21) 2-Butanone-d5	7.081	46		41168	23.252	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	46.500%		
24) Chloroform-d	7.654	84		335937	21.950	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	87.800%		
26) 1,2-Dichloroethane-d4	8.307	65		181612	22.576	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	90.320%		
32) Benzene-d6	8.276	84		602490	24.897	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	99.600%		
36) 1,2-Dichloropropane-d6	9.270	67		210359	29.610	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	118.440%		
41) Toluene-d8	10.325	98		412846	18.843	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	75.360%		
43) trans-1,3-Dichloroprop...	10.581	79		4032	1.462	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	5.840%#		
47) 2-Hexanone-d5	10.928	63		2583	3.894	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	7.780%#		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		142813	25.904	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	103.600%		
66) 1,2-Dichlorobenzene-d4	13.848	152		63893	20.500	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	82.000%		
Target Compounds							
						Qvalue	
13) Acetone	4.118	43		178964	115.441	ug/L	100
15) Methyl Acetate	4.673	43		23710	7.356	ug/L #	89
16) Methylene chloride	4.917	84		36862m	3.699	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090823\
Data File : VW027021.D
Acq On : 08 Sep 2023 13:28
Operator : SY/MD
Sample : 04332-08
Misc : 4.26g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AC8

Manual IntegrationsAPPROVED

Quant Time: Sep 09 03:01:03 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Sep 09 02:59:49 2023
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/11/2023
Supervised By :Mahesh Dadoda 09/11/2023

