

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090922\
 Data File : VW024592.D
 Acq On : 09 Sep 2022 10:15
 Operator : SY/VA
 Sample : VW0909SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK401

Quant Time: Sep 10 00:39:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Sep 10 00:38:15 2022
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		8.836	114	264920	25.000	ug/L	0.00
28) Chlorobenzene-d5		11.628	117	277253	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.554	152	118599	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		2.343	65	164215	30.024	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	= 120.080%		
7) Chloroethane-d5		2.873	69	119969	29.499	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	= 118.000%		
11) 1,1-Dichloroethene-d2		4.007	63	107098	18.559	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	= 74.240%		
21) 2-Butanone-d5		6.891	46	257	0.291	ug/L	-0.19
Spiked Amount	50.000	Range	20 - 135	Recovery	= 0.580%#		
24) Chloroform-d		7.647	84	178083	26.394	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	= 105.560%		
26) 1,2-Dichloroethane-d4		8.305	65	110946	29.164	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	= 116.640%		
32) Benzene-d6		8.275	84	360541	26.437	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	= 105.760%		
36) 1,2-Dichloropropane-d6		9.268	67	104203	25.915	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	= 103.640%		
41) Toluene-d8		10.323	98	336140	25.283	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	= 101.120%		
43) trans-1,3-Dichloroprop...		10.573	79	43111	23.924	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	= 95.680%		
47) 2-Hexanone-d5		10.921	63	39875	53.951	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	= 107.900%		
56) 1,1,2,2-Tetrachloroeth...		12.689	84	90180	23.399	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	= 93.600%		
66) 1,2-Dichlorobenzene-d4		13.847	152	105783	28.161	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	= 112.640%		
Target Compounds							Qvalue
39) cis-1,3-Dichloropropene		10.037	75	3888	0.677	ug/L	# 68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090922\
Data File : VW024592.D
Acq On : 09 Sep 2022 10:15
Operator : SY/VA
Sample : VW0909SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK401

Quant Time: Sep 10 00:39:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090622SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Sep 10 00:38:15 2022
Response via : Initial Calibration

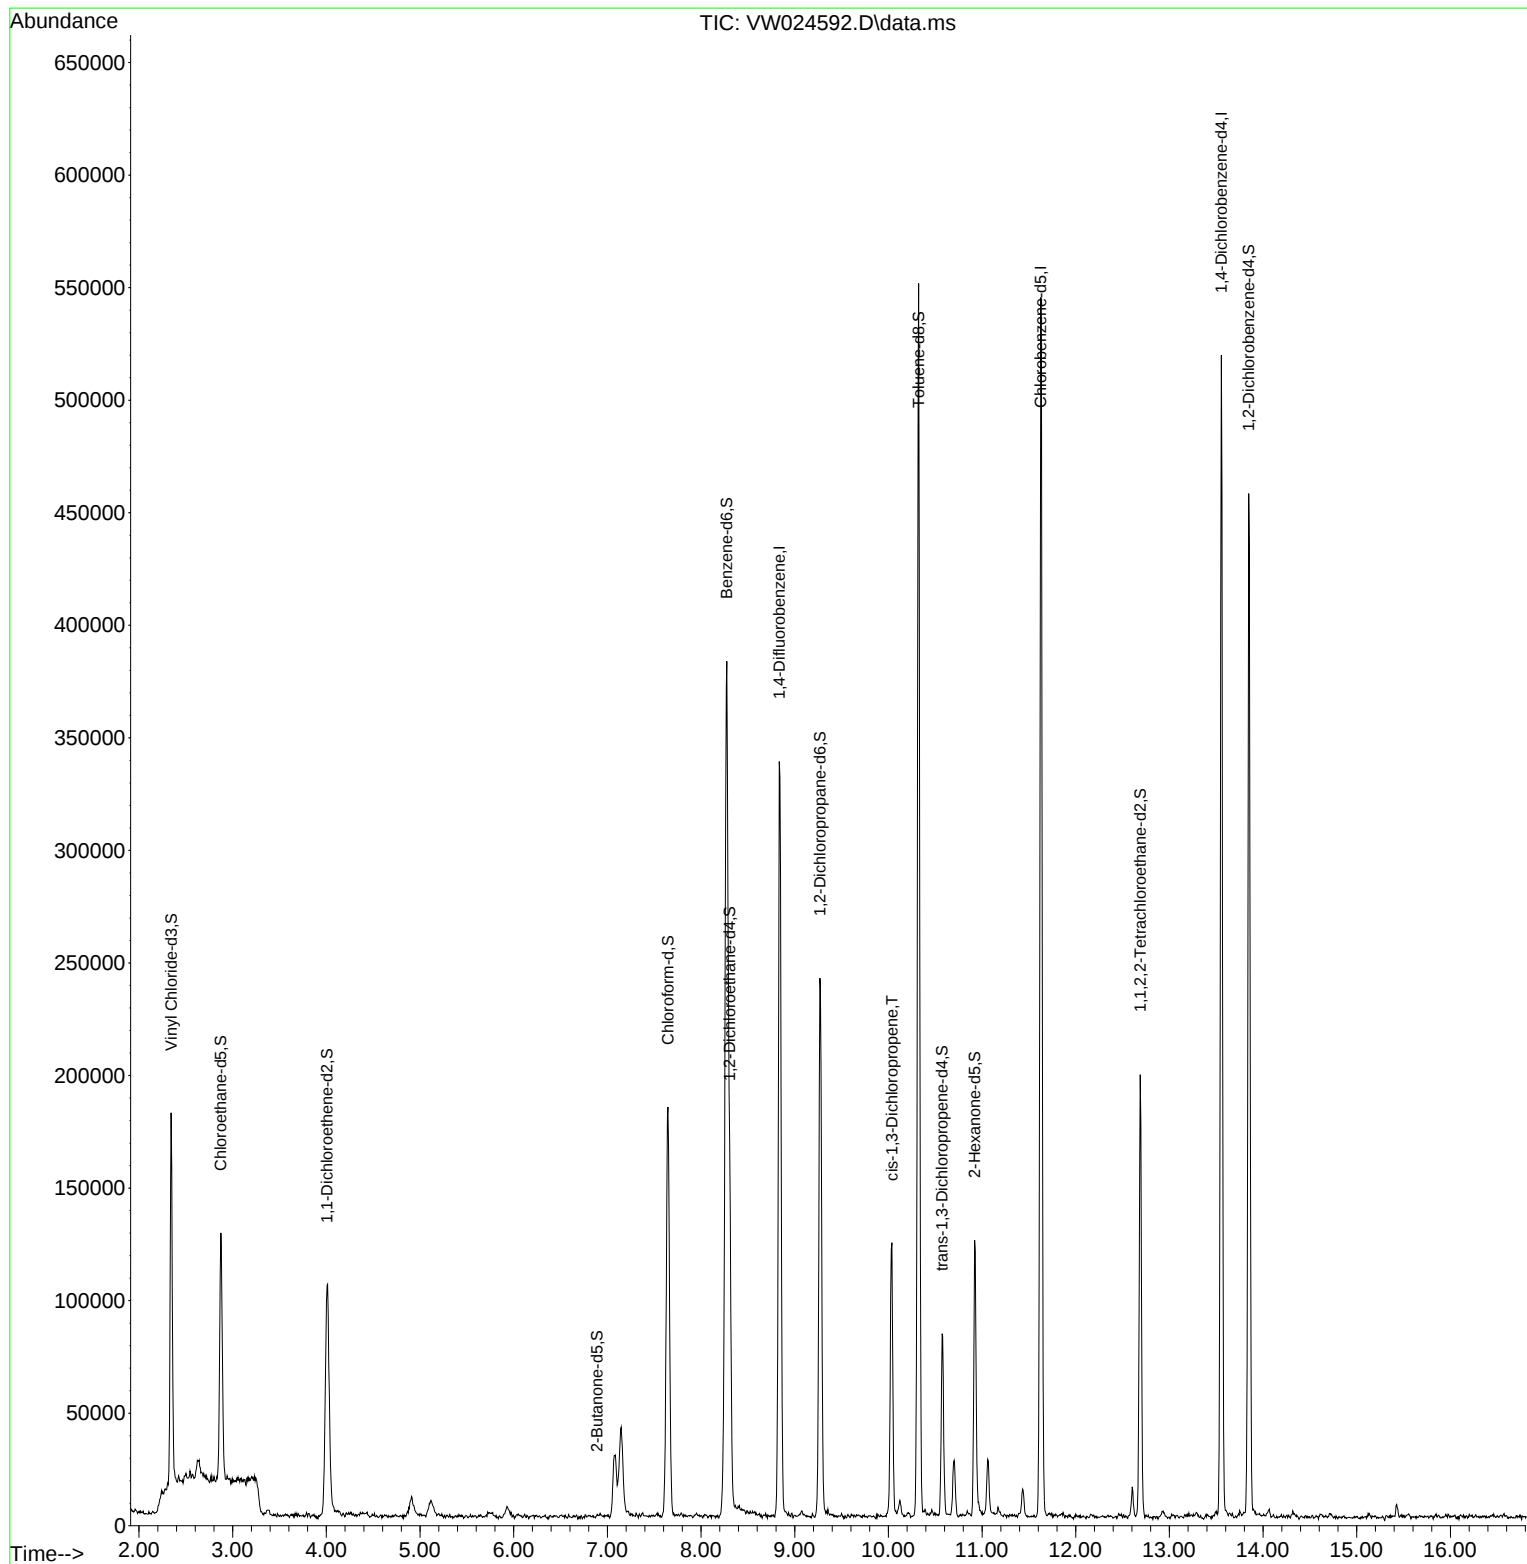

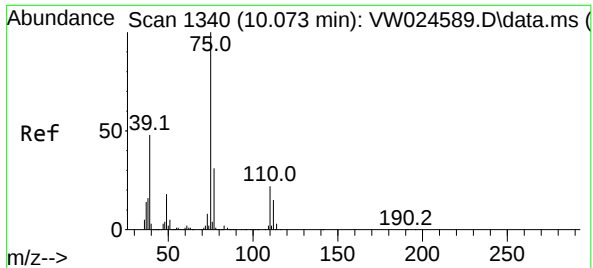

#39
 cis-1,3-Dichloropropene
 Concen: 0.677 ug/L
 RT: 10.037 min Scan# 11
 Delta R.T. -0.036 min
 Lab File: VW024592.D
 Acq: 09 Sep 2022 10:15

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK401

Tgt Ion: 75 Resp: 3888
 Ion Ratio Lower Upper
 75 100
 77 49.2 21.9 40.7#

