




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090922\
Data File : VW024596.D
Acq On : 09 Sep 2022 13:06
Operator : SY/VA
Sample : N4483-15
Misc : 5.05g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/12/2022
Supervised By :Mahesh Dadoda 09/12/2022

Quant Time: Sep 10 00:40:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090622SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Sep 10 00:38:15 2022
Response via : Initial Calibration

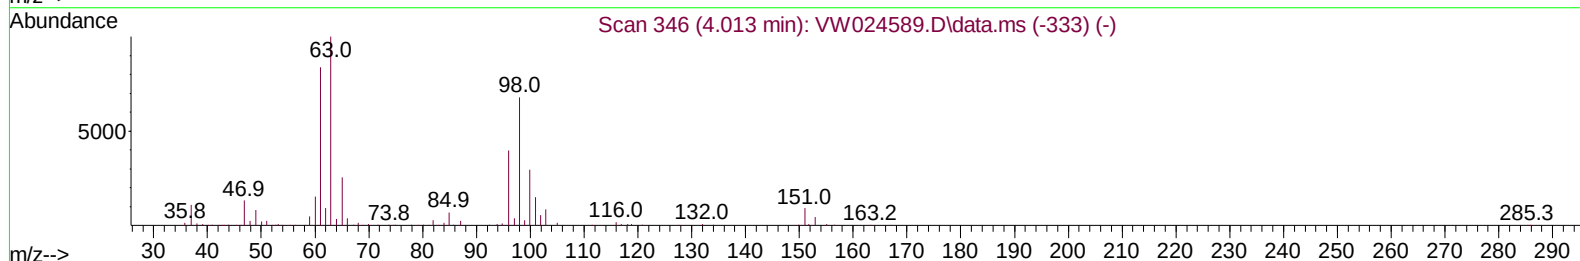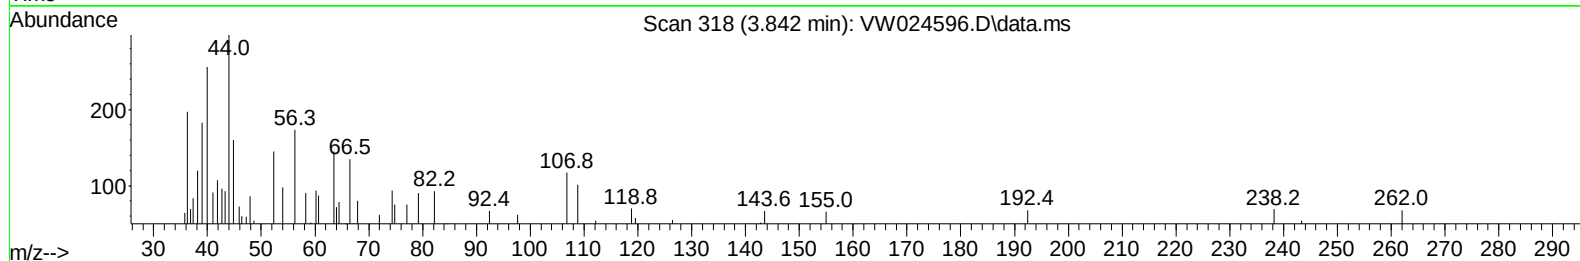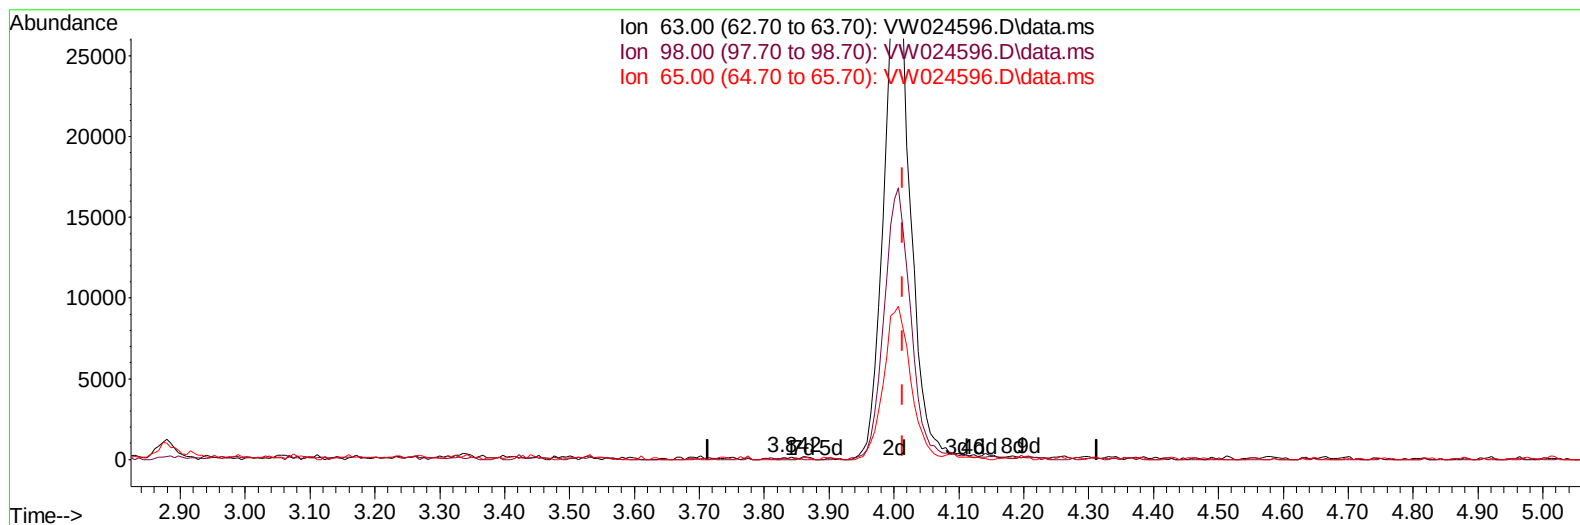

TIC: VW024596.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

3.842min (-0.171) 0.03 ug/L

response 150

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	73.20	71.33
65.00	23.40	26.67
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090922\
Data File : VW024596.D
Acq On : 09 Sep 2022 13:06
Operator : SY/VA
Sample : N4483-15
Misc : 5.05g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/12/2022
Supervised By :Mahesh Dadoda 09/12/2022

Quant Time: Sep 10 00:40:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090622SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Sep 10 00:38:15 2022
Response via : Initial Calibration

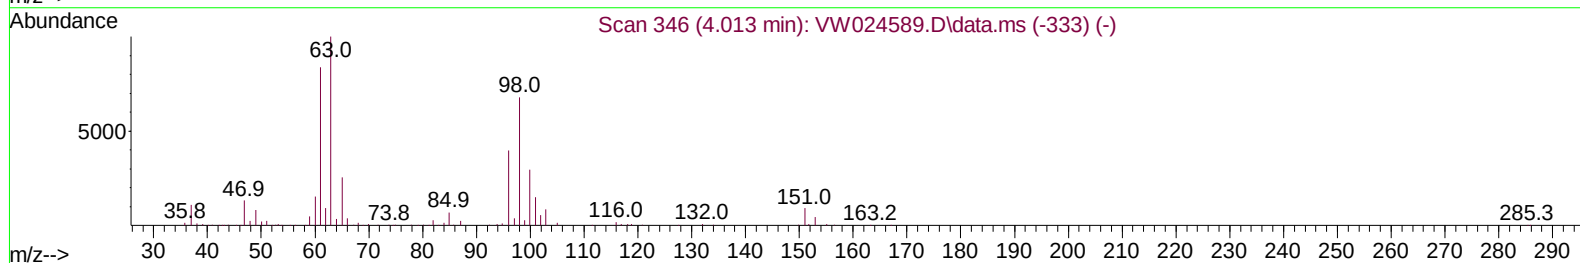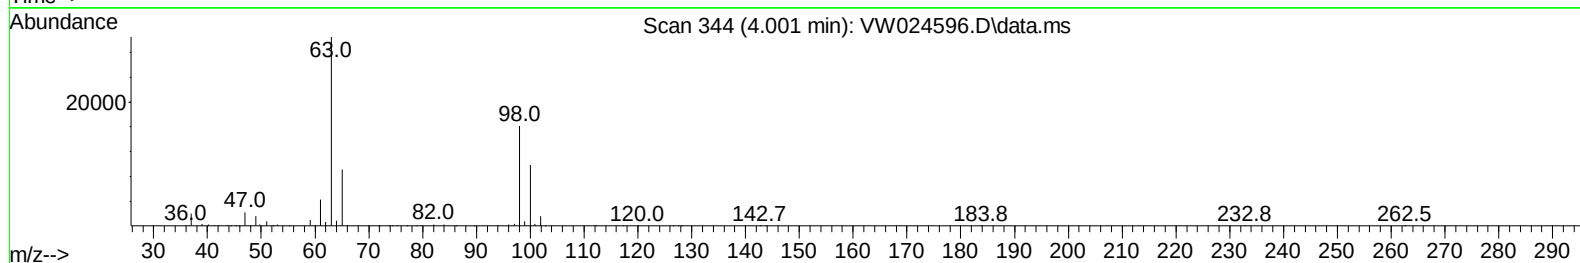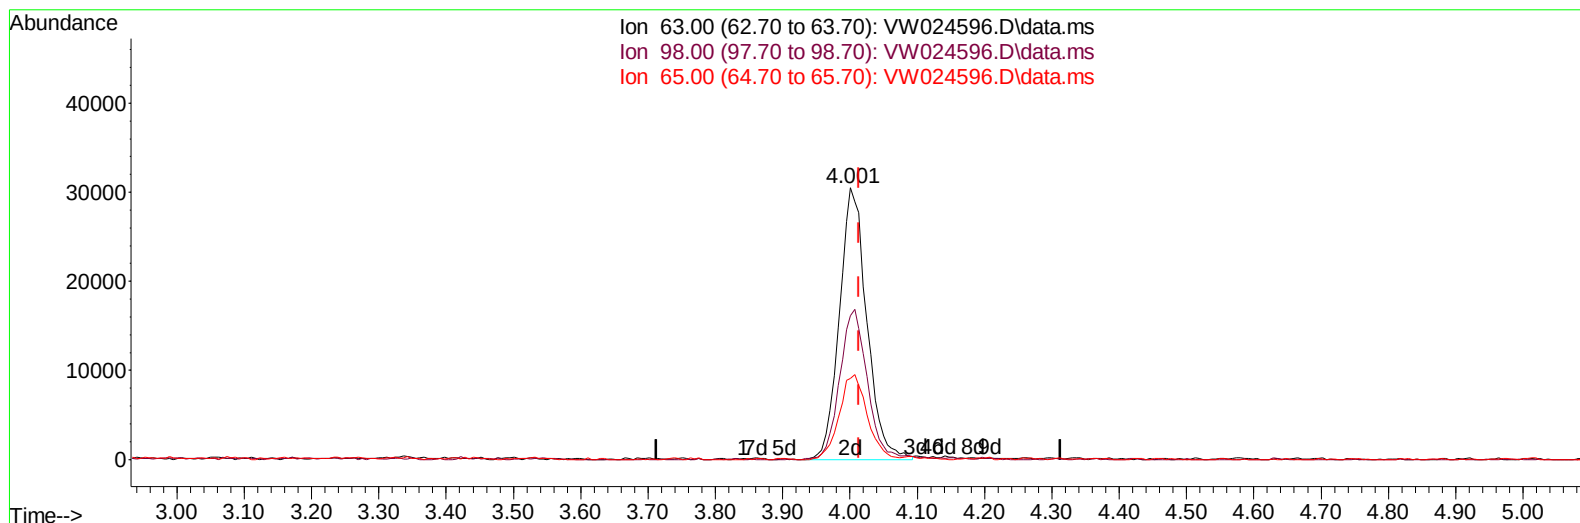

TIC: VW024596.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.001min (-0.012) 16.53 ug/L m

response 86209

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	73.20	0.12#
65.00	23.40	0.05#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090922\
 Data File : VW024596.D
 Acq On : 09 Sep 2022 13:06
 Operator : SY/VA
 Sample : N4483-15
 Misc : 5.05g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/12/2022
 Supervised By :Mahesh Dadoda 09/12/2022

Quant Time: Sep 10 00:40:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Sep 10 00:38:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.835	114	239354	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	246576	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	104065	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	154131	31.190	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	124.760%	
7) Chloroethane-d5	2.879	69	114807	31.245	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	124.960%	
11) 1,1-Dichloroethene-d2	4.001	63	86209m	16.535	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110	Recovery	=	66.120%	
21) 2-Butanone-d5	7.074	46	35360	44.356	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	88.720%	
24) Chloroform-d	7.640	84	141287	23.177	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	92.720%	
26) 1,2-Dichloroethane-d4	8.299	65	89305	25.983	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	103.920%	
32) Benzene-d6	8.268	84	292917	24.150	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	96.600%	
36) 1,2-Dichloropropane-d6	9.268	67	85529	23.917	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	95.680%	
41) Toluene-d8	10.323	98	267996	22.665	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	90.680%	
43) trans-1,3-Dichloroprop...	10.573	79	35051	21.872	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	87.480%	
47) 2-Hexanone-d5	10.926	63	29376	44.690	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	89.380%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	67511	19.697	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	78.800%	
66) 1,2-Dichlorobenzene-d4	13.853	152	87003	26.396	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	105.600%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090922\
Data File : VW024596.D
Acq On : 09 Sep 2022 13:06
Operator : SY/VA
Sample : N4483-15
Misc : 5.05g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/12/2022
Supervised By :Mahesh Dadoda 09/12/2022

Quant Time: Sep 10 00:40:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090622SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Sep 10 00:38:15 2022
Response via : Initial Calibration

