

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091024\
 Data File : VW030125.D
 Acq On : 10 Sep 2024 11:45
 Operator : SY/MD
 Sample : VW0910SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Sep 11 01:36:34 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Sep 11 01:35:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	229376	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	215900	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	98256	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	74737	21.895	ug/L	-0.01
Spiked Amount 25.000	Range 30 - 150		Recovery =	87.600%		
7) Chloroethane-d5	2.893	69	49542	20.450	ug/L	-0.01
Spiked Amount 25.000	Range 30 - 150		Recovery =	81.800%		
11) 1,1-Dichloroethene-d2	4.009	65	31445	21.562	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	86.240%		
21) 2-Butanone-d5	7.094	46	27712	40.727	ug/L	0.01
Spiked Amount 50.000	Range 20 - 135		Recovery =	81.460%		
24) Chloroform-d	7.648	84	151302	24.460	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	97.840%		
26) 1,2-Dichloroethane-d4	8.307	65	77174	24.571	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	98.280%		
32) Benzene-d6	8.270	84	299378	23.492	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	93.960%		
36) 1,2-Dichloropropane-d6	9.270	67	91712	24.563	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	98.240%		
41) Toluene-d8	10.325	98	270490	23.319	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	93.280%		
43) trans-1,3-Dichloroprop...	10.575	79	34423	22.413	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	89.640%		
47) 2-Hexanone-d5	10.922	63	22148	38.758	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	77.520%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	61551	22.390	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	89.560%		
66) 1,2-Dichlorobenzene-d4	13.848	152	81218	22.853	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	91.400%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	2563	0.475	ug/L	# 76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091024\
Data File : VW030125.D
Acq On : 10 Sep 2024 11:45
Operator : SY/MD
Sample : VW0910SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Sep 11 01:36:34 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Sep 11 01:35:57 2024
Response via : Initial Calibration

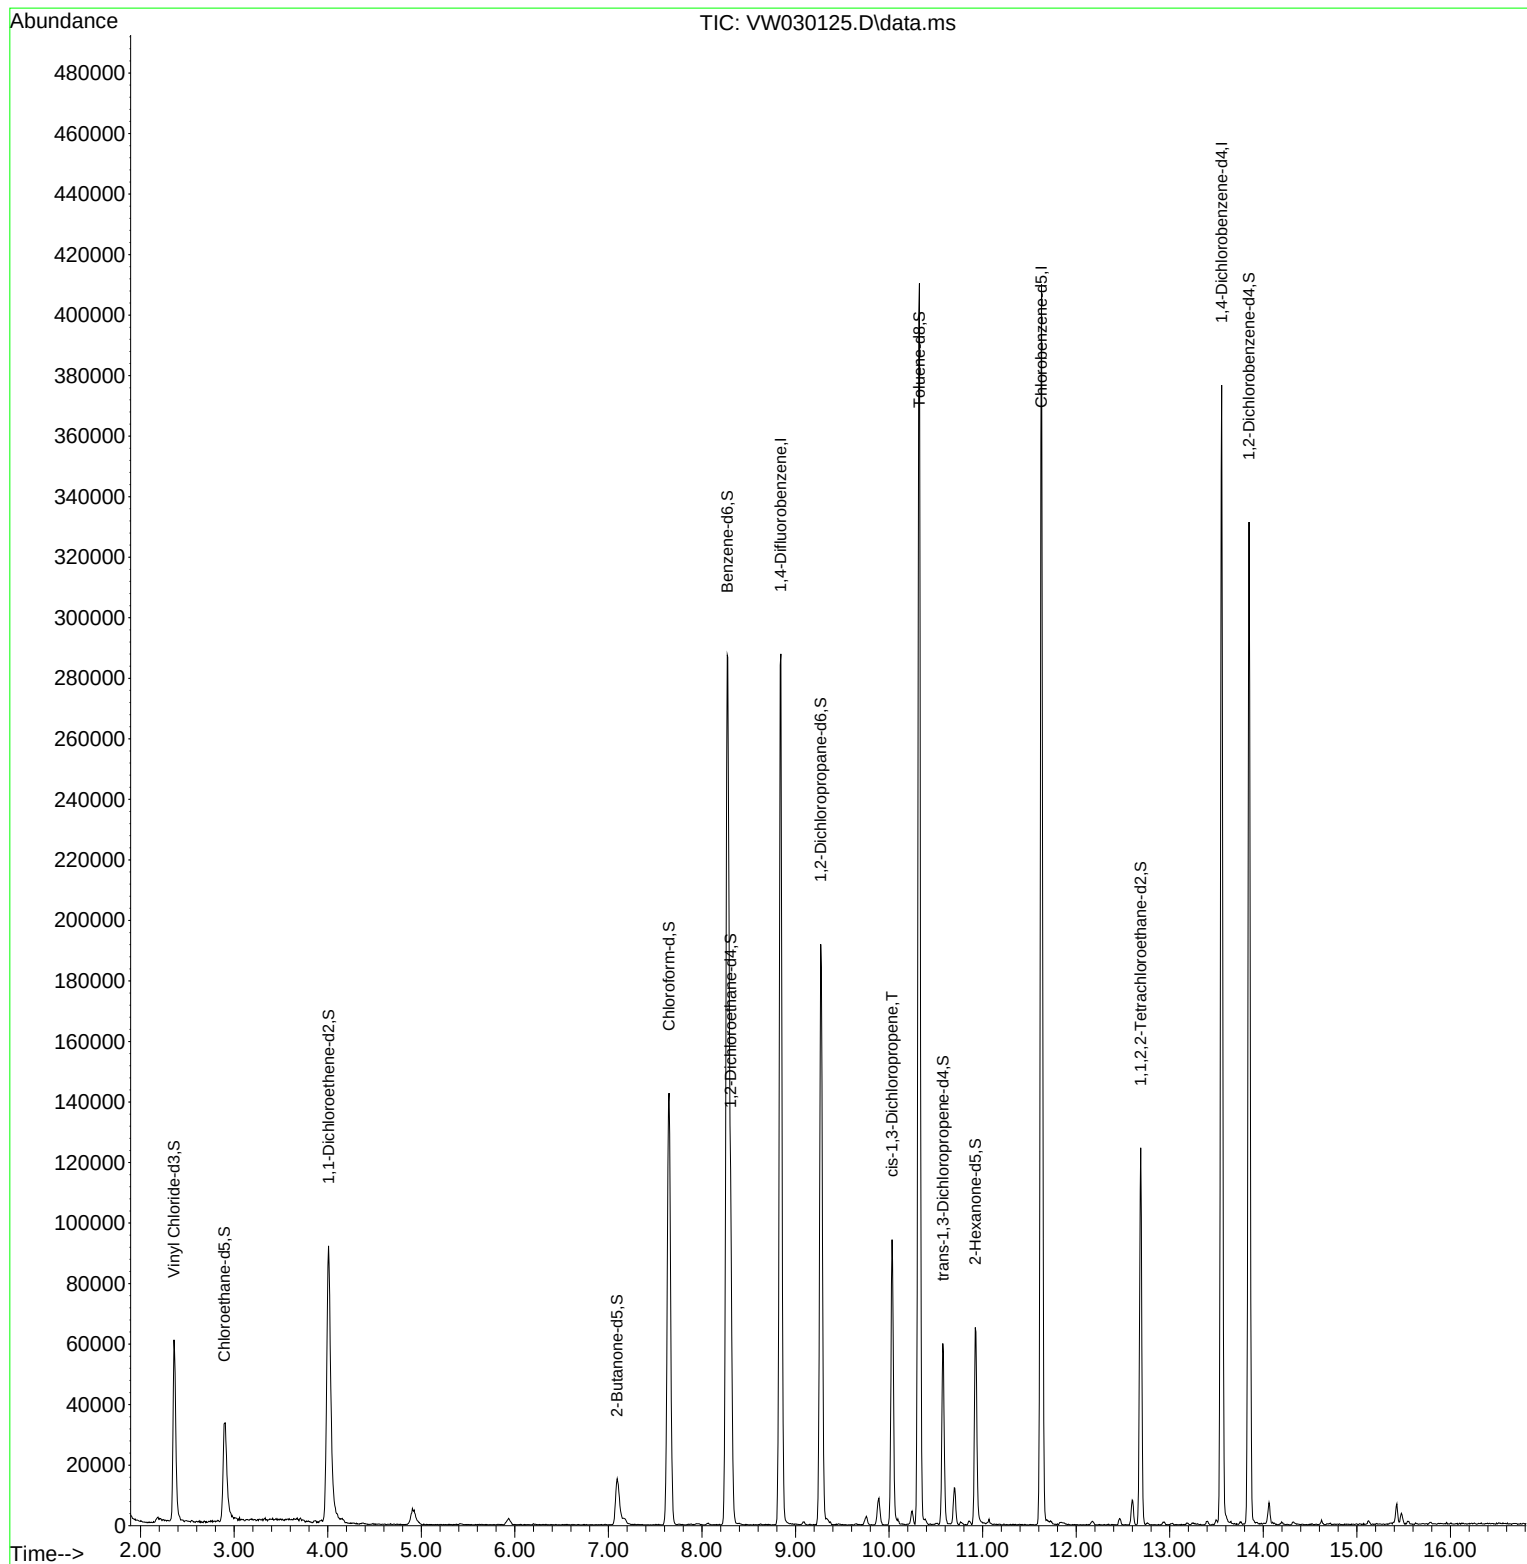

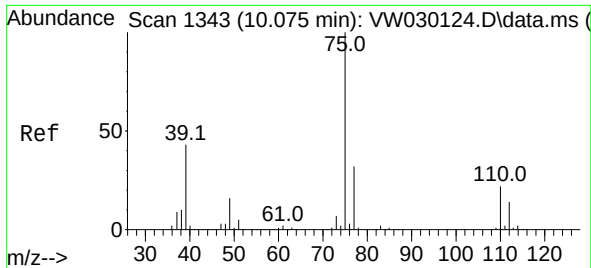

#39
cis-1,3-Dichloropropene
Concen: 0.475 ug/L
RT: 10.032 min Scan# 14
Delta R.T. -0.043 min
Lab File: VW030125.D
Acq: 10 Sep 2024 11:45

Instrument :
MSVOA_W
ClientSampleId :

Tgt Ion: 75 Resp: 2563
Ion Ratio Lower Upper
75 100
77 46.0 22.8 42.4#

